

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
 Data File : BG017039.D
 Acq On : 11 May 2015 00:46
 Operator : TP/IZ
 Sample : G2109-05
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-29

Quant Time: May 11 05:38:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 11 05:17:53 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	99670	20.00	ng	0.00
21) Naphthalene-d8	10.58	136	481459	20.00	ng	0.00
38) Acenaphthene-d10	14.43	164	324235	20.00	ng	0.00
63) Phenanthrene-d10	17.17	188	667290	20.00	ng	0.00
75) Chrysene-d12	21.35	240	634451	20.00	ng	0.00
86) Perylene-d12	23.65	264	636661	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	293381	51.25	ng	0.00
7) Phenol-d6	6.98	99	275167	33.65	ng	0.00
23) Nitrobenzene-d5	8.95	82	633028	64.23	ng	0.00
41) 2,4,6-Tribromophenol	15.92	330	365343	112.24	ng	0.00
44) 2-Fluorobiphenyl	13.05	172	1260999	58.69	ng	0.00
78) Terphenyl-d14	19.80	244	1556674	57.52	ng	0.00
Target Compounds						
32) Benzoic acid	10.03	122	669	Below Cal	Qvalue #	21

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG017039.D
Acq On : 11 May 2015 00:46
Operator : TP/IZ
Sample : G2109-05
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-29

Quant Time: May 11 05:38:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 05:17:53 2015
Response via : Initial Calibration

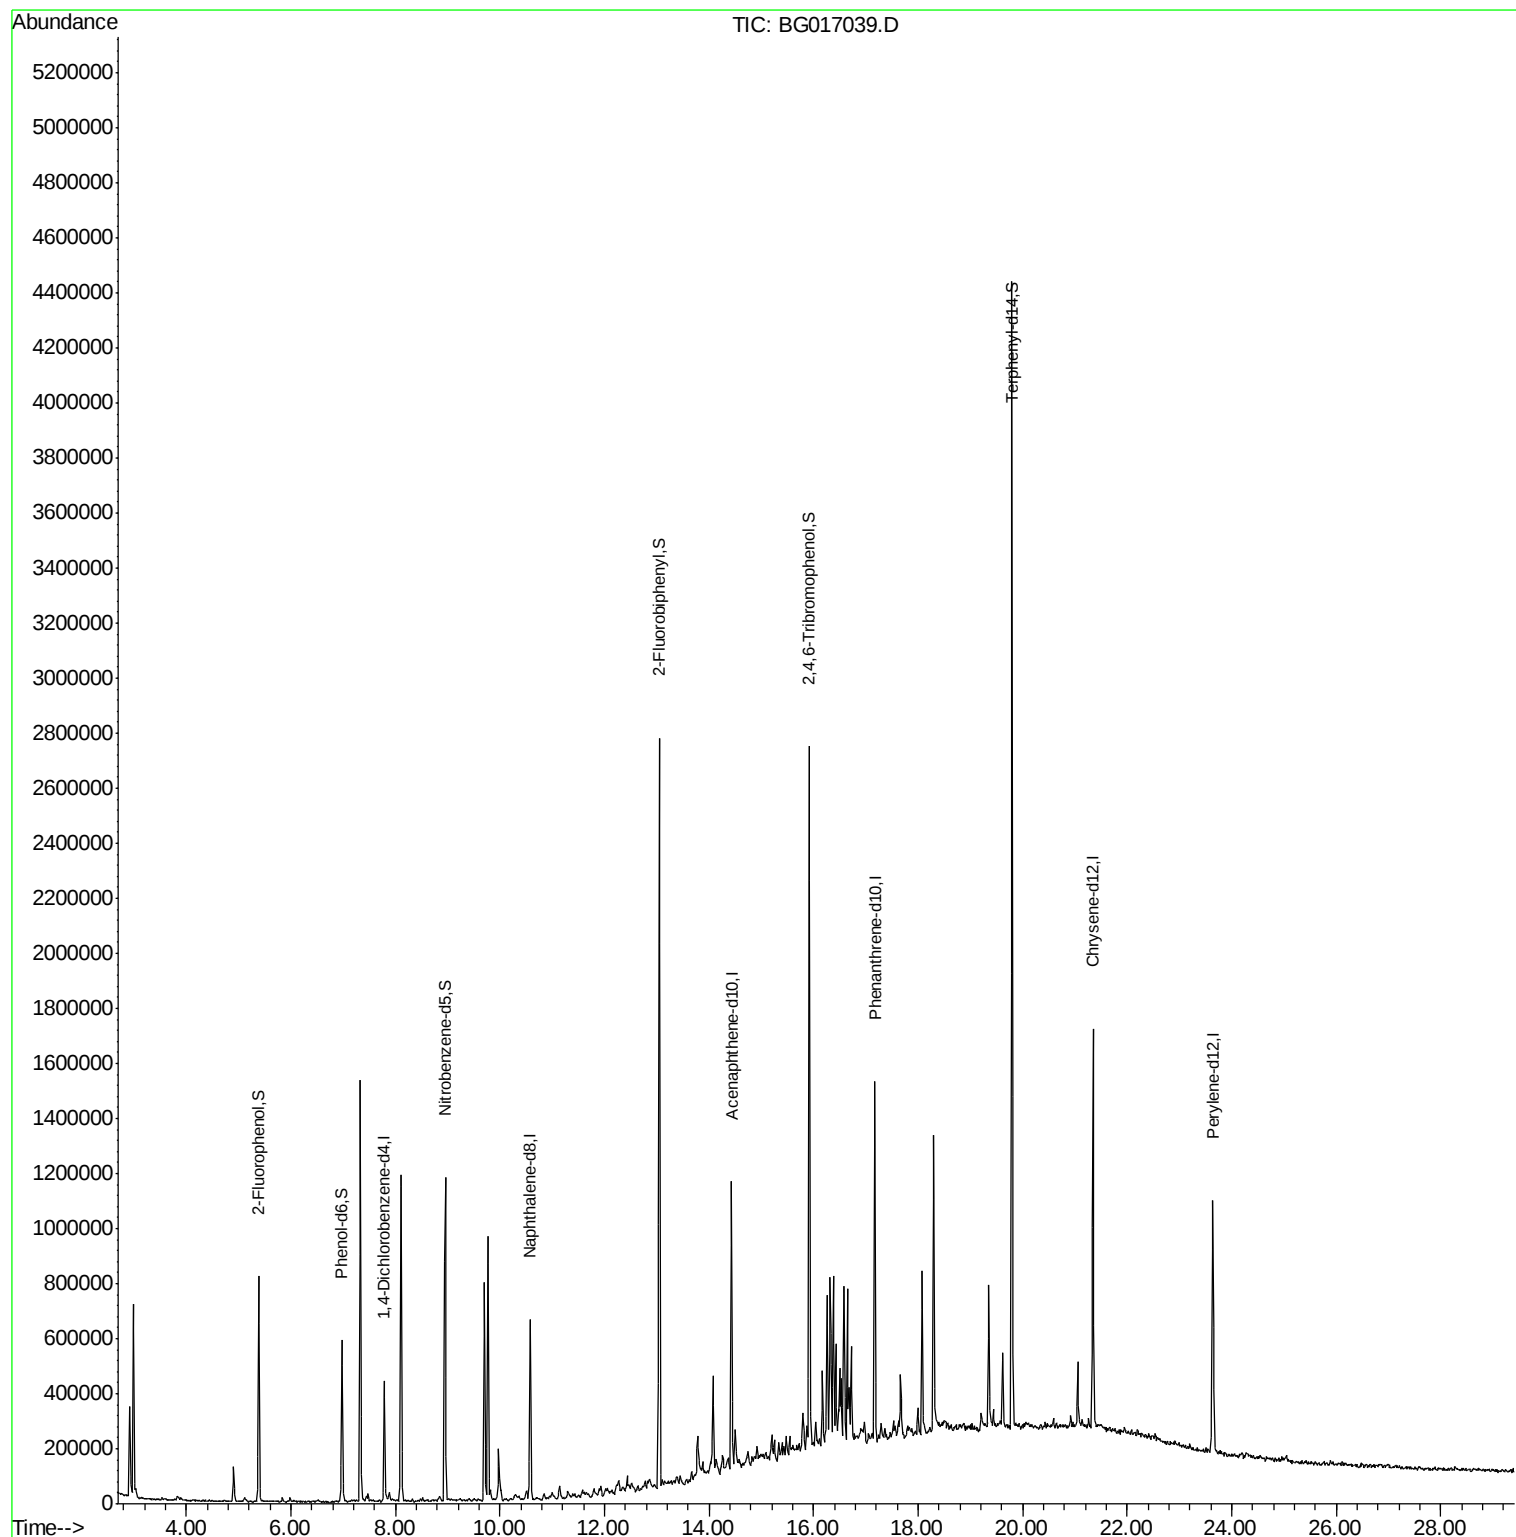



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 868

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46

Instrument :

BNA_G

ClientSampleId :

W-29


Tgt Ion:152 Resp: 99670

Ion Ratio Lower Upper

152 100

150 154.8 121.0 181.4



115 64.2 50.5 75.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

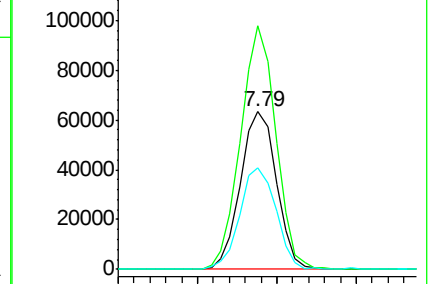

#5

2-Fluorophenol

Concen: 51.25 ng

RT: 5.39 min Scan# 459

Delta R.T. 0.01 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46


Tgt Ion:112 Resp: 293381

Ion Ratio Lower Upper

112 100

64 67.3 51.4 77.2



63 39.2 28.1 42.1



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

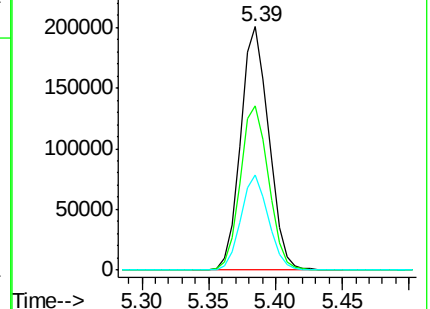



#7

Phenol-d6

Concen: 33.65 ng

RT: 6.98 min Scan# 730

Delta R.T. 0.01 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46

Instrument :

BNA_G

ClientSampleId :

W-29


Tgt Ion: 99 Resp: 275167

Ion Ratio Lower Upper




99 100

42 25.2 22.1 33.1

71 43.1 33.4 50.0



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

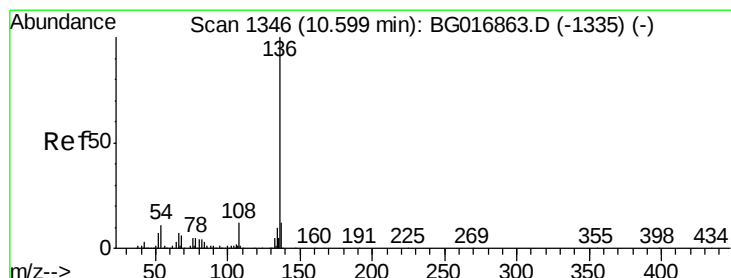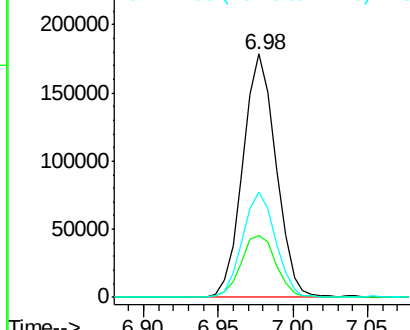

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1343

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46

Tgt Ion: 136 Resp: 481459


Ion Ratio Lower Upper

136 100



137 10.7 9.8 14.8

54 9.8 8.7 13.1

68 6.4 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



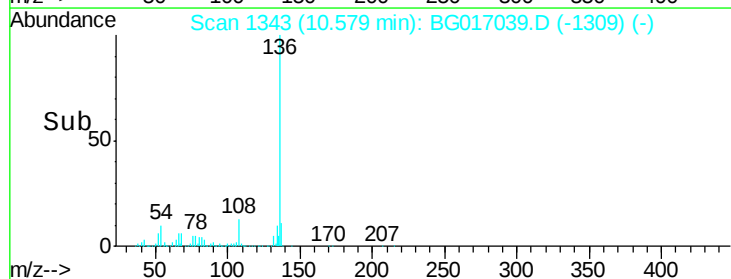
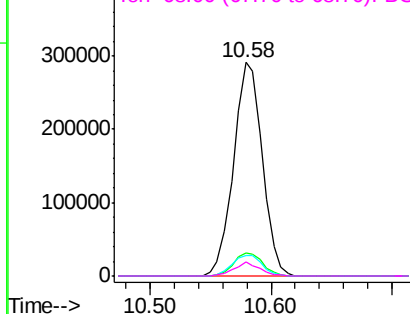




#23
 Nitrobenzene-d5
 Concen: 64.23 ng
 RT: 8.95 min Scan# 1065
 Delta R.T. -0.01 min
 Lab File: BG017039.D
 Acq: 11 May 2015 00:46




Instrument :
 BNA_G
 ClientSampleId :
 W-29


Tgt Ion: 82 Resp: 633028
 Ion Ratio Lower Upper
 82 100
 128 41.6 33.2 49.8
 54 60.6 48.6 72.8

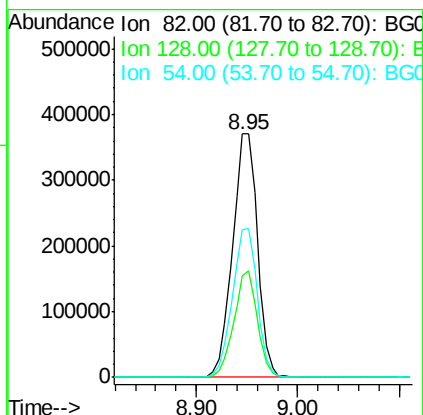

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. -0.00 min
 Lab File: BG017039.D
 Acq: 11 May 2015 00:46

Tgt Ion: 164 Resp: 324235
 Ion Ratio Lower Upper
 164 100
 162 97.0 74.0 111.0
 160 44.1 34.7 52.1



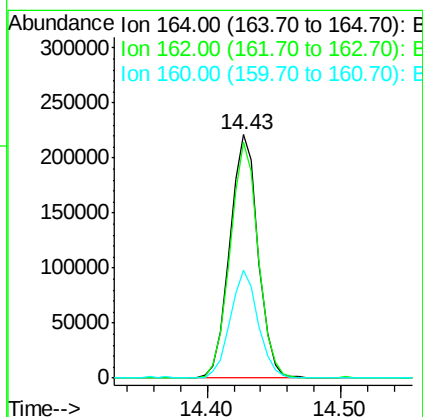



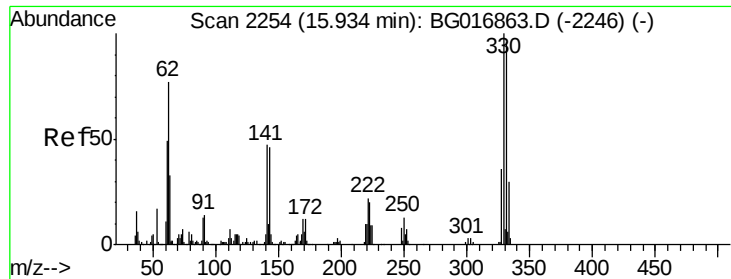

#41
 2,4,6-Tribromophenol
 Concen: 112.24 ng
 RT: 15.92 min Scan# 2252
 Delta R.T. -0.00 min
 Lab File: BG017039.D
 Acq: 11 May 2015 00:46




Instrument :
 BNA_G
 ClientSampleId :
 W-29


Tgt Ion:330 Resp: 365343
 Ion Ratio Lower Upper
 330 100
 332 97.8 0.0 0.0#
 141 49.9 0.0 0.0#

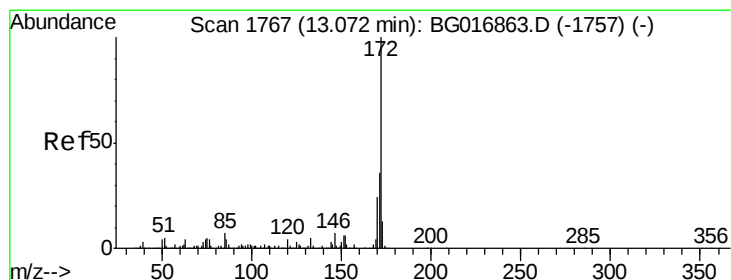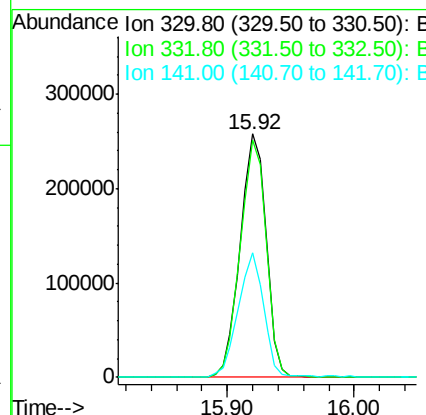

#44
 2-Fluorobiphenyl
 Concen: 58.69 ng
 RT: 13.05 min Scan# 1764
 Delta R.T. -0.00 min
 Lab File: BG017039.D
 Acq: 11 May 2015 00:46

Tgt Ion:172 Resp: 1260999
 Ion Ratio Lower Upper
 172 100
 171 37.8 29.0 43.4
 170 25.0 19.0 28.4

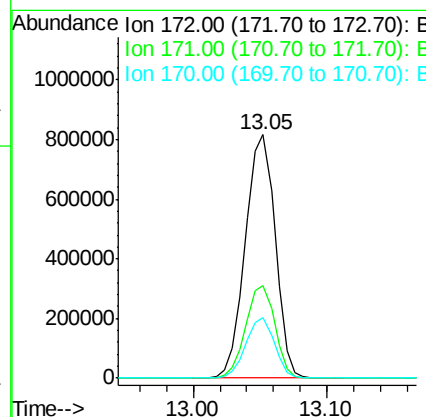



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2465

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46

Instrument :

BNA_G

ClientSampleId :

W-29


Tgt Ion:188 Resp: 667290

Ion Ratio Lower Upper

188 100

94 9.1 8.2 12.4


80 10.7 8.8 13.2





Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

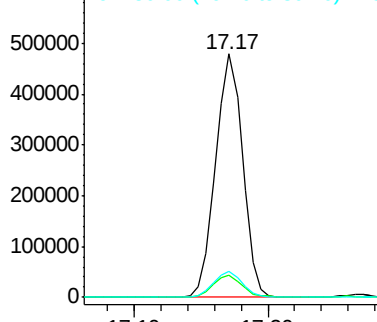

Time-->



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.35 min Scan# 3176

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46


Tgt Ion:240 Resp: 634451

Ion Ratio Lower Upper

240 100

120 10.1 9.1 13.7


236 25.9 20.2 30.4




Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

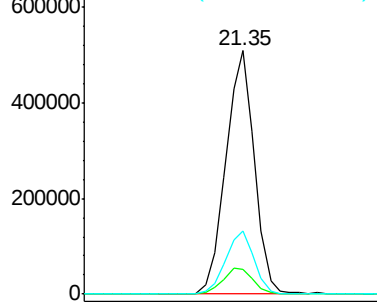

Time-->



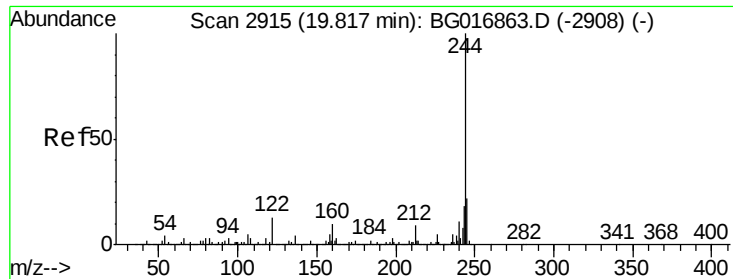

#78

Terphenyl-d14

Concen: 57.52 ng

RT: 19.80 min Scan# 2912

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46

Instrument :

BNA_G

ClientSampleId :

W-29


Tgt Ion:244 Resp: 1556674

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6




122 13.3 10.4 15.6

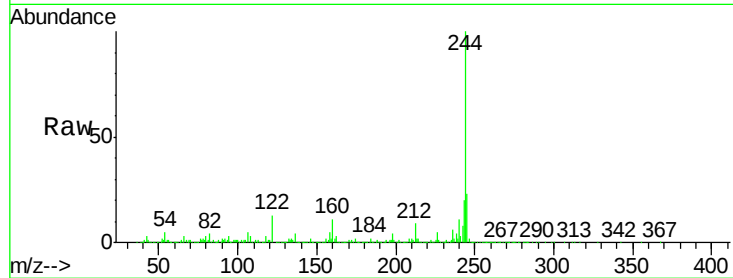

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

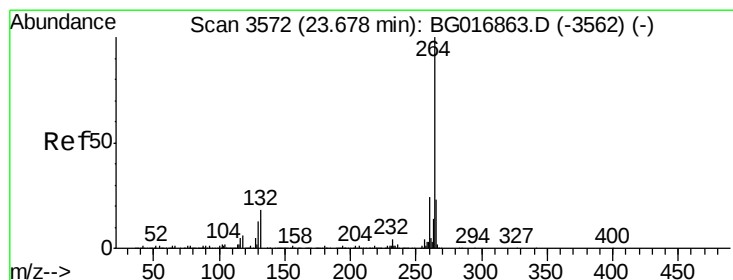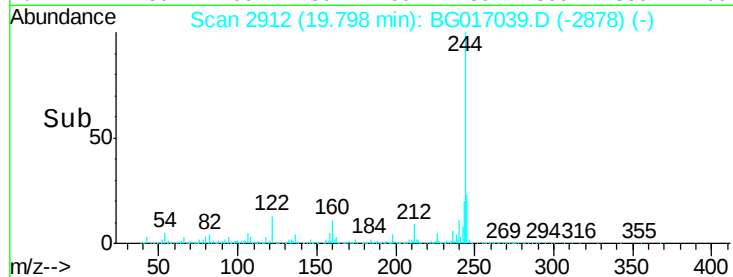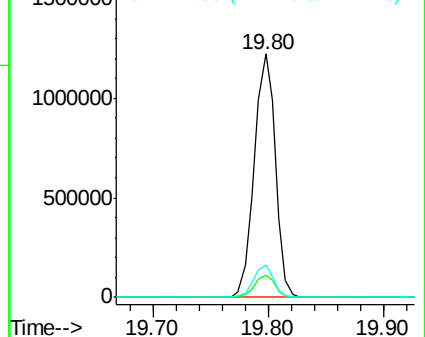

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.65 min Scan# 3567

Delta R.T. -0.00 min

Lab File: BG017039.D

Acq: 11 May 2015 00:46


Tgt Ion:264 Resp: 636661

Ion Ratio Lower Upper

264 100

260 22.9 19.5 29.3

265 22.0 18.5 27.7

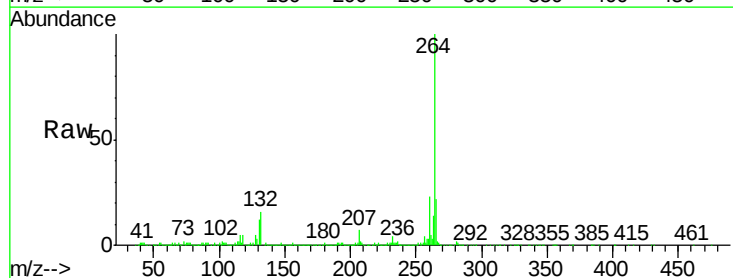

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

