
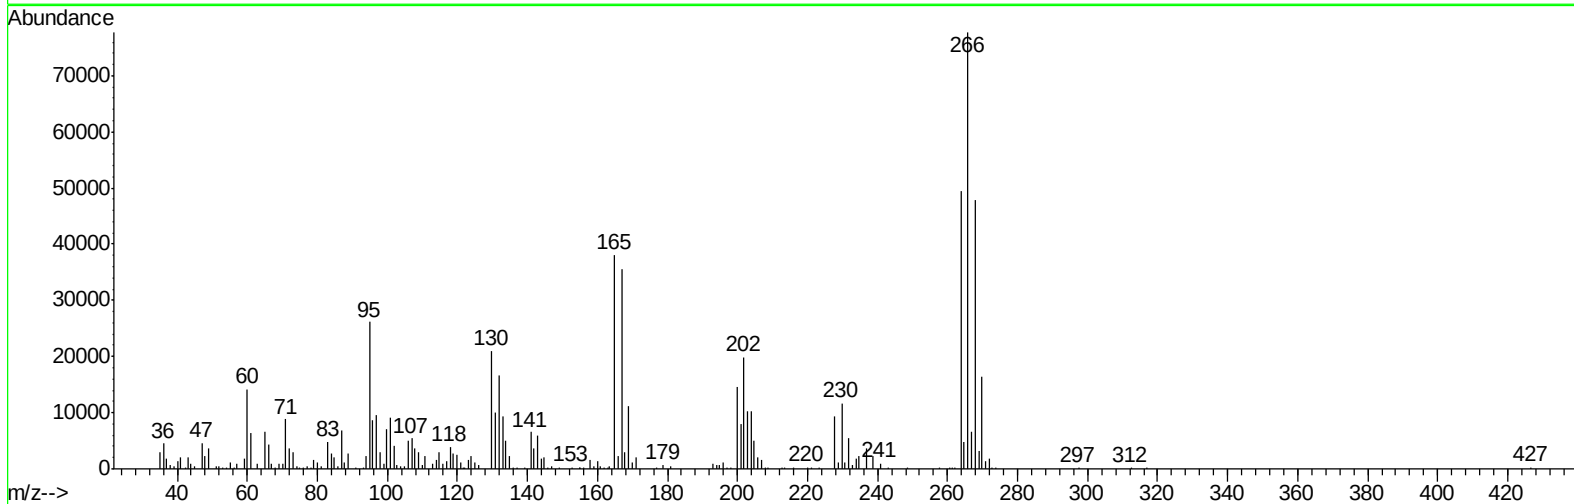


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016950.D
Acq On : 8 May 2015 11:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:03:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

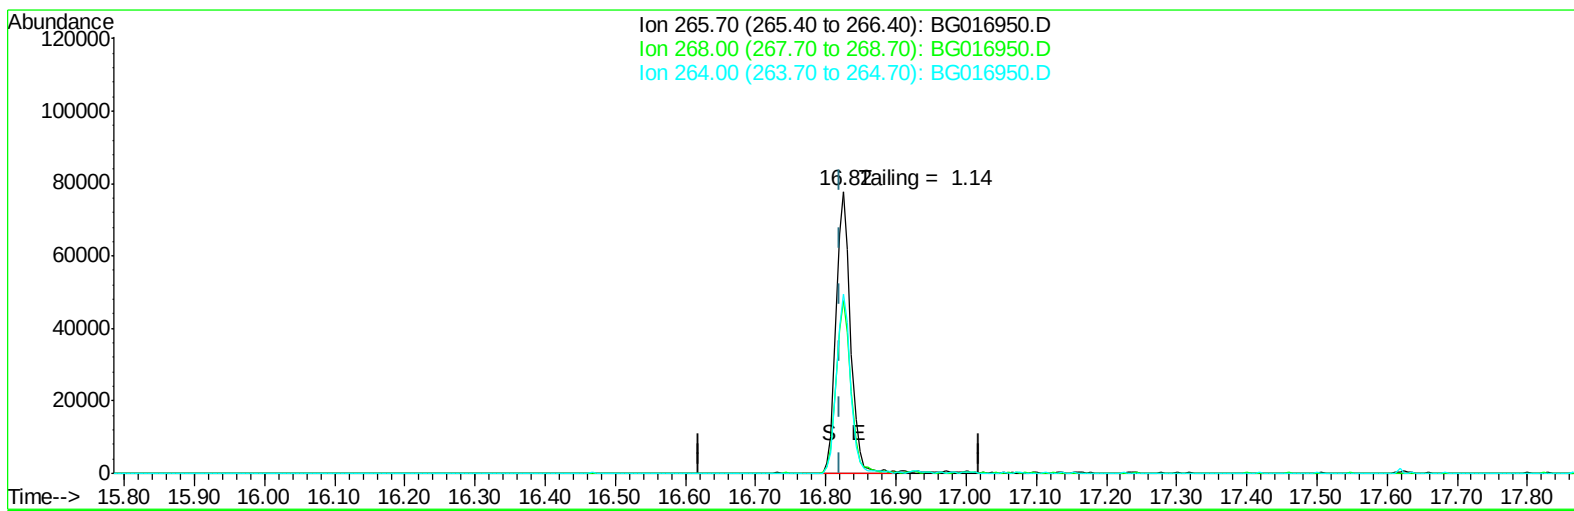

TIC: BG016950.D

(69) Pentachlorophenol (C)



16.825min (+0.005) 103808.71ng

response 109859

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	61.59
264.00	64.20	63.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016950.D
Acq On : 8 May 2015 11:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:03:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

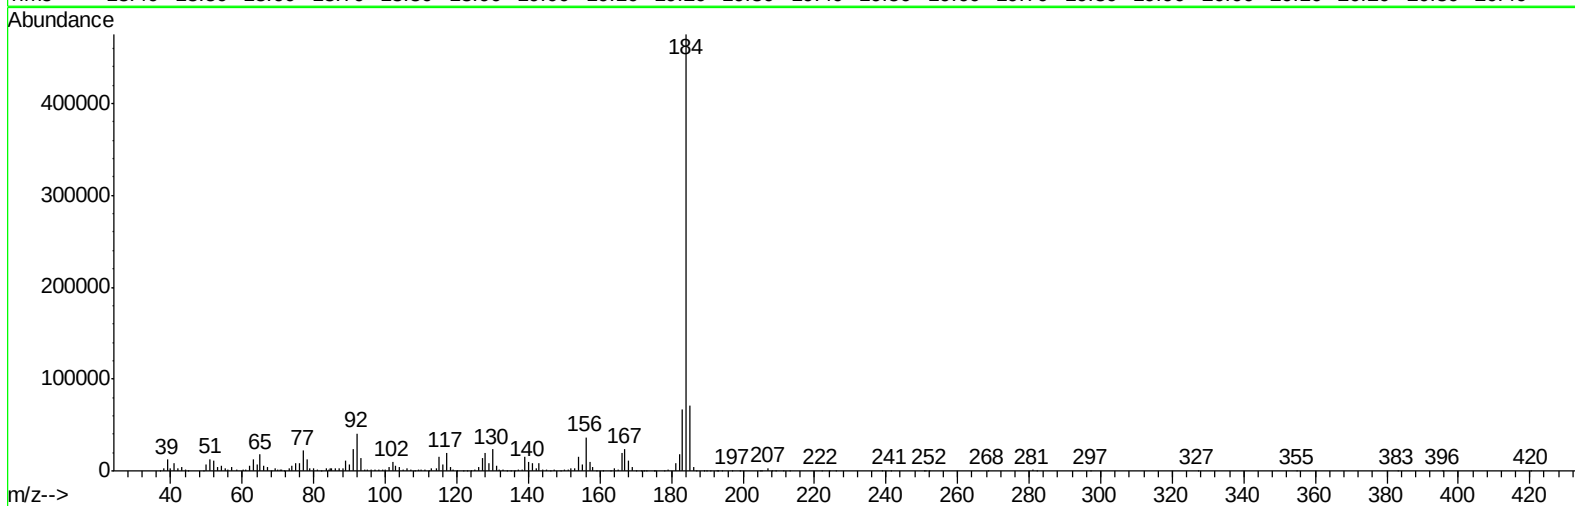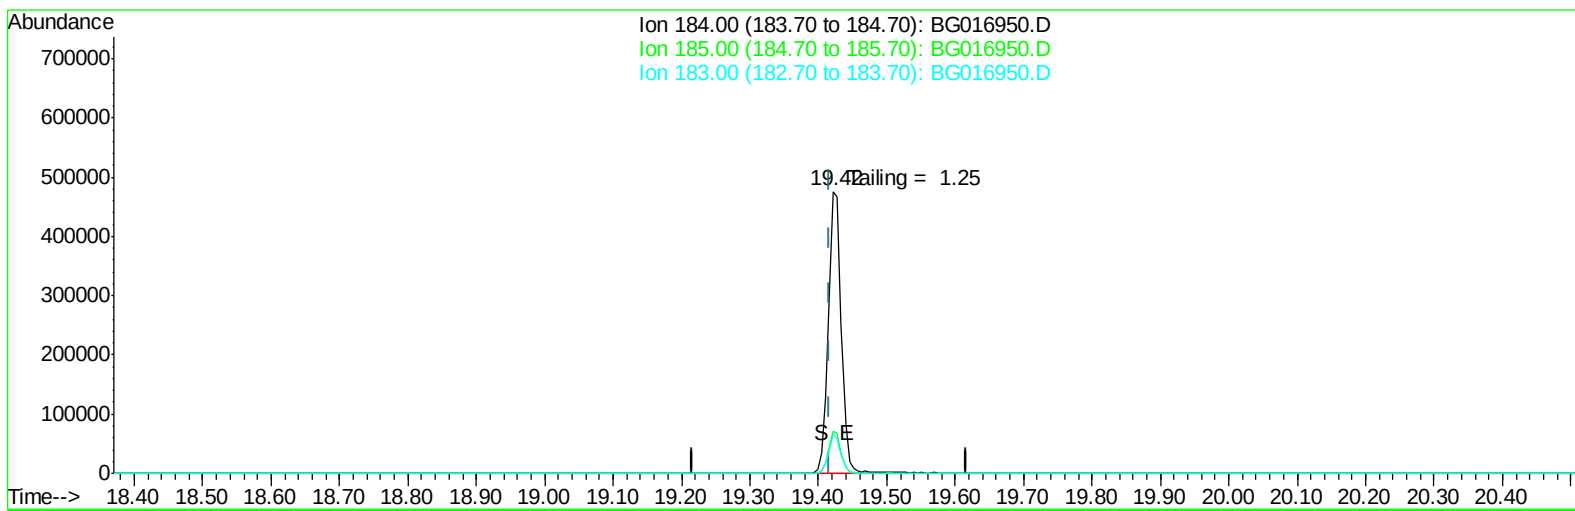

TIC: BG016950.D

(76) Benzidine

19.422min (+0.005) 28194.07ng

response 635151

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.89
183.00	13.20	14.17
0.00	0.00	0.00