
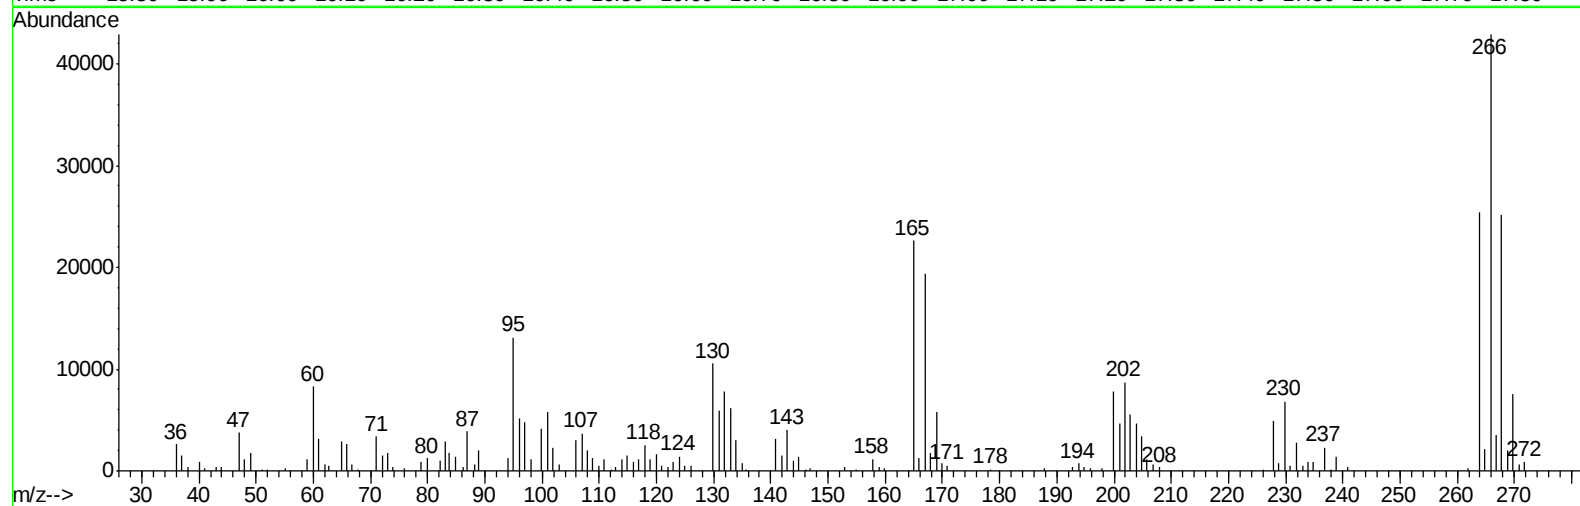


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016969.D
Acq On : 9 May 2015 00:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:05:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

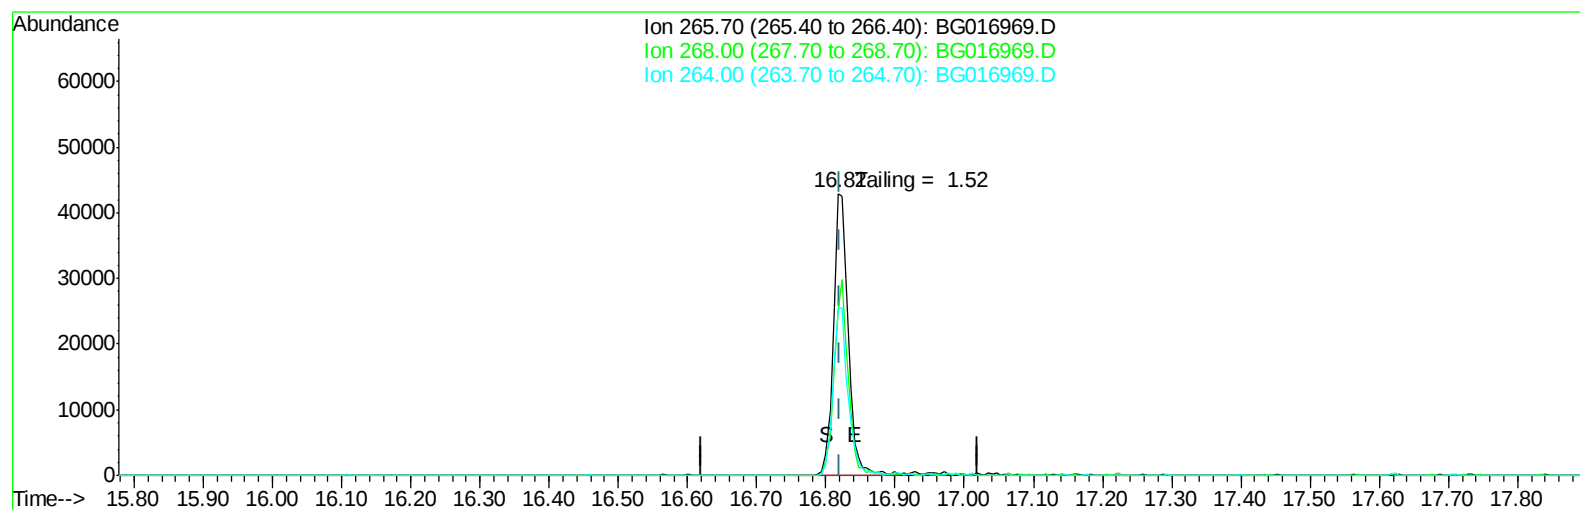

TIC: BG016969.D

(69) Pentachlorophenol (C)



16.818min (-0.002) 142796.40ng

response 63784

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	58.57
264.00	64.20	59.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016969.D
Acq On : 9 May 2015 00:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:05:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

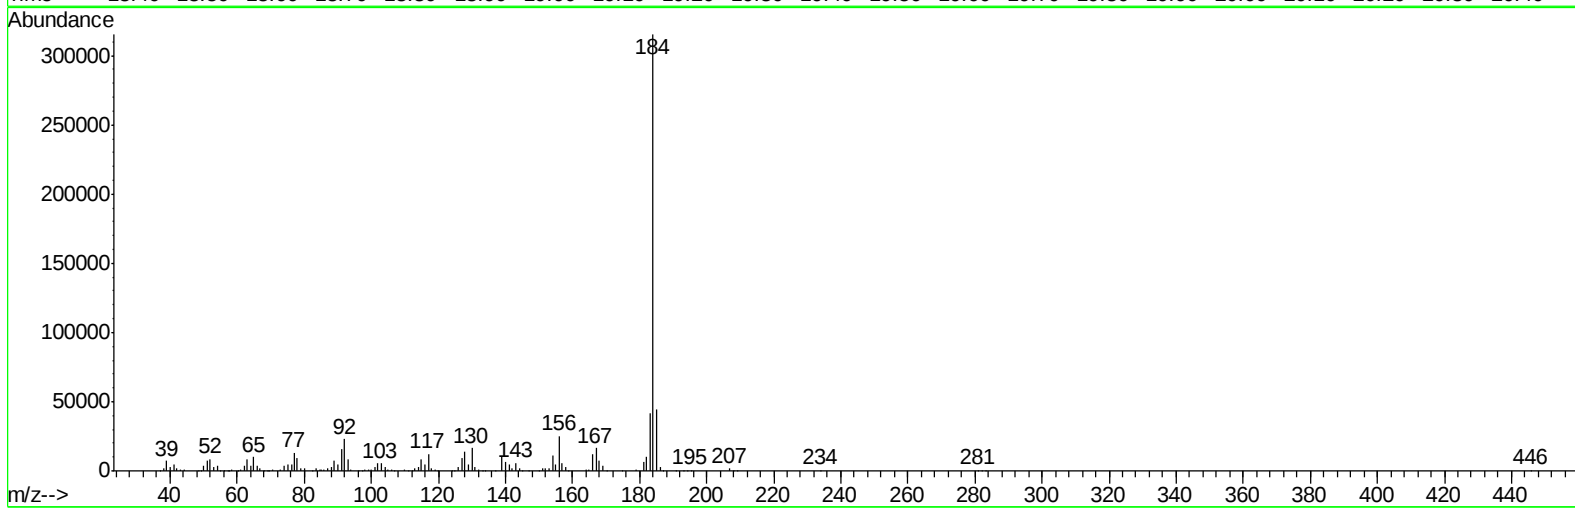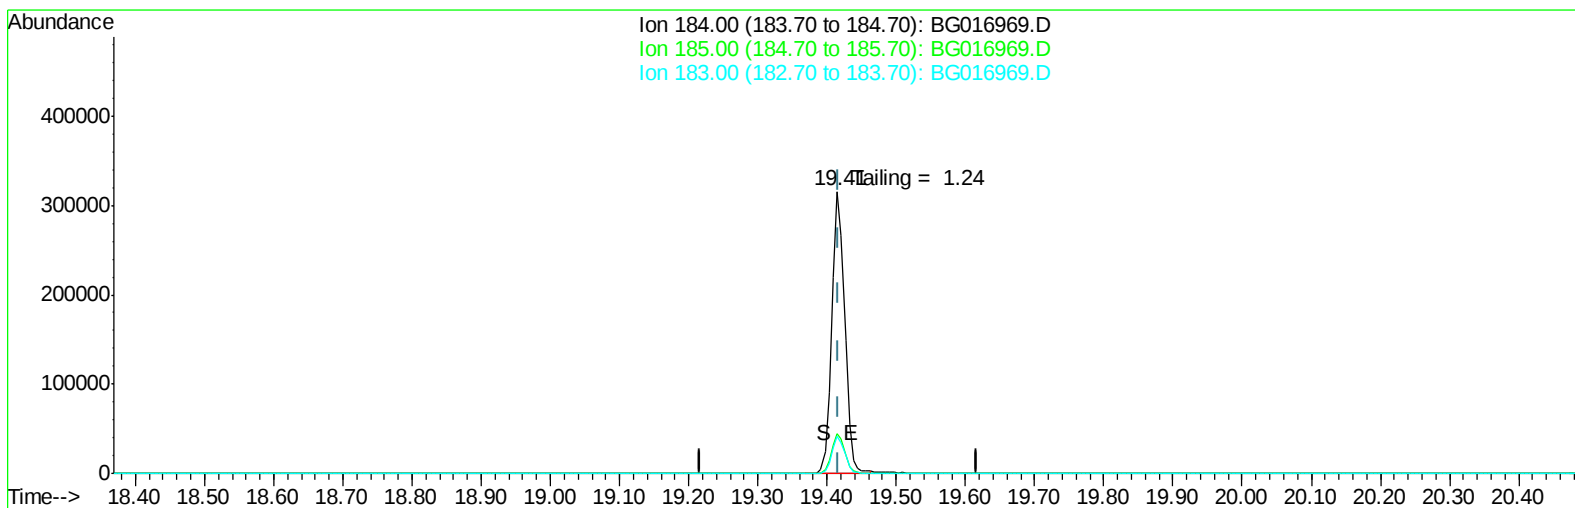

TIC: BG016969.D

(76) Benzidine

19.415min (-0.002) 129672.33ng

response 409766

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.99
183.00	13.20	13.25
0.00	0.00	0.00