

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
 Data File : BG016974.D
 Acq On : 9 May 2015 3:36
 Operator : TP/IZ
 Sample : G2059-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A3-SEEP

Quant Time: May 09 05:07:18 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 09 03:28:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	52761	20.00	ng	0.00
21) Naphthalene-d8	10.58	136	242475	20.00	ng	0.00
38) Acenaphthene-d10	14.43	164	163208	20.00	ng	0.00
63) Phenanthrene-d10	17.17	188	396227	20.00	ng	0.00
75) Chrysene-d12	21.35	240	393897	20.00	ng	0.00
86) Perylene-d12	23.64	264	376061	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	222952	73.58	ng	0.00
7) Phenol-d6	6.96	99	224169	51.78	ng	0.00
23) Nitrobenzene-d5	8.95	82	454771	91.62	ng	0.00
41) 2,4,6-Tribromophenol	15.92	330	303262	185.09	ng	0.00
44) 2-Fluorobiphenyl	13.05	172	992529	91.77	ng	0.00
78) Terphenyl-d14	19.80	244	1585454	94.36	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016974.D
Acq On : 9 May 2015 3:36
Operator : TP/IZ
Sample : G2059-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A3-SEEP

Quant Time: May 09 05:07:18 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 09 03:28:47 2015
Response via : Initial Calibration

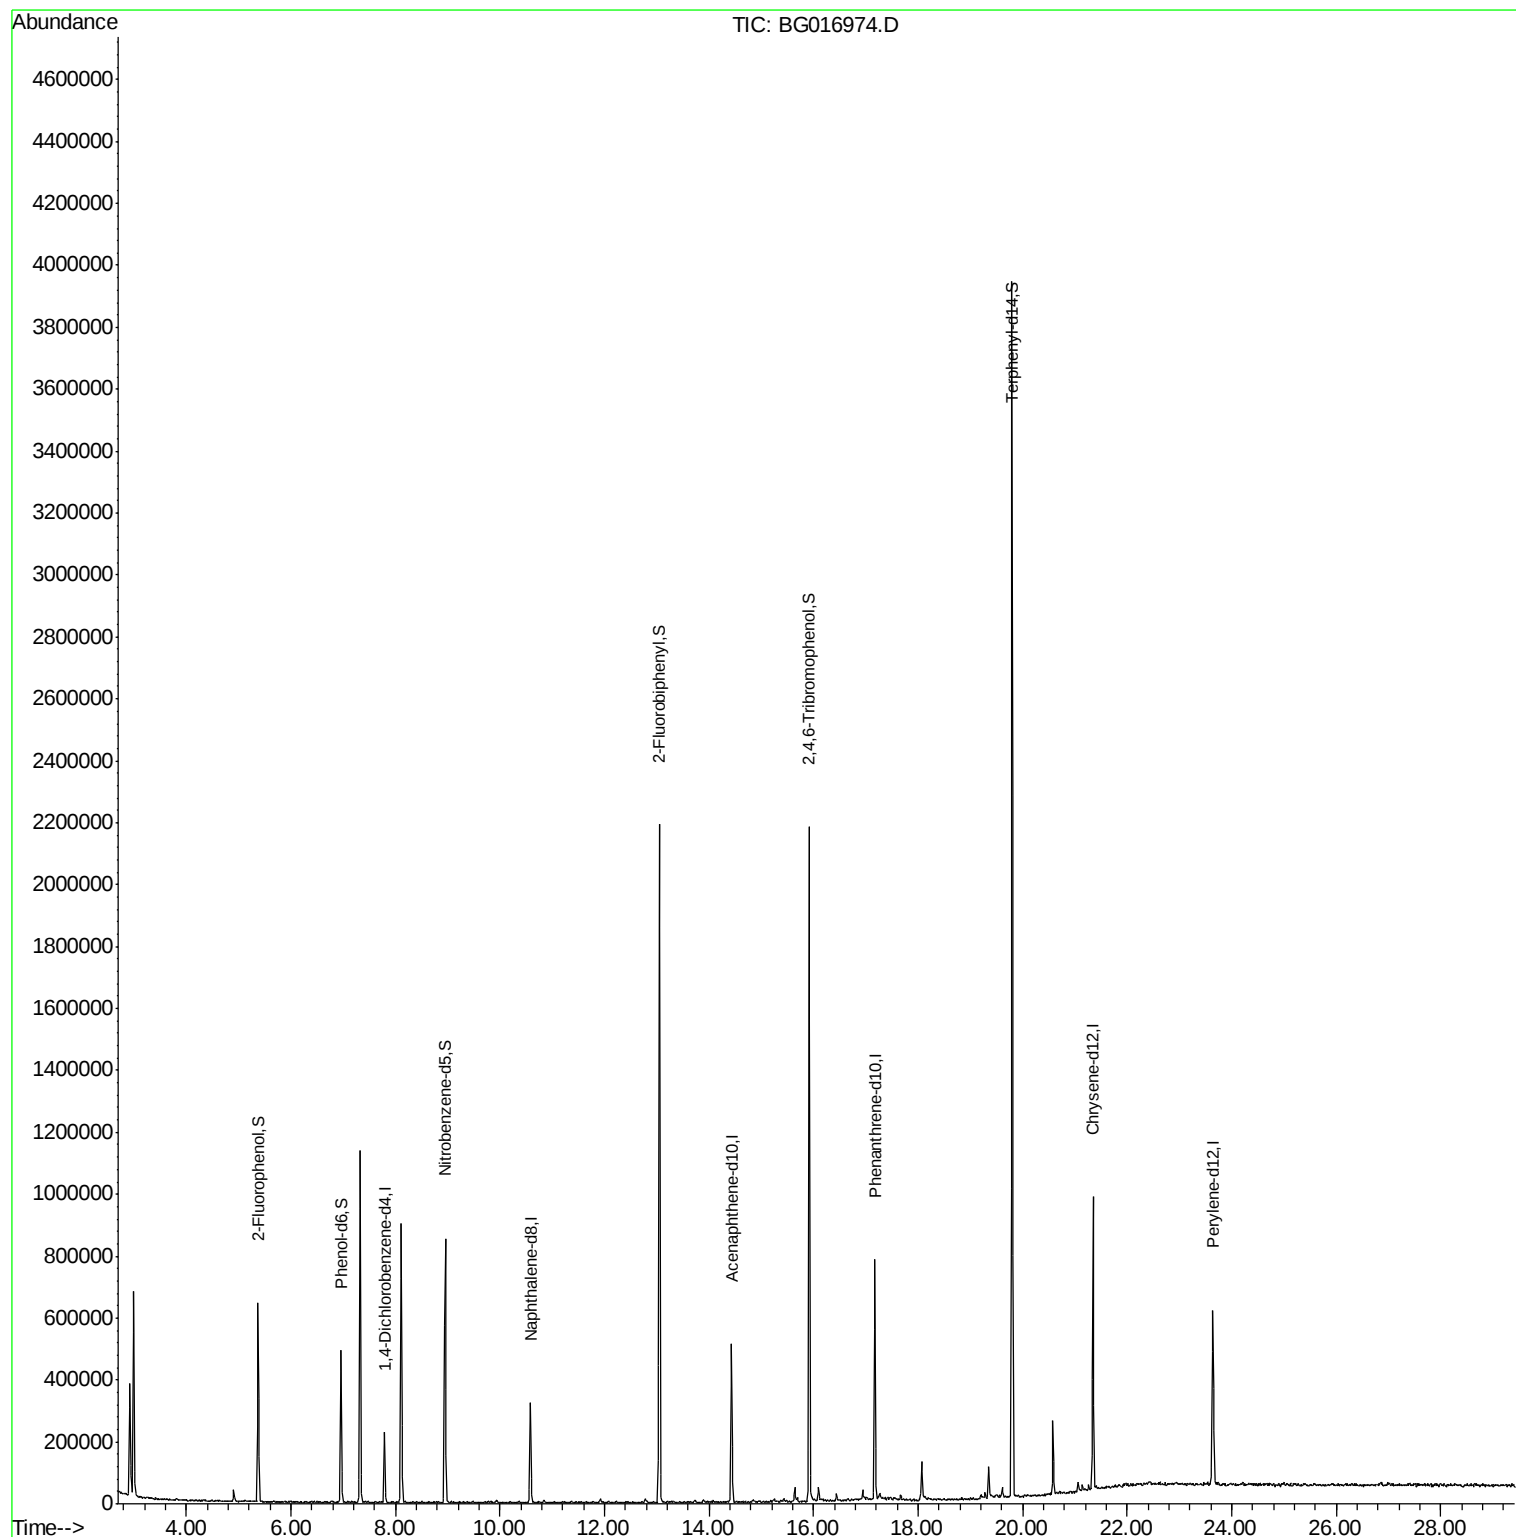



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 869

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36

Instrument :

BNA_G

ClientSampleId :

A3-SEEP


Tgt Ion:152 Resp: 52761

Ion Ratio Lower Upper

152 100

150 150.0 121.0 181.4



115 61.0 50.5 75.7

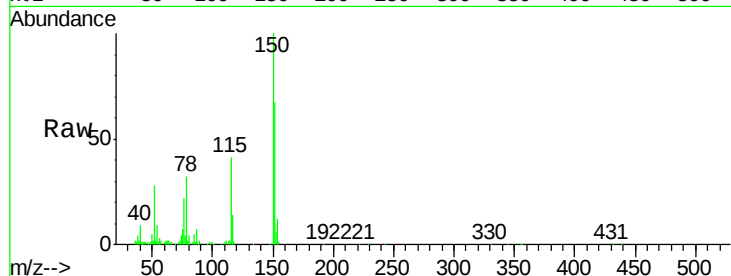

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

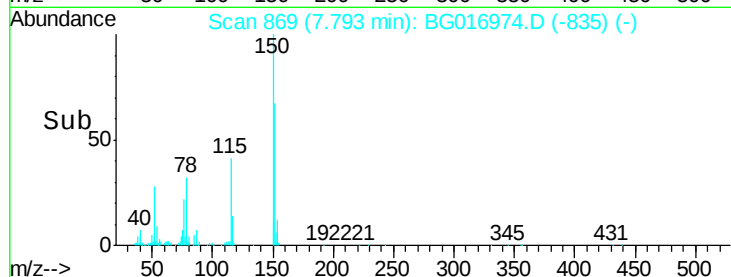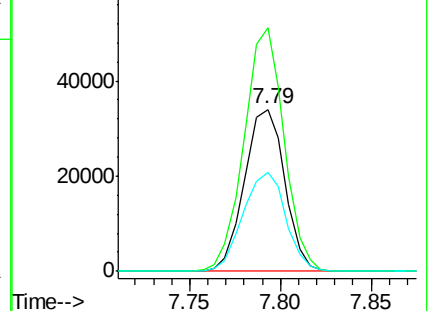

#5

2-Fluorophenol

Concen: 73.58 ng

RT: 5.37 min Scan# 457

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36


Tgt Ion:112 Resp: 222952

Ion Ratio Lower Upper

112 100

64 70.3 51.4 77.2



63 38.4 28.1 42.1




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

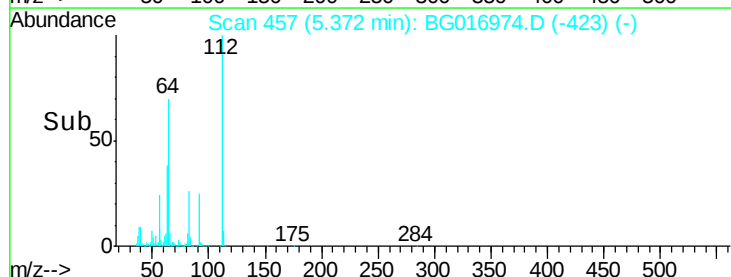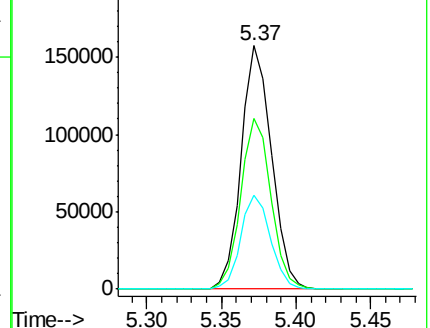

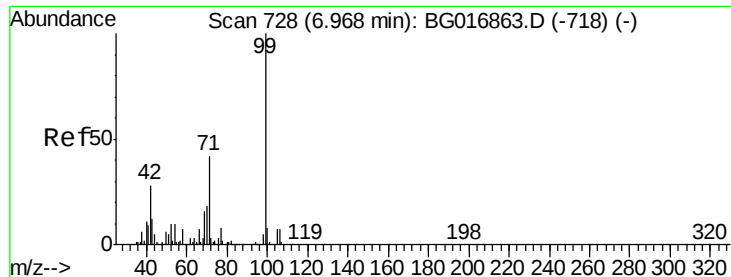

#7

Phenol-d6

Concen: 51.78 ng

RT: 6.96 min Scan# 727

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36

Instrument :

BNA_G

ClientSampleId :

A3-SEEP


Tgt Ion: 99 Resp: 224169

Ion Ratio Lower Upper




99 100

42 25.9 22.1 33.1

71 41.9 33.4 50.0



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

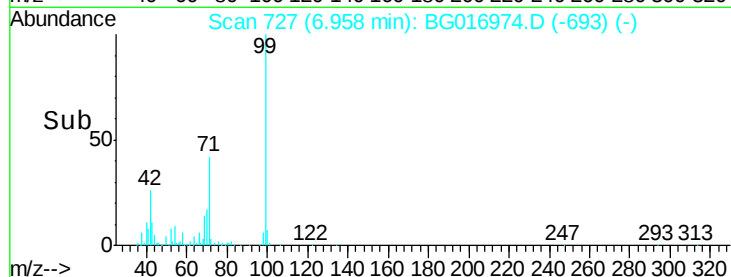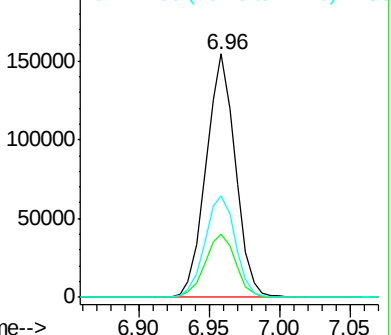

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1344

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36

Tgt Ion: 136 Resp: 242475


Ion Ratio Lower Upper

136 100



137 11.2 9.8 14.8

54 9.8 8.7 13.1

68 5.3 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



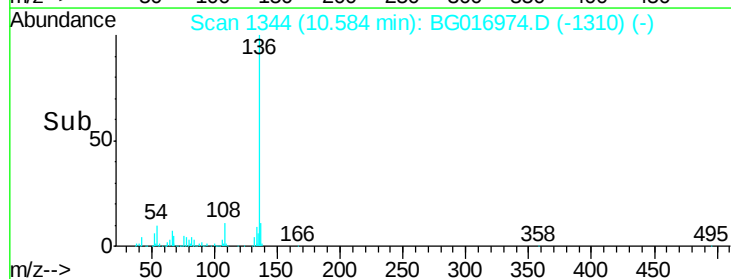
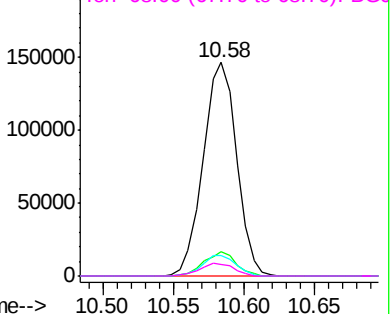




#23
 Nitrobenzene-d5
 Concen: 91.62 ng
 RT: 8.95 min Scan# 1066
 Delta R.T. -0.00 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36




Instrument :
 BNA_G
 ClientSampleId :
 A3-SEEP


Tgt Ion: 82 Resp: 454771
 Ion Ratio Lower Upper
 82 100
 128 40.3 33.2 49.8
 54 55.8 48.6 72.8

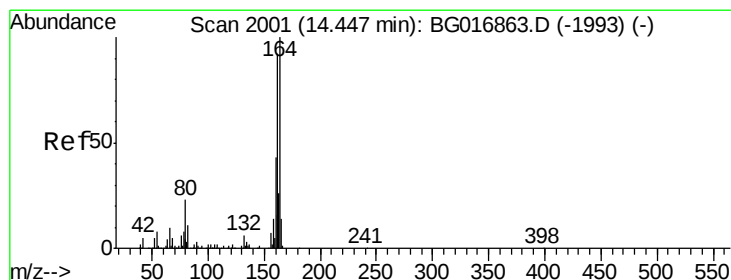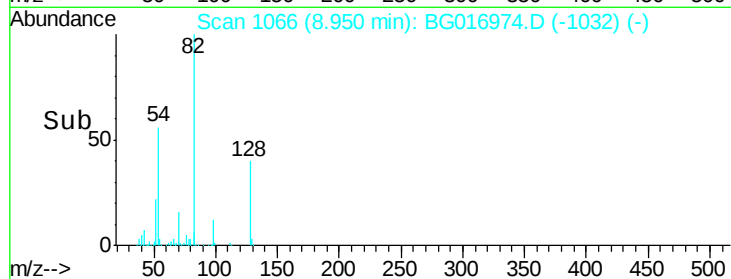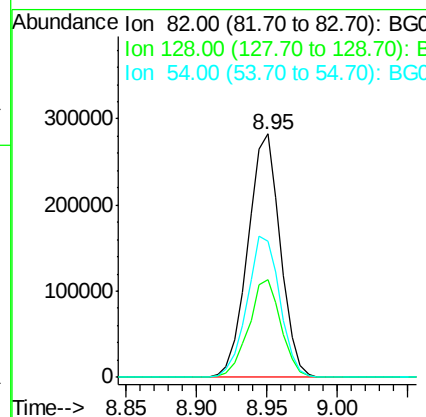

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. -0.01 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36

Tgt Ion: 164 Resp: 163208
 Ion Ratio Lower Upper
 164 100
 162 91.9 74.0 111.0
 160 42.2 34.7 52.1


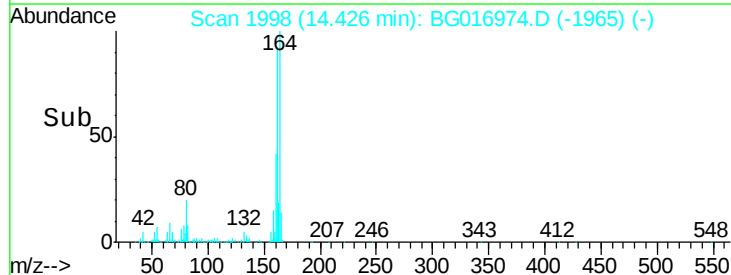
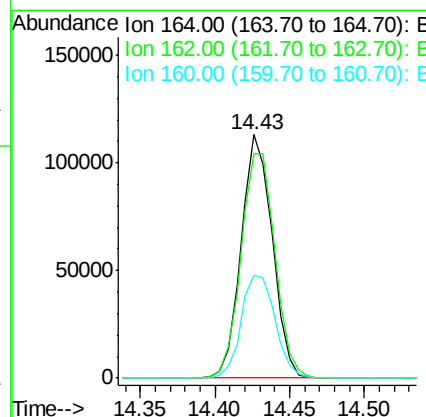



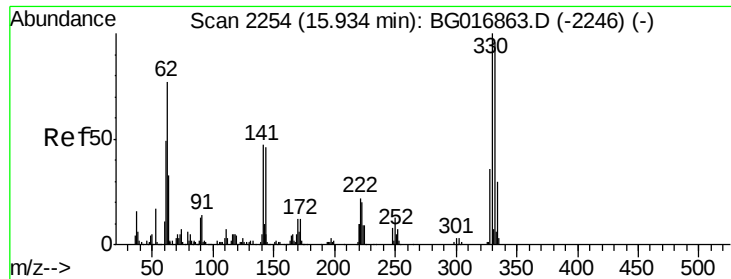

#41
 2,4,6-Tribromophenol
 Concen: 185.09 ng
 RT: 15.92 min Scan# 2252
 Delta R.T. -0.00 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36




Instrument :
 BNA_G
 ClientSampleId :
 A3-SEEP


Tgt Ion:330 Resp: 303262
 Ion Ratio Lower Upper
 330 100
 332 96.8 0.0 0.0#
 141 50.0 0.0 0.0#

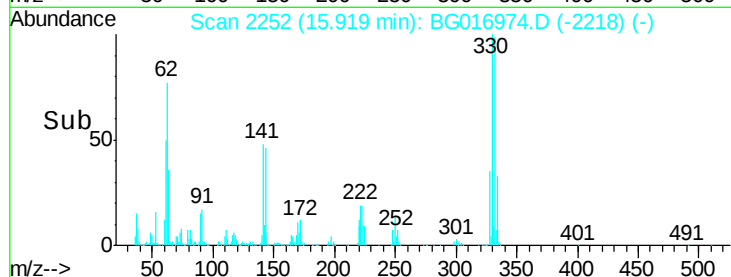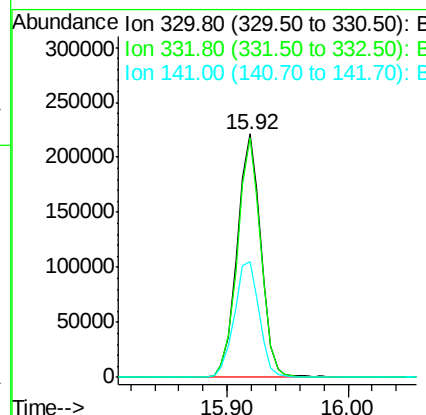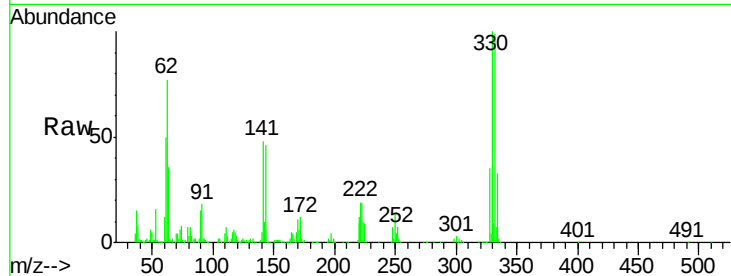

#44
 2-Fluorobiphenyl
 Concen: 91.77 ng
 RT: 13.05 min Scan# 1764
 Delta R.T. -0.00 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36

Tgt Ion:172 Resp: 992529
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.0 43.4
 170 24.3 19.0 28.4

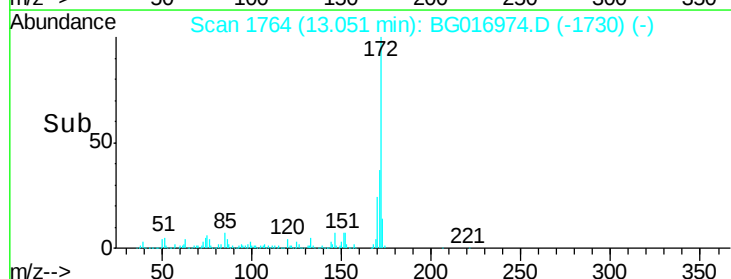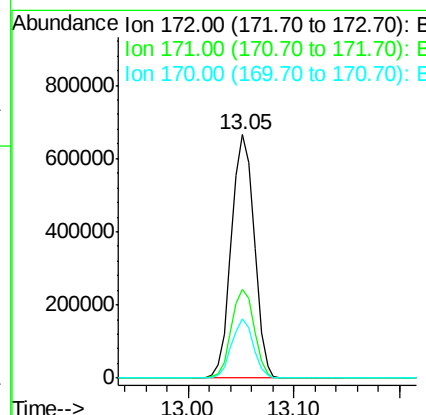

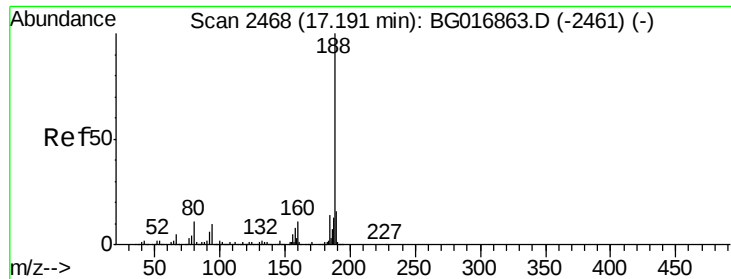

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2465

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36

Instrument :

BNA_G

ClientSampleId :

A3-SEEP


Tgt Ion:188 Resp: 396227

Ion Ratio Lower Upper

188 100

94 8.9 8.2 12.4




80 11.6 8.8 13.2

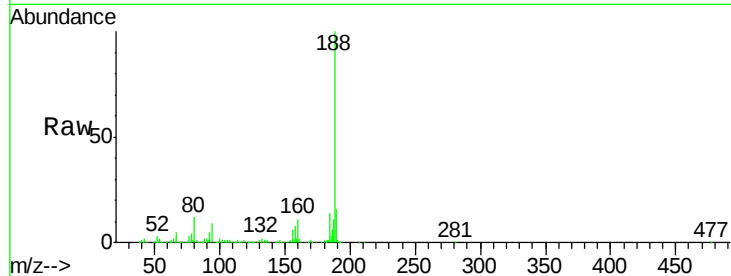

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

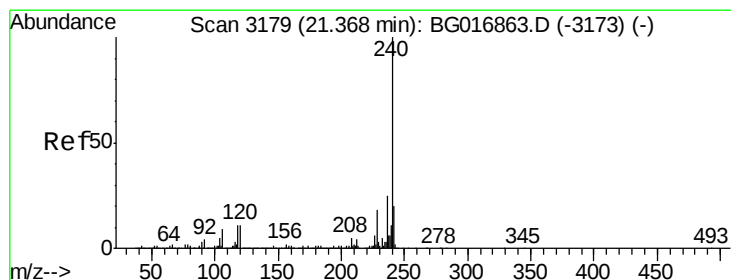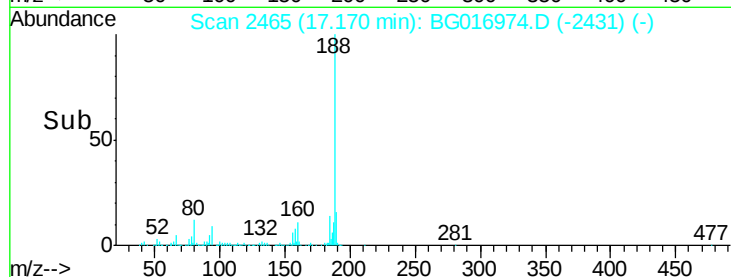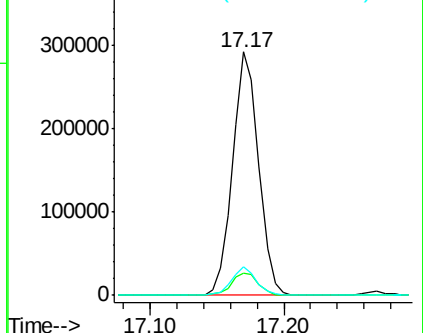

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.35 min Scan# 3176

Delta R.T. -0.00 min

Lab File: BG016974.D

Acq: 9 May 2015 3:36


Tgt Ion:240 Resp: 393897

Ion Ratio Lower Upper

240 100

120 10.1 9.1 13.7



236 26.8 20.2 30.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

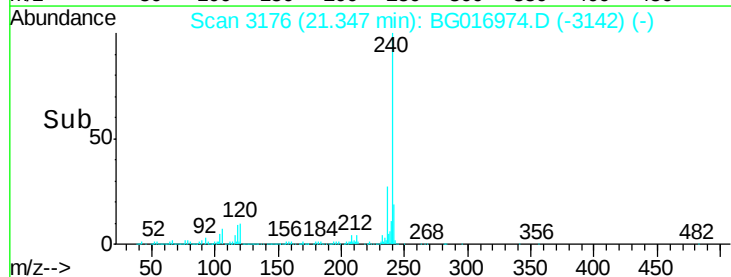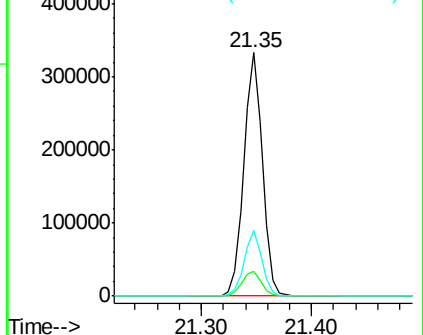







#78
 Terphenyl-d14
 Concen: 94.36 ng
 RT: 19.80 min Scan# 2913
 Delta R.T. 0.00 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36

Instrument :
 BNA_G
 ClientSampleId :
 A3-SEEP

Tgt Ion:244 Resp: 1585454
 Ion Ratio Lower Upper
 244 100
 212 8.8 7.0 10.6
 122 12.3 10.4 15.6




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

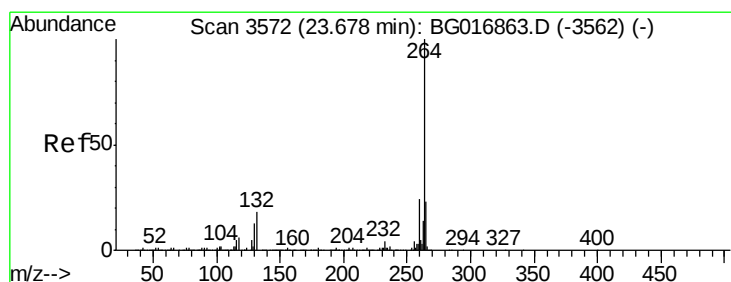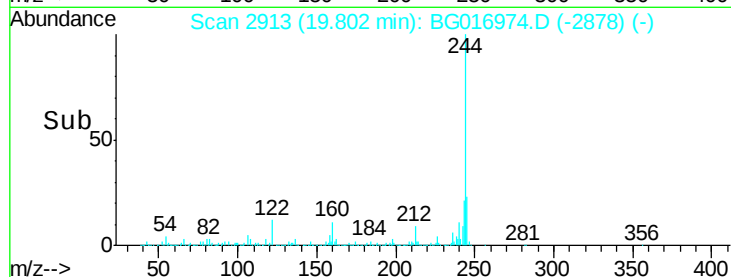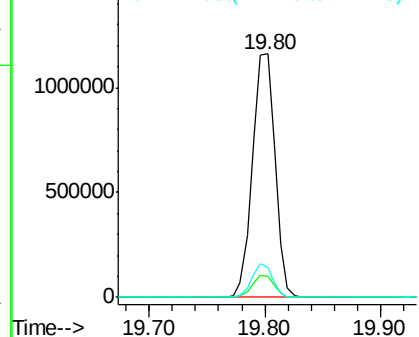

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.64 min Scan# 3567
 Delta R.T. -0.00 min
 Lab File: BG016974.D
 Acq: 9 May 2015 3:36

Tgt Ion:264 Resp: 376061
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.5 29.3
 265 22.4 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

