

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
 Data File : BG017044.D
 Acq On : 11 May 2015 3:40
 Operator : TP/IZ
 Sample : G2109-10
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 W-33

Quant Time: May 11 06:00:20 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 11 05:17:53 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	62502	20.00	ng	0.00
21) Naphthalene-d8	10.58	136	302520	20.00	ng	0.00
38) Acenaphthene-d10	14.43	164	202014	20.00	ng	0.00
63) Phenanthrene-d10	17.17	188	456325	20.00	ng	0.00
75) Chrysene-d12	21.34	240	426897	20.00	ng	0.00
86) Perylene-d12	23.64	264	433054	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	260765	72.65	ng	0.00
7) Phenol-d6	6.98	99	223228	43.53	ng	0.00
23) Nitrobenzene-d5	8.95	82	585018	94.47	ng	0.00
41) 2,4,6-Tribromophenol	15.92	330	362173	178.58	ng	0.00
44) 2-Fluorobiphenyl	13.05	172	1198059	89.49	ng	0.00
78) Terphenyl-d14	19.80	244	1545048	84.84	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.88	163	33310	2.21	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG017044.D
Acq On : 11 May 2015 3:40
Operator : TP/IZ
Sample : G2109-10
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
W-33

Quant Time: May 11 06:00:20 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 05:17:53 2015
Response via : Initial Calibration

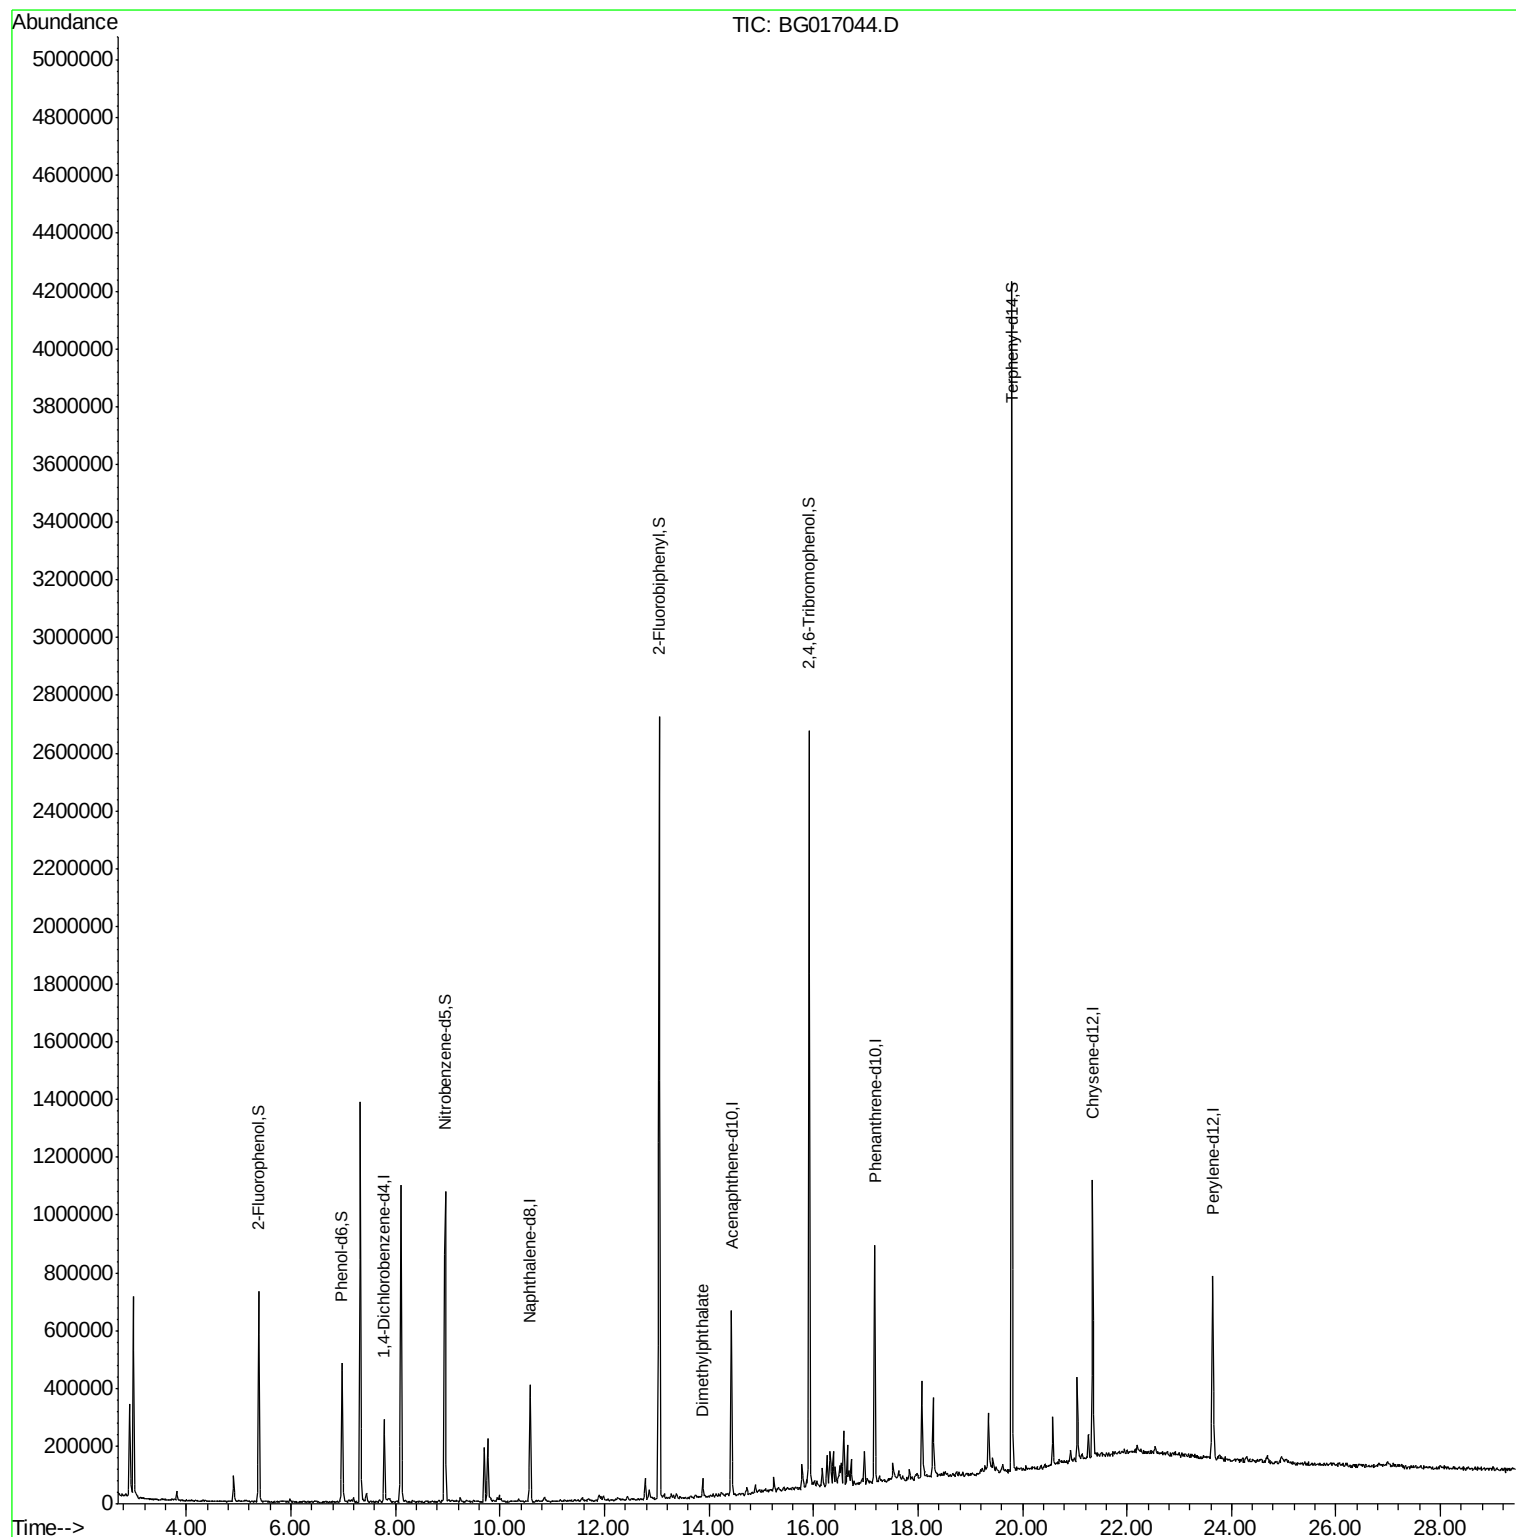







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.79 min Scan# 868
Delta R.T. 0.00 min
Lab File: BG017044.D
Acq: 11 May 2015 3:40

Instrument :
BNA_G
ClientSampleId :
W-33




Tgt Ion	Ratio	Lower	Upper
152	100		
150	150.0	121.0	181.4
115	57.2	50.5	75.7

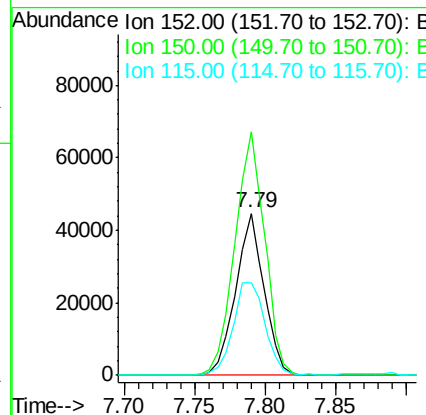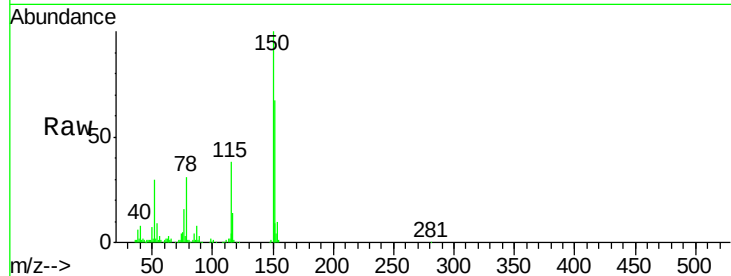


#5

2-Fluorophenol
Concen: 72.65 ng
RT: 5.39 min Scan# 459
Delta R.T. 0.01 min
Lab File: BG017044.D
Acq: 11 May 2015 3:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.8	51.4	77.2
63	39.0	28.1	42.1

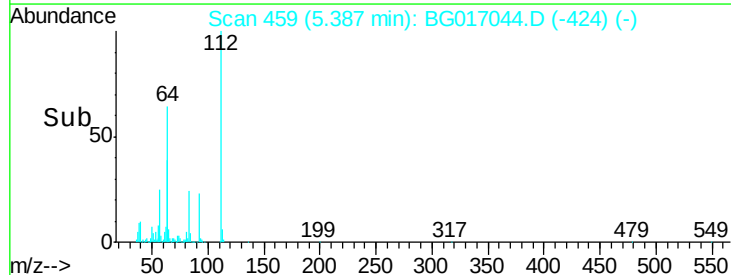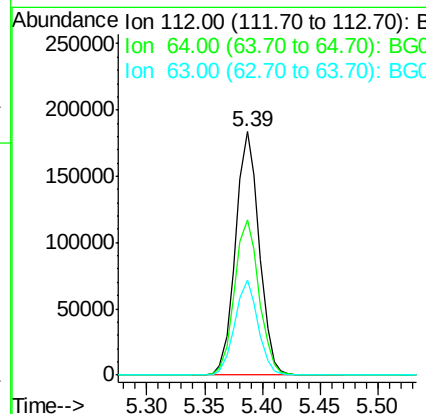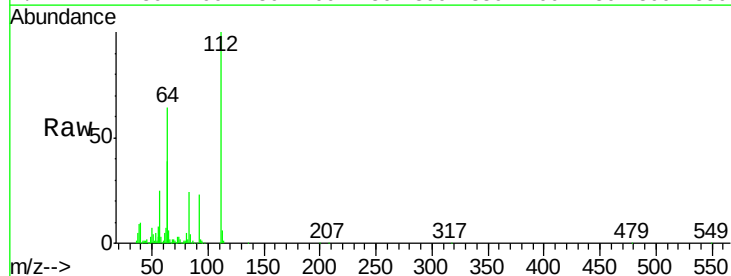

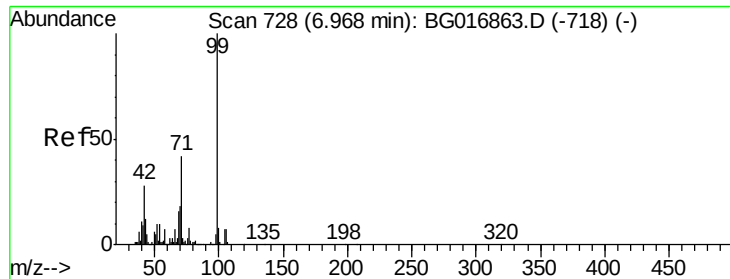

#7

Phenol-d6

Concen: 43.53 ng

RT: 6.98 min Scan# 730

Delta R.T. 0.01 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Instrument :

BNA_G

ClientSampleId :

W-33


Tgt Ion: 99 Resp: 223228

Ion Ratio Lower Upper




99 100

42 28.2 22.1 33.1

71 43.4 33.4 50.0

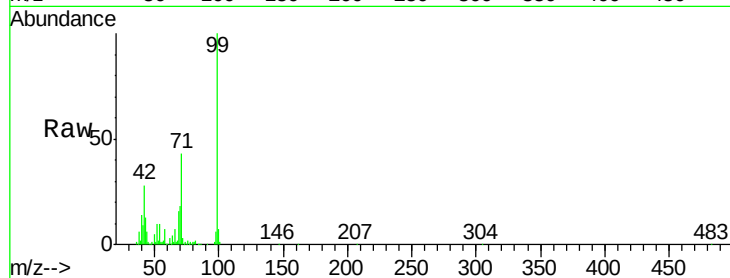

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

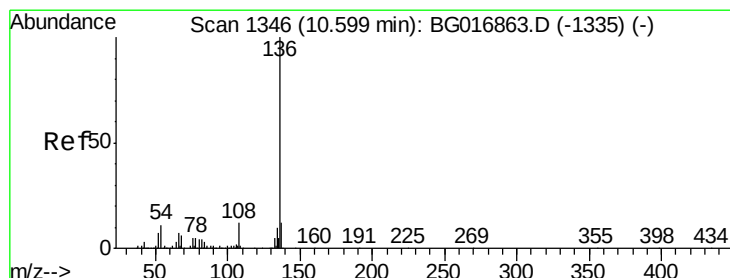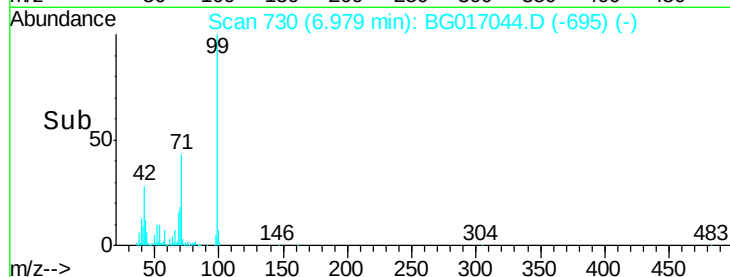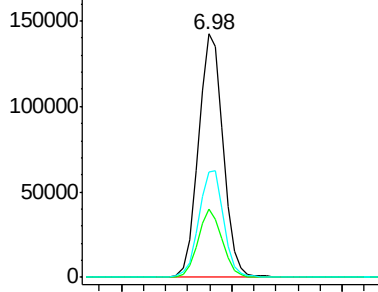

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1343

Delta R.T. 0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Tgt Ion: 136 Resp: 302520


Ion Ratio Lower Upper

136 100



137 10.5 9.8 14.8


54 9.3 8.7 13.1

68 5.3 5.0 7.4

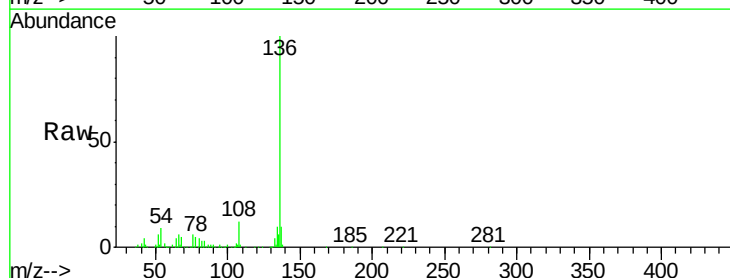

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



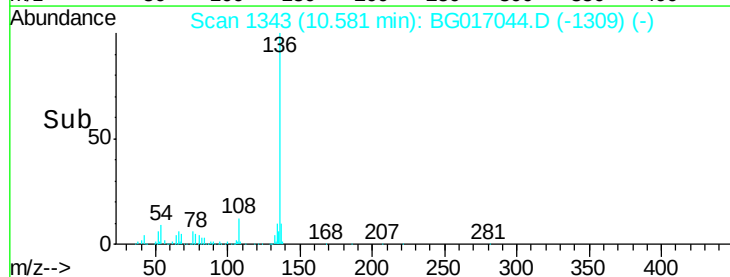
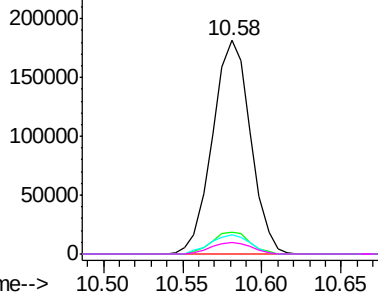




#23
 Nitrobenzene-d5
 Concen: 94.47 ng
 RT: 8.95 min Scan# 1065
 Delta R.T. -0.00 min
 Lab File: BG017044.D
 Acq: 11 May 2015 3:40




Instrument :
 BNA_G
 ClientSampleId :
 W-33


Tgt Ion: 82 Resp: 585018
 Ion Ratio Lower Upper
 82 100
 128 40.8 33.2 49.8
 54 59.1 48.6 72.8

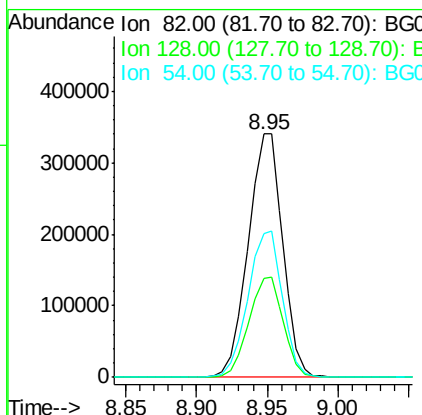

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. 0.00 min
 Lab File: BG017044.D
 Acq: 11 May 2015 3:40

Tgt Ion: 164 Resp: 202014
 Ion Ratio Lower Upper
 164 100
 162 98.5 74.0 111.0
 160 42.0 34.7 52.1

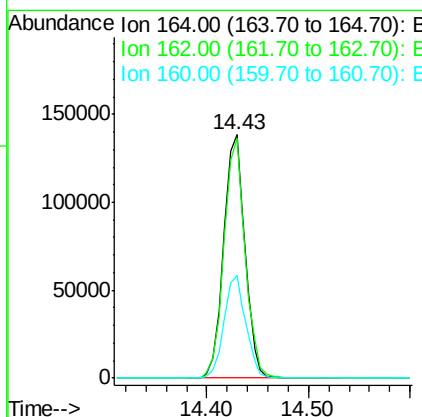



#41

2,4,6-Tribromophenol

Concen: 178.58 ng

RT: 15.92 min Scan# 2252

Delta R.T. 0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Instrument :

BNA_G

ClientSampleId :

W-33


Tgt Ion:330 Resp: 362173

Ion Ratio Lower Upper




330 100

332 96.0 0.0 0.0#

141 50.7 0.0 0.0#

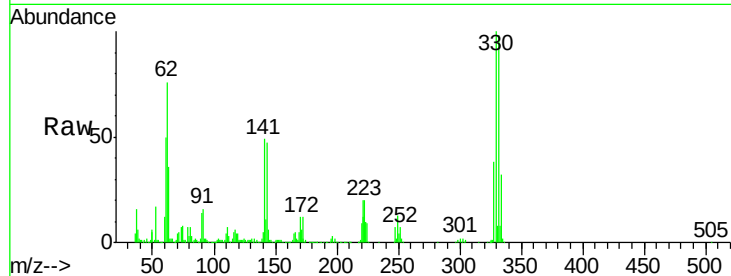

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

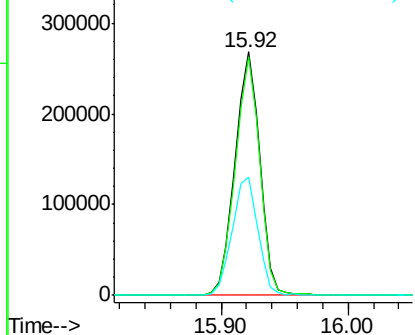

#44

2-Fluorobiphenyl

Concen: 89.49 ng

RT: 13.05 min Scan# 1763

Delta R.T. -0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40


Tgt Ion:172 Resp: 1198059

Ion Ratio Lower Upper



172 100


171 37.7 29.0 43.4

170 24.8 19.0 28.4



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

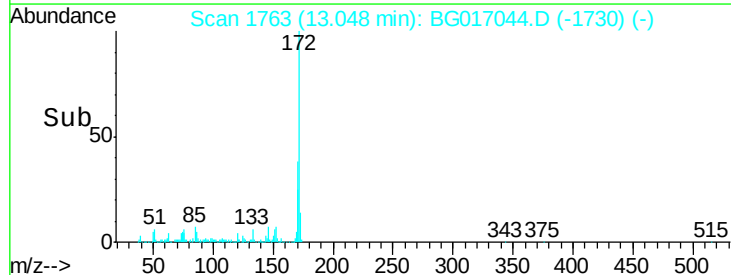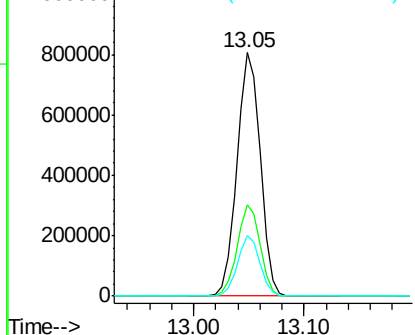



#49

Dimethylphthalate

Concen: 2.21 ng

RT: 13.88 min Scan# 1905

Delta R.T. -0.01 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Instrument :

BNA_G

ClientSampleId :

W-33


Tgt Ion:163 Resp: 33310

Ion Ratio Lower Upper




163 100

194 4.6 5.2 7.8#

164 9.9 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

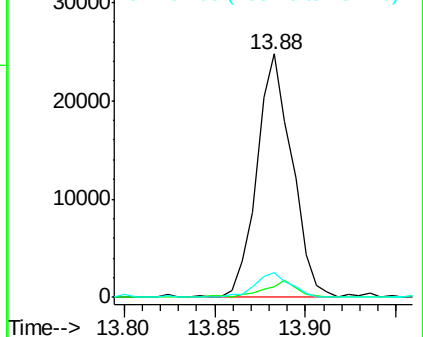

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2465

Delta R.T. 0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40


Tgt Ion:188 Resp: 456325

Ion Ratio Lower Upper



188 100


94 9.4 8.2 12.4

80 9.9 8.8 13.2



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

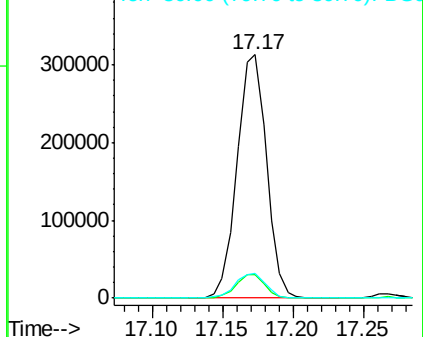



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.34 min Scan# 3175

Delta R.T. -0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Instrument :

BNA_G

ClientSampleId :

W-33


Tgt Ion:240 Resp: 426897

Ion Ratio Lower Upper

240 100

120 11.1 9.1 13.7




236 26.3 20.2 30.4

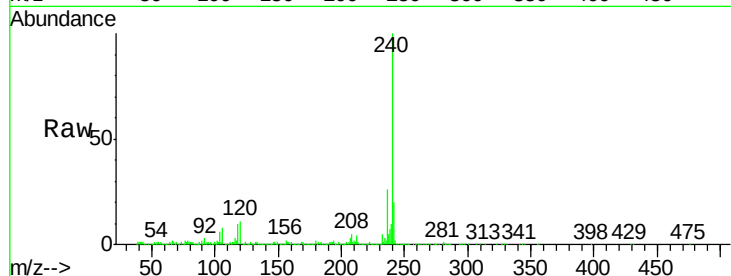

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

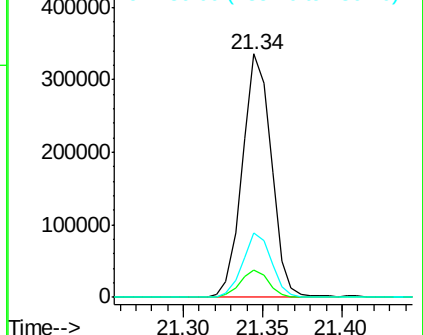

#78

Terphenyl-d14

Concen: 84.84 ng

RT: 19.80 min Scan# 2912

Delta R.T. 0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40


Tgt Ion:244 Resp: 1545048

Ion Ratio Lower Upper

244 100

212 9.0 7.0 10.6



122 12.4 10.4 15.6




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

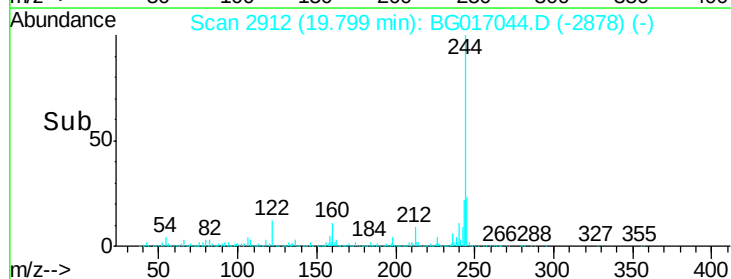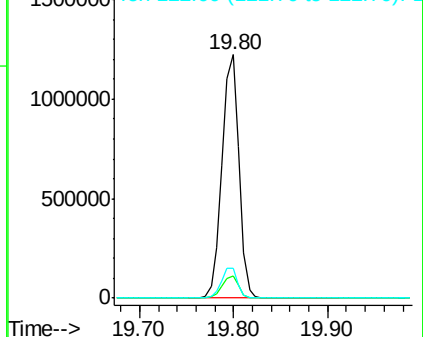

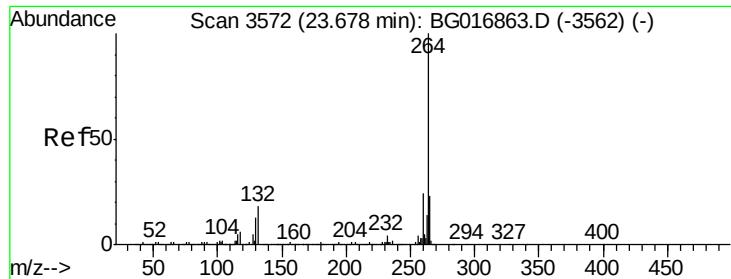

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.64 min Scan# 3566

Delta R.T. -0.00 min

Lab File: BG017044.D

Acq: 11 May 2015 3:40

Instrument :

BNA_G

ClientSampleId :

W-33

Tgt Ion: 264 Resp: 433054

Ion Ratio Lower Upper

264 100

260 23.1 19.5 29.3

265 22.2 18.5 27.7

