


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050815\
 Data File : BG016950.D
 Acq On : 8 May 2015 11:00
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 05 16:13:58 2015

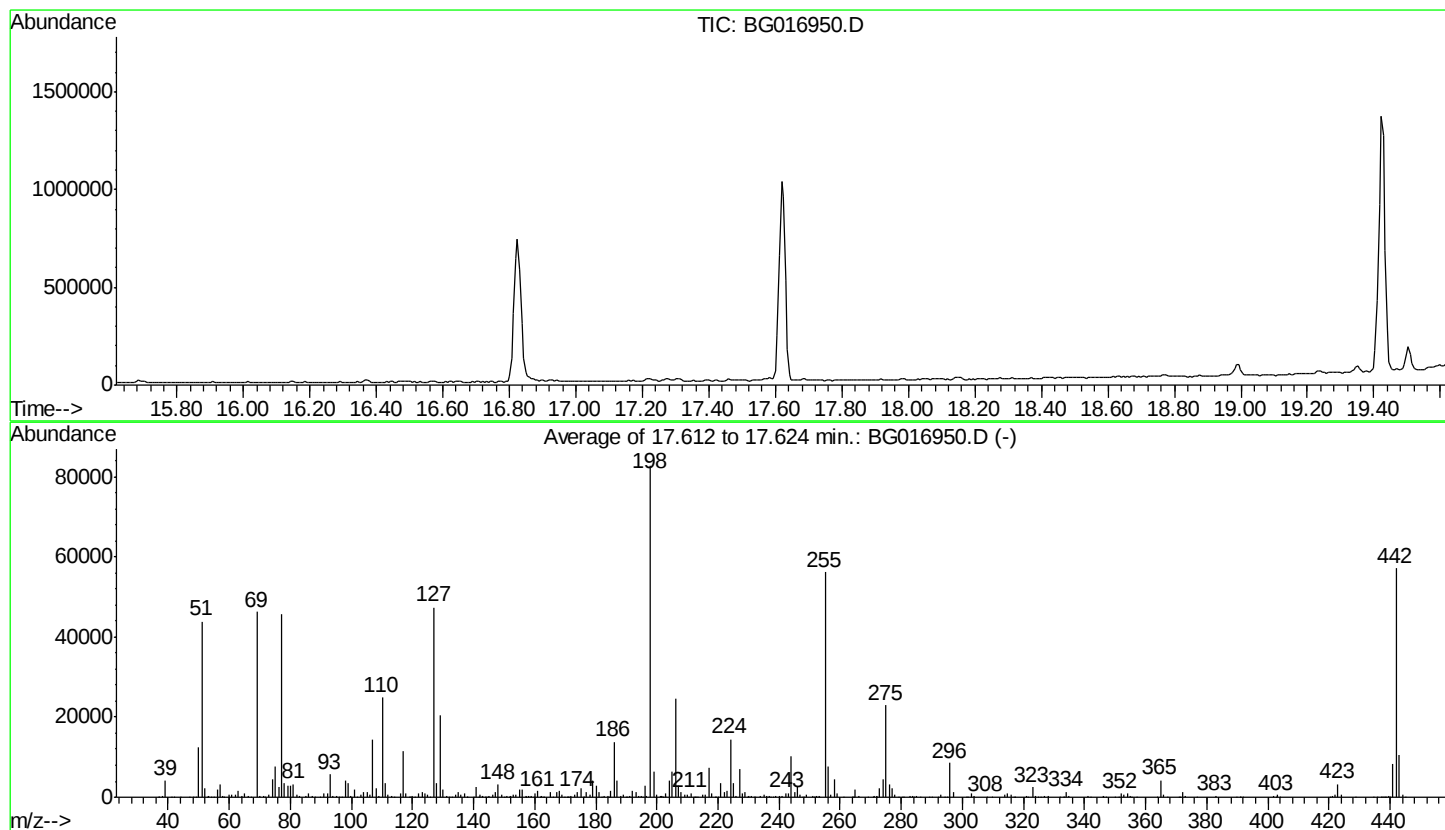

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2534

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	43805	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.9	46299	PASS
70	69	0.00	2	0.8	357	PASS
127	198	10	80	57.1	47293	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82776	PASS
199	198	5	9	7.7	6349	PASS
275	198	10	60	27.7	22906	PASS
365	198	1	100	5.1	4237	PASS
441	442	0.01	24	14.6	8338	PASS
442	198	50	100	69.0	57088	PASS
443	442	15	24	18.5	10544	PASS