

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050819\
 Data File : BG040796.D
 Acq On : 8 May 2019 20:17
 Operator : HP/JU
 Sample : K2641-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-050719-A

Quant Time: May 09 05:19:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	38670	20.00	ng	-0.02
21) Naphthalene-d8	10.97	136	156816	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	119309	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	344355	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	321205	20.00	ng	-0.03
87) Perylene-d12	25.15	264	235582	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	363641	165.77	ng	-0.01
7) Phenol-d6	7.28	99	483613	143.18	ng	-0.02
23) Nitrobenzene-d5	9.32	82	429357	126.51	ng	-0.02
42) 2,4,6-Tribromophenol	16.25	330	275670	168.10	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	913014	110.52	ng	-0.02
79) Terphenyl-d14	20.11	244	1903421	131.28	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050819\
Data File : BG040796.D
Acq On : 8 May 2019 20:17
Operator : HP/JU
Sample : K2641-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-050719-A

Quant Time: May 09 05:19:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

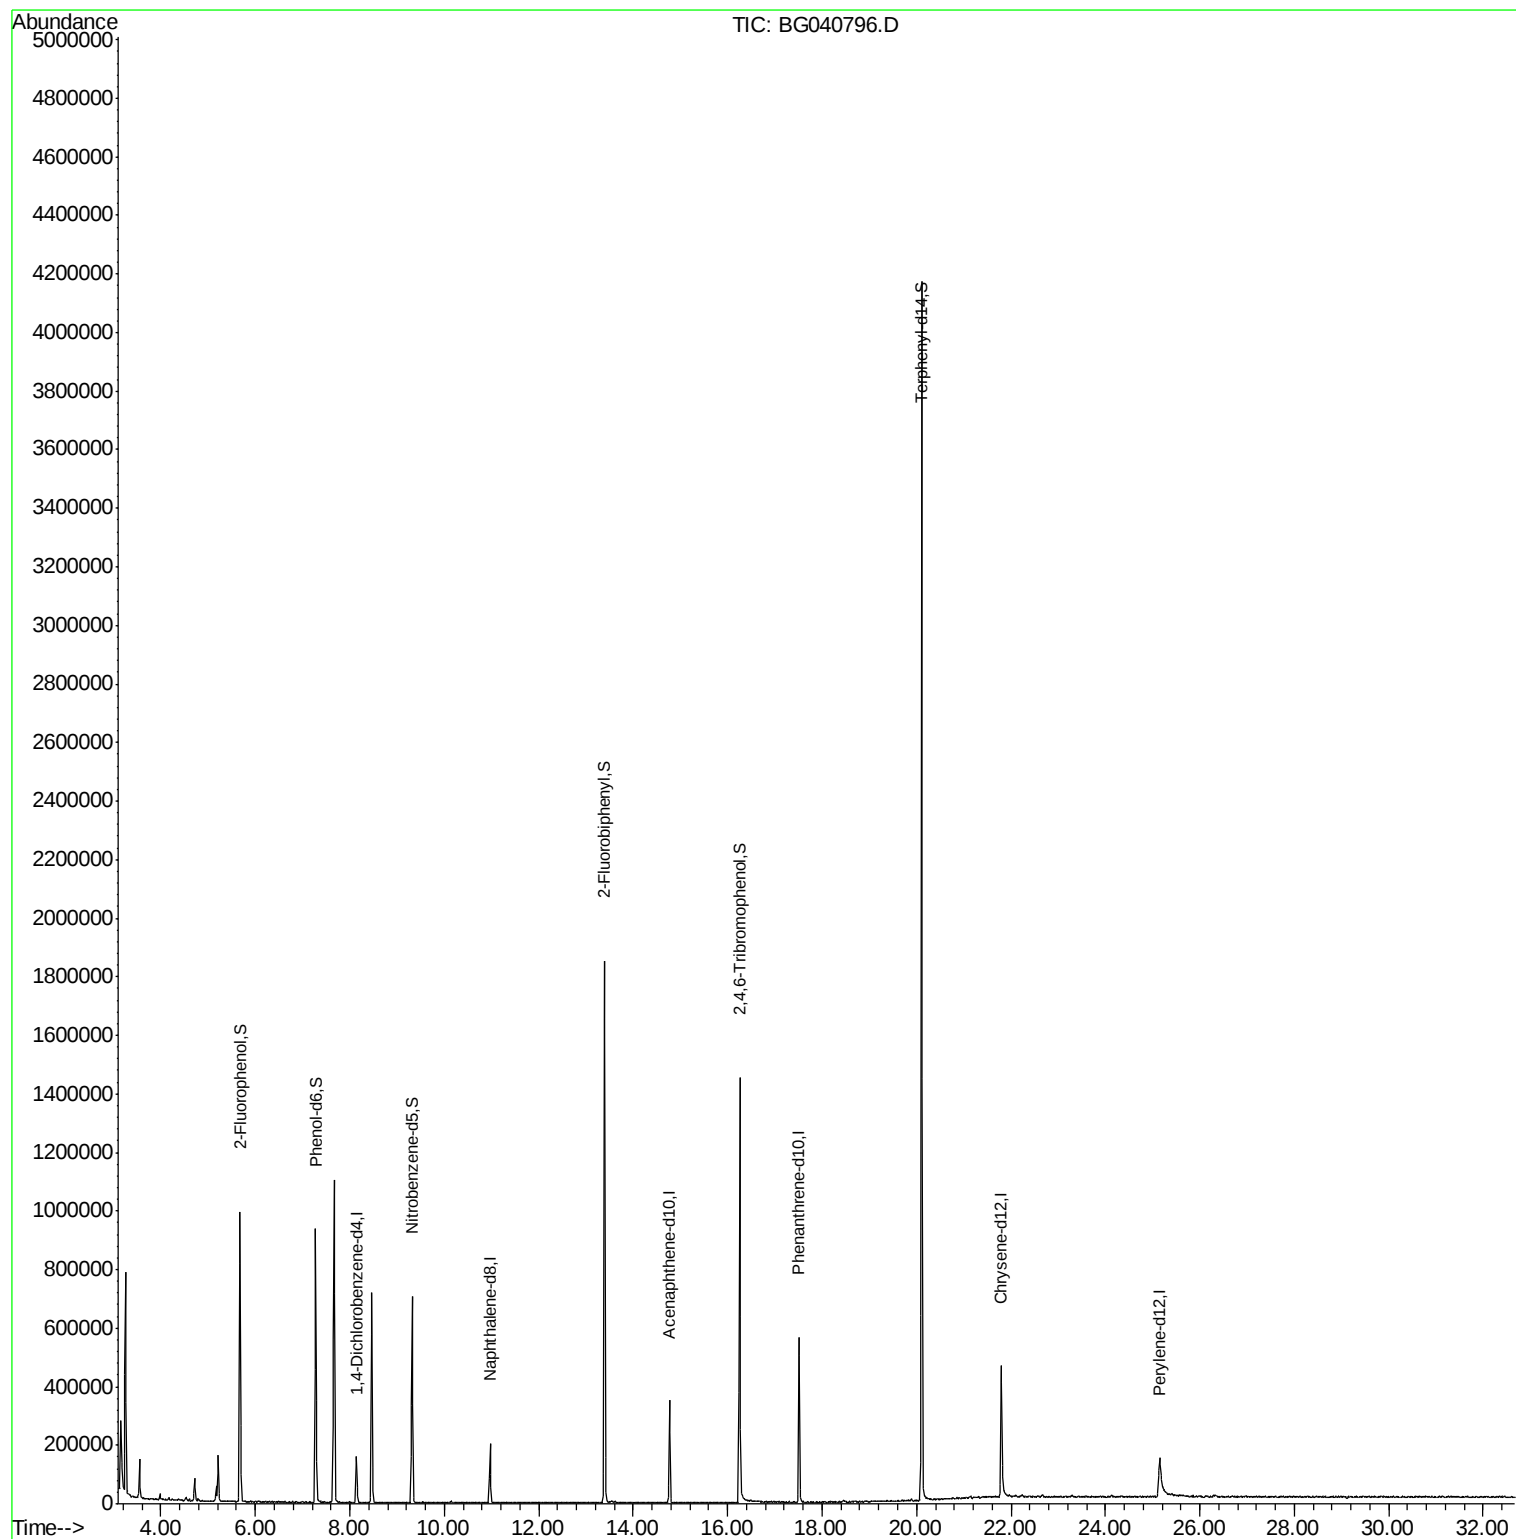




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.02 min
Lab File: BG040796.D
Acq: 8 May 2019 20:17

Instrument :
BNA_G
ClientSampleId :
CL-02-050719-A

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.8	120.2	180.2
115	58.3	46.2	69.2


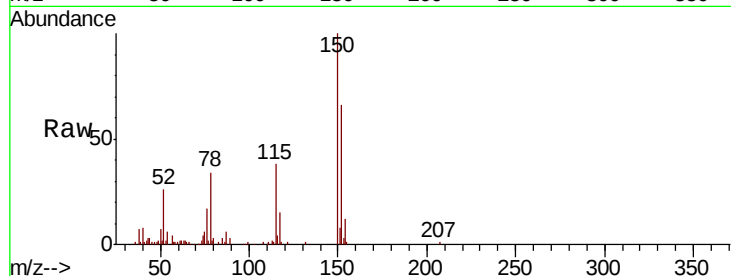


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

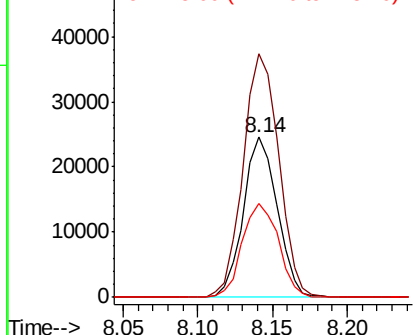

#5

2-Fluorophenol
Concen: 165.765 ng
RT: 5.67 min Scan# 440
Delta R.T. -0.01 min
Lab File: BG040796.D
Acq: 8 May 2019 20:17

Tgt Ion	Ratio	Lower	Upper
112	100		
64	74.3	61.4	92.0
63	43.3	37.8	56.6


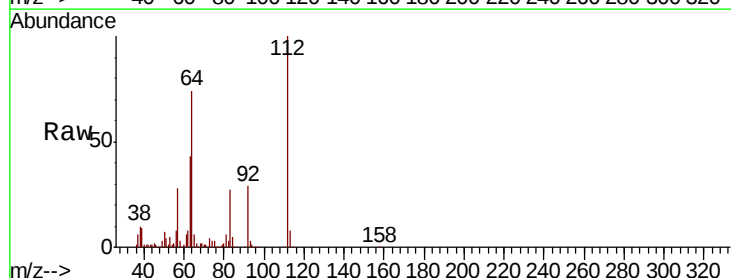


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

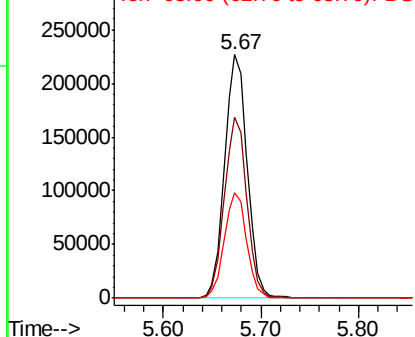



#7

Phenol-d6

Concen: 143.178 ng

RT: 7.28 min Scan# 713

Delta R.T. -0.02 min

Lab File: BG040796.D

Acq: 8 May 2019 20:17

Instrument :

BNA_G

ClientSampleId :

CL-02-050719-A


Tot Ion: 99 Resp: 483613

Ion Ratio Lower Upper




99 100

42 24.0 21.8 32.8

71 46.7 38.6 57.8

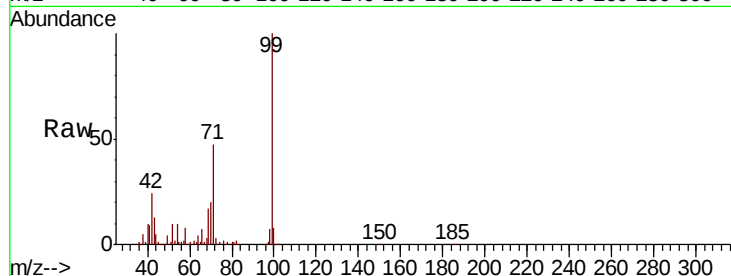

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

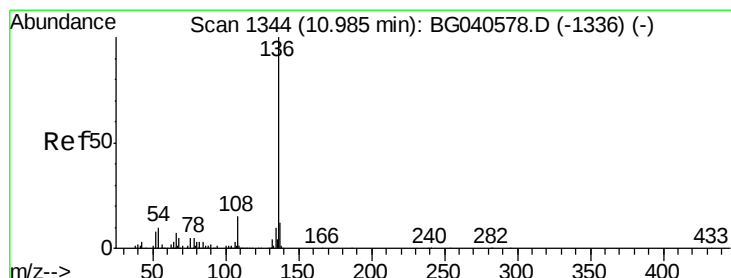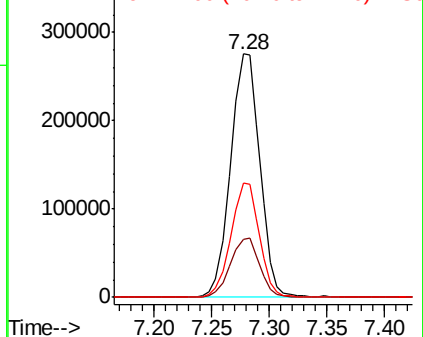

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1341

Delta R.T. -0.02 min

Lab File: BG040796.D

Acq: 8 May 2019 20:17

Tgt Ion: 136 Resp: 156816


Ion Ratio Lower Upper

136 100



137 11.6 9.7 14.5


54 8.6 8.6 12.8

68 5.0 4.8 7.2

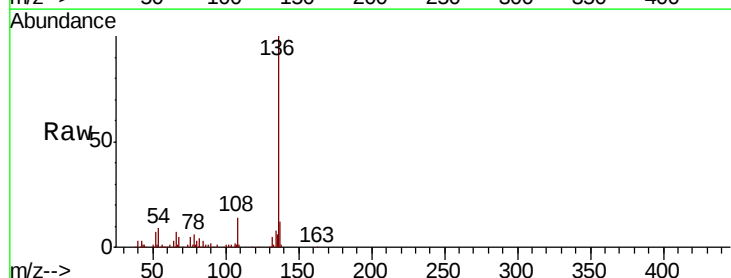

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




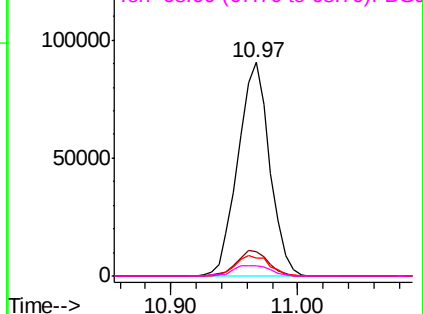




#23
 Nitrobenzene-d5
 Concen: 126.511 ng
 RT: 9.32 min Scan# 1061
 Delta R.T. -0.02 min
 Lab File: BG040796.D
 Acq: 8 May 2019 20:17




Instrument :
 BNA_G
 ClientSampleId :
 CL-02-050719-A


Tot Ion	82	Resp	429357
Ion	Ratio	Lower	Upper
82	100		
128	36.3	28.9	43.3
54	55.6	47.2	70.8

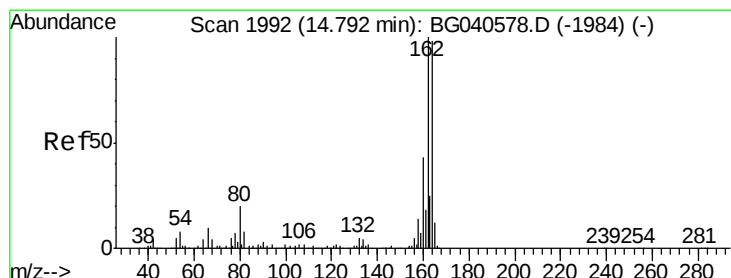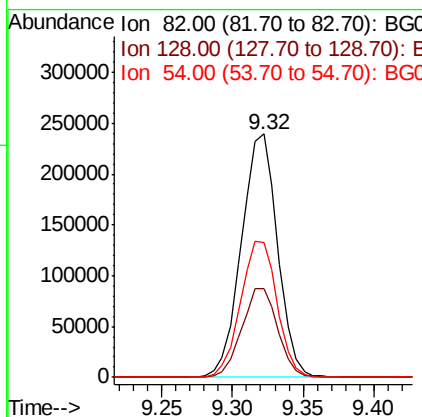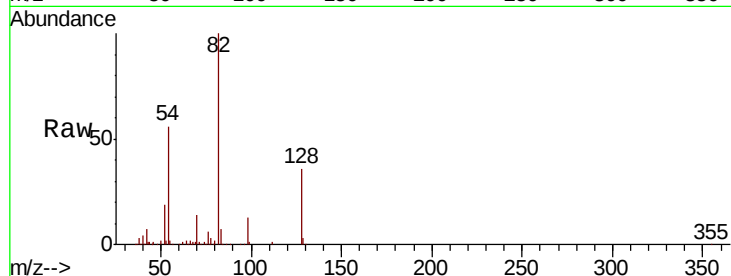

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.77 min Scan# 1988
 Delta R.T. -0.02 min
 Lab File: BG040796.D
 Acq: 8 May 2019 20:17

Tgt Ion	164	Resp	119309
Ion	Ratio	Lower	Upper
164	100		
162	104.1	81.9	122.9
160	47.1	35.4	53.2

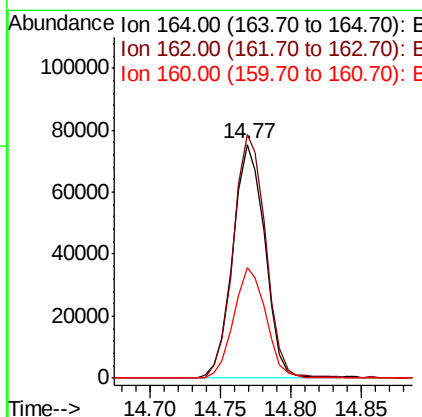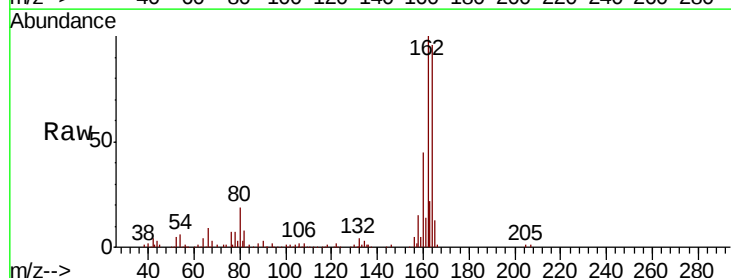




#42
 2,4,6-Tribromophenol
 Concen: 168.099 ng
 RT: 16.25 min Scan# 2241
 Delta R.T. -0.02 min
 Lab File: BG040796.D
 Acq: 8 May 2019 20:17




Instrument :
 BNA_G
 ClientSampleId :
 CL-02-050719-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.7	75.9	113.9
141	36.7	32.4	48.6

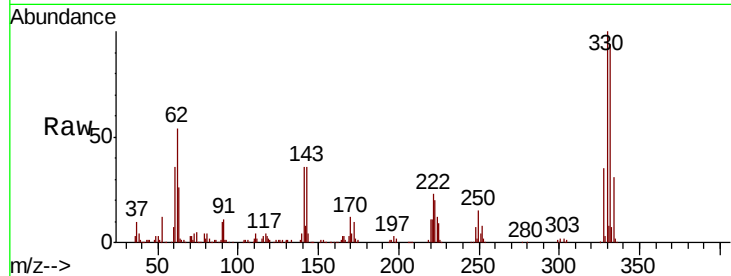


Abundance

Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

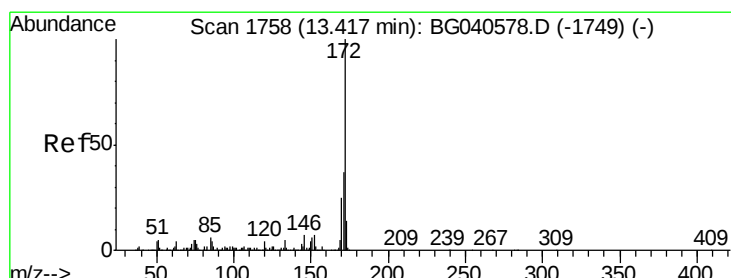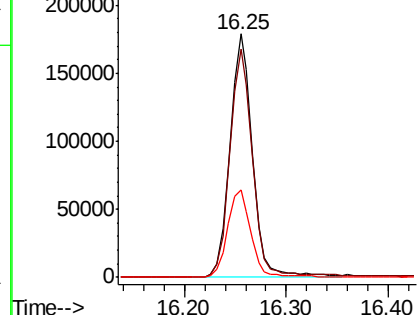



#45
 2-Fluorobiphenyl
 Concen: 110.518 ng
 RT: 13.39 min Scan# 1754
 Delta R.T. -0.02 min
 Lab File: BG040796.D
 Acq: 8 May 2019 20:17


Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	29.4	44.2
170	24.7	19.9	29.9

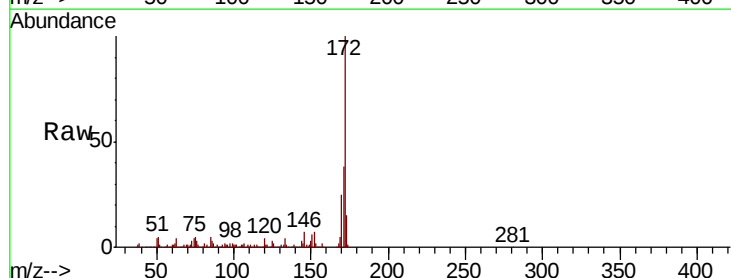

Abundance

Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



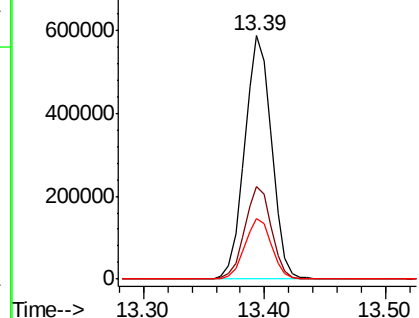



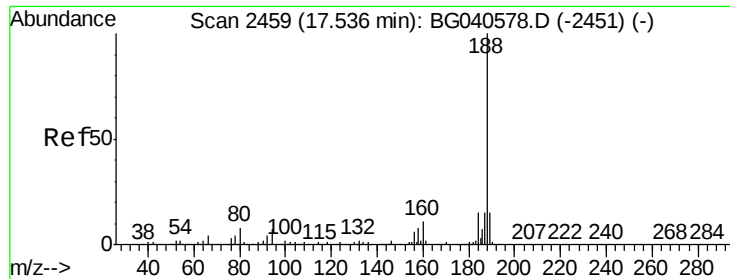

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.51 min Scan# 2455
Delta R.T. -0.02 min
Lab File: BG040796.D
Acq: 8 May 2019 20:17




Instrument :
BNA_G
ClientSampleId :
CL-02-050719-A


Tot Ion	Ratio	Lower	Upper
188	100		
94	6.8	5.6	8.4
80	7.8	6.4	9.6

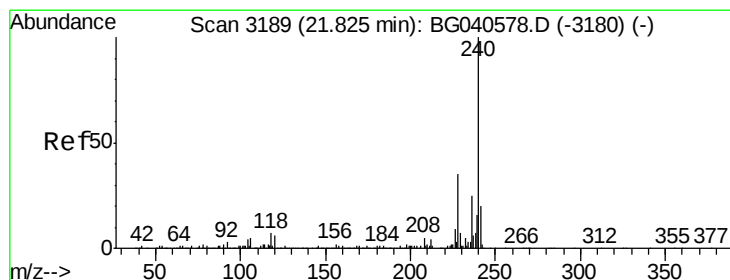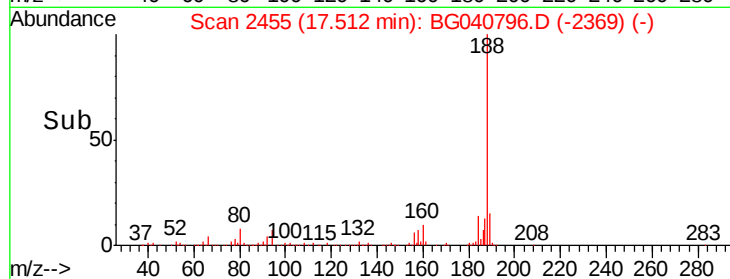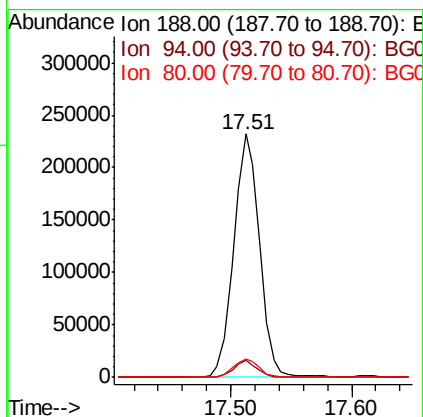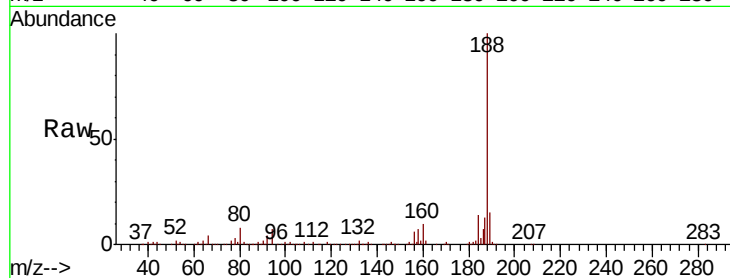

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.80 min Scan# 3184
Delta R.T. -0.03 min
Lab File: BG040796.D
Acq: 8 May 2019 20:17

Tgt Ion	Ratio	Lower	Upper
240	100		
120	4.8	5.0	7.6#
236	25.9	20.3	30.5

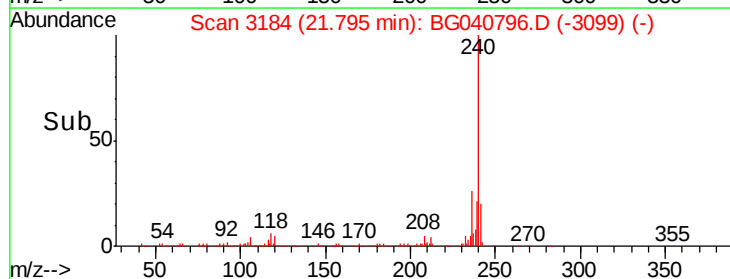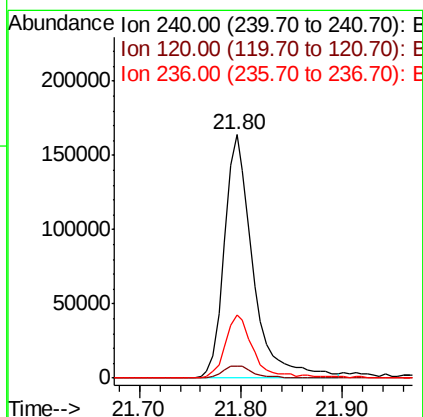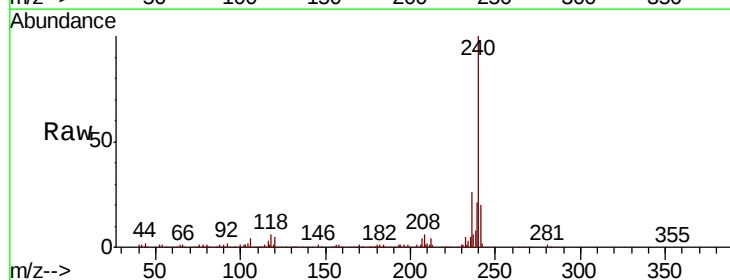

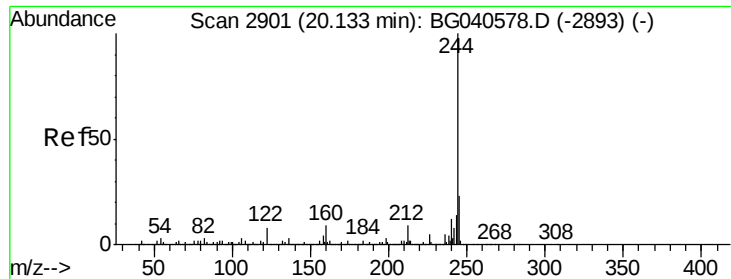

#79

Terphenyl-d14

Concen: 131.283 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040796.D

Acq: 8 May 2019 20:17

Instrument :

BNA_G

ClientSampleId :

CL-02-050719-A


Tot Ion:244 Resp: 1903421

Ion Ratio Lower Upper

244 100

212 9.5 7.2 10.8




122 8.0 6.6 10.0

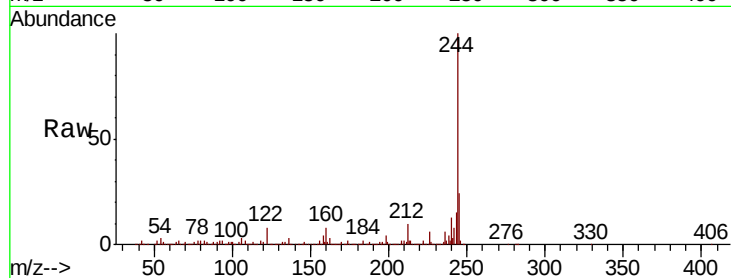

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

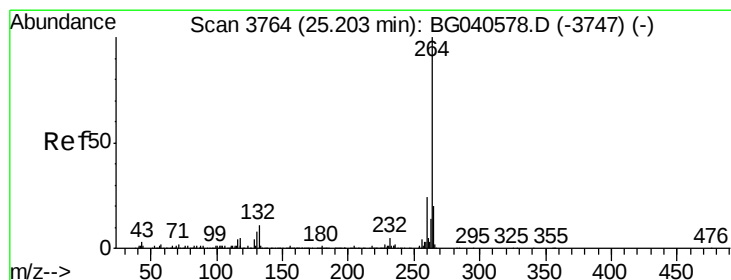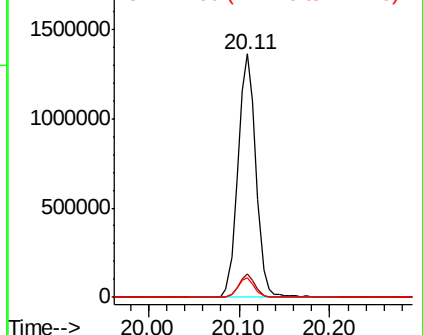

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3755

Delta R.T. -0.05 min

Lab File: BG040796.D

Acq: 8 May 2019 20:17


Tgt Ion:264 Resp: 235582

Ion Ratio Lower Upper

264 100

260 23.5 19.2 28.8

265 22.7 16.6 25.0

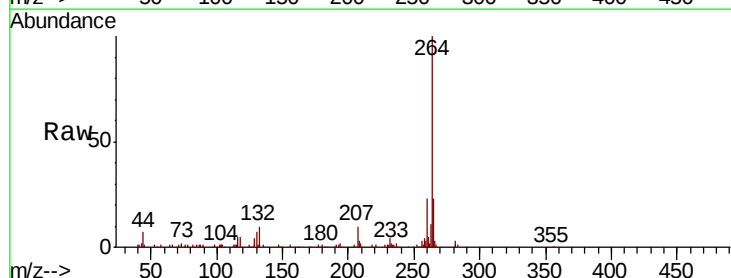

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

