

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050819\
 Data File : BG040817.D
 Acq On : 9 May 2019 11:29
 Operator : HP/JU
 Sample : K2645-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-050719-D

Quant Time: May 09 15:05:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	42293	20.00	ng	-0.02
21) Naphthalene-d8	10.96	136	170342	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	128881	20.00	ng	-0.03
64) Phenanthrene-d10	17.51	188	359002	20.00	ng	-0.03
76) Chrysene-d12	21.79	240	329716	20.00	ng	-0.03
87) Perylene-d12	25.15	264	234385	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	372854	155.40	ng	-0.01
7) Phenol-d6	7.28	99	507742	137.44	ng	-0.01
23) Nitrobenzene-d5	9.32	82	446049	120.99	ng	-0.02
42) 2,4,6-Tribromophenol	16.25	330	268323	151.47	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	985697	110.45	ng	-0.03
79) Terphenyl-d14	20.11	244	1981332	133.13	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050819\
Data File : BG040817.D
Acq On : 9 May 2019 11:29
Operator : HP/JU
Sample : K2645-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-02-050719-D

Quant Time: May 09 15:05:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

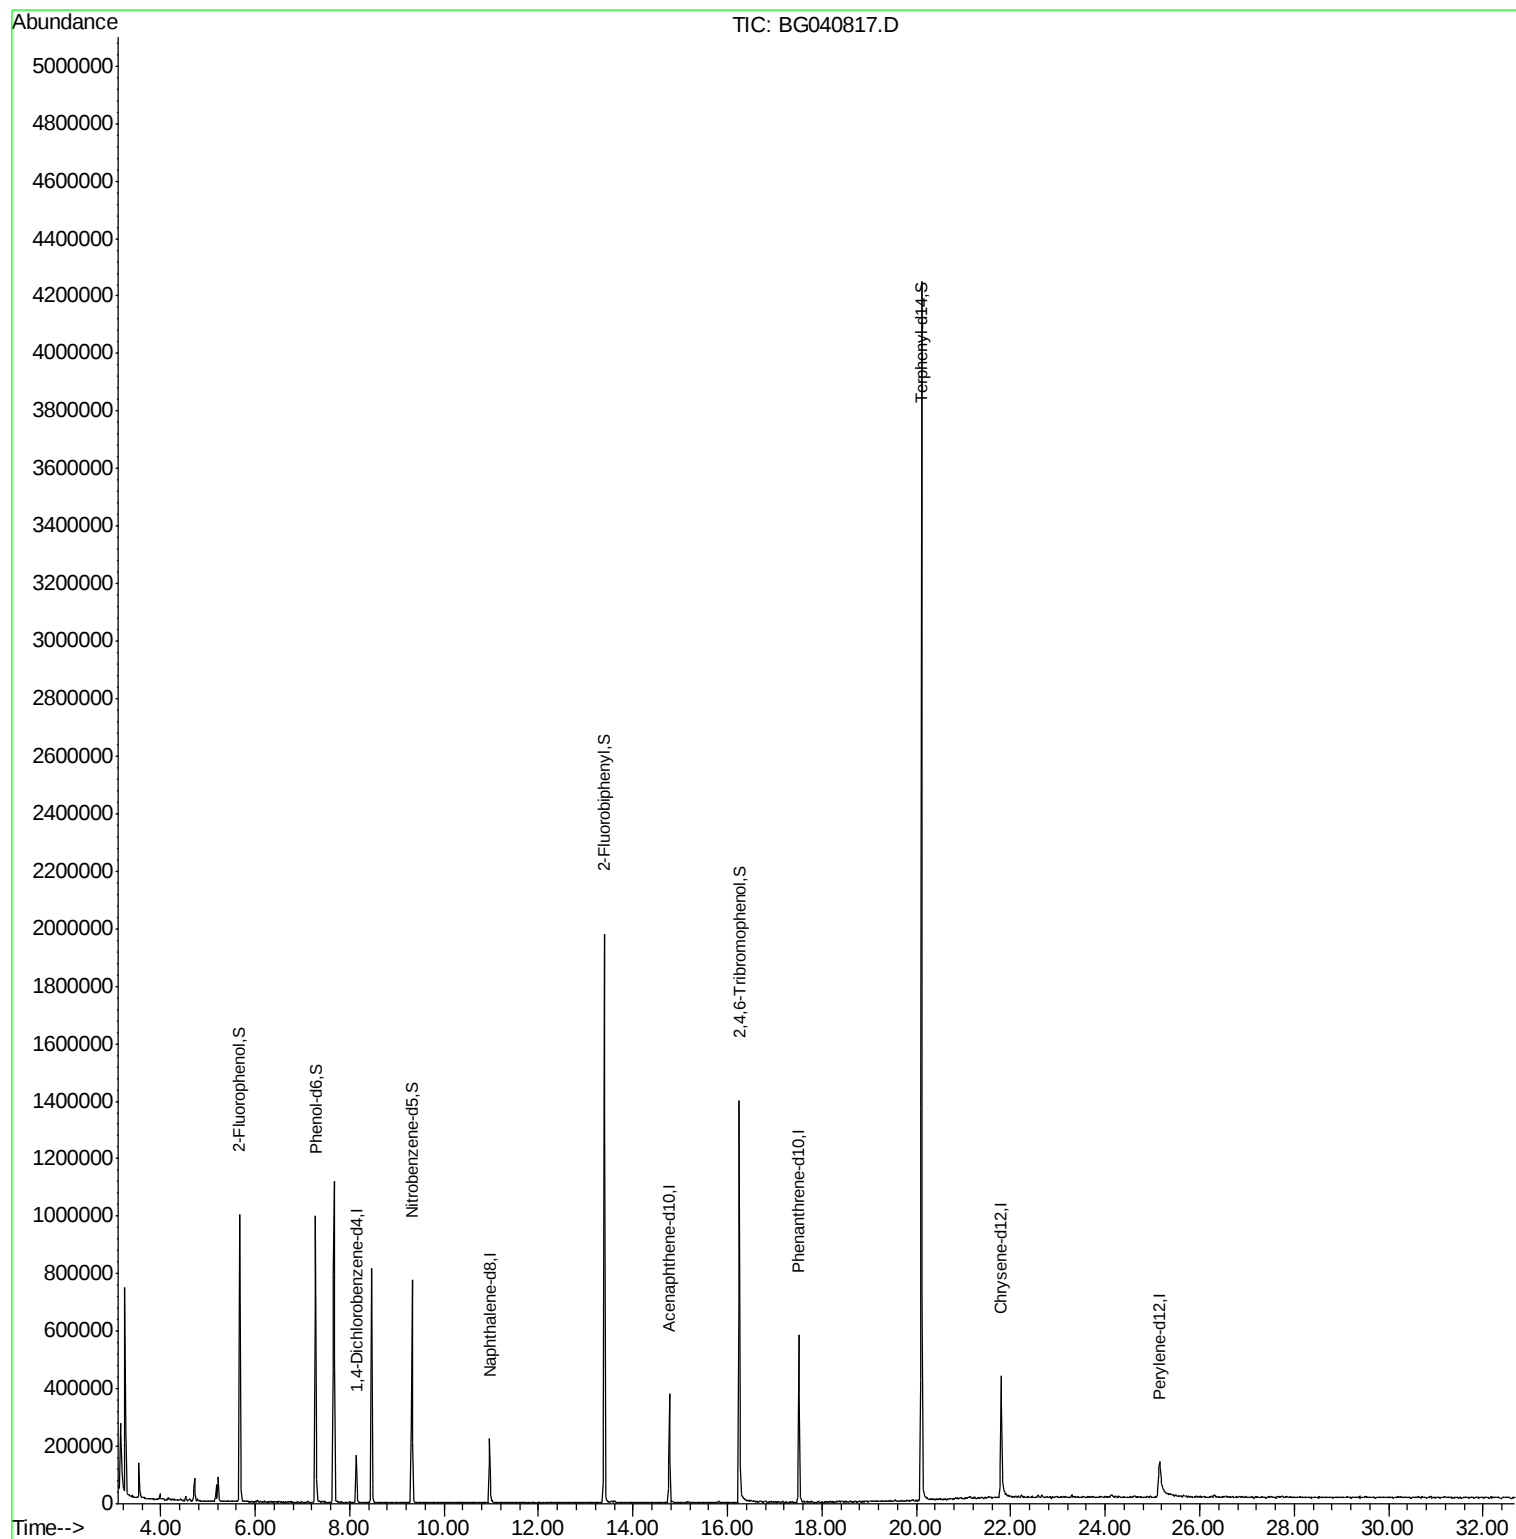




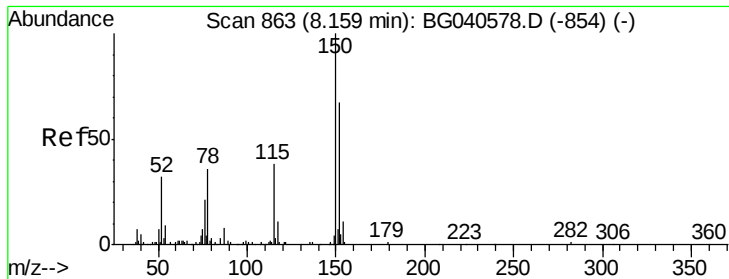


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 859
Delta R.T. -0.02 min
Lab File: BG040817.D
Acq: 9 May 2019 11:29

Instrument :
BNA_G
ClientSampleId :
PL-02-050719-D




Tot Ion	Ratio	Lower	Upper
152	100		
150	147.6	120.2	180.2
115	58.9	46.2	69.2

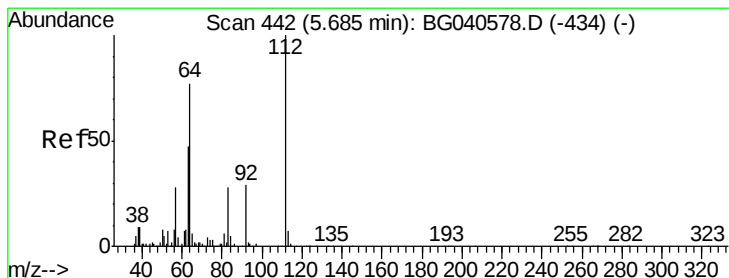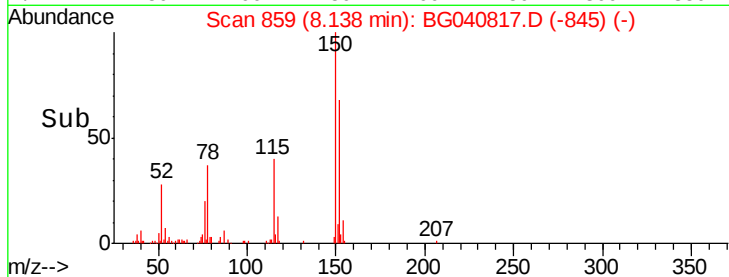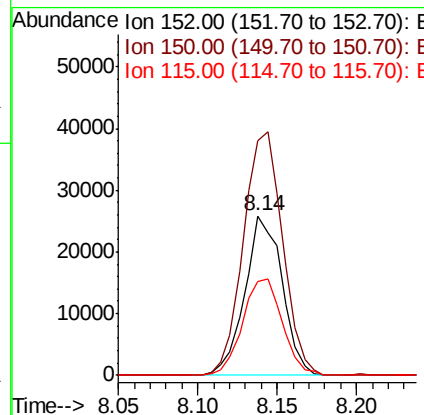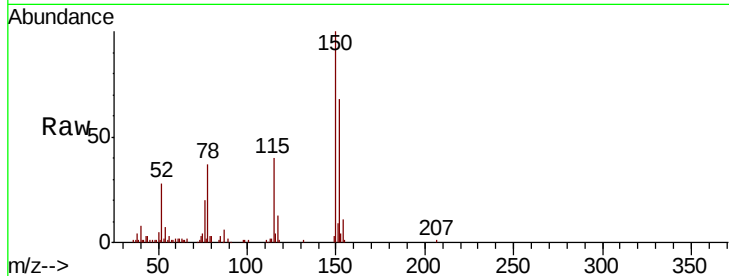

#5

2-Fluorophenol
Concen: 155.405 ng
RT: 5.67 min Scan# 439
Delta R.T. -0.01 min
Lab File: BG040817.D
Acq: 9 May 2019 11:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	77.0	61.4	92.0
63	44.2	37.8	56.6

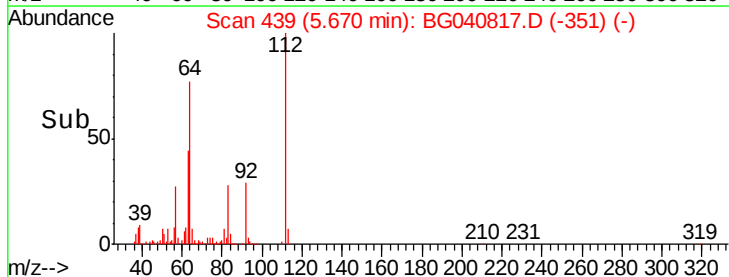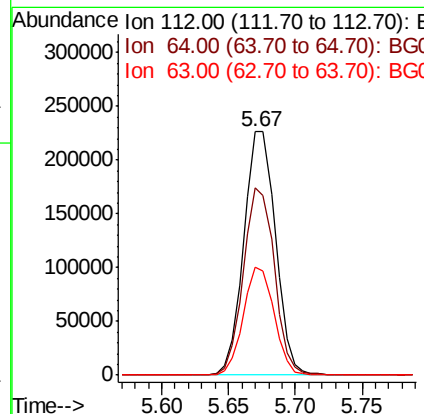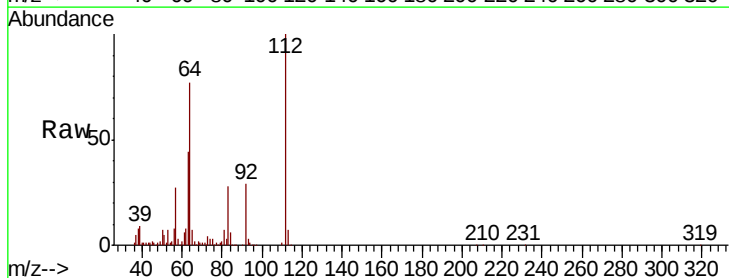



#7

Phenol-d6

Concen: 137.445 ng

RT: 7.28 min Scan# 713

Delta R.T. -0.01 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29

Instrument :

BNA_G

ClientSampleId :

PL-02-050719-D





Tot Ion: 99 Resp: 507742

Ion Ratio Lower Upper

99 100

42 24.0 21.8 32.8

71 46.4 38.6 57.8

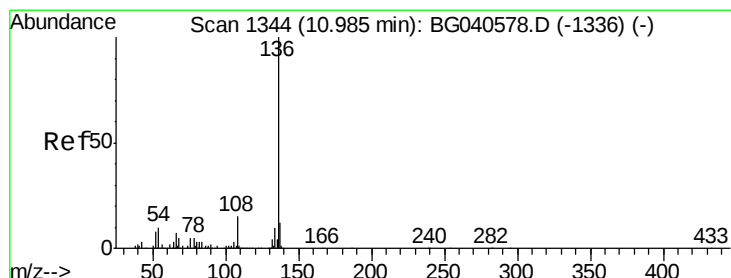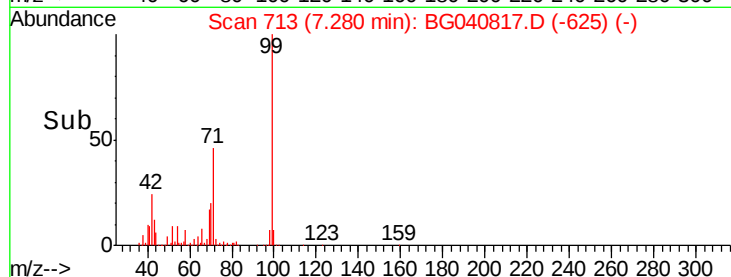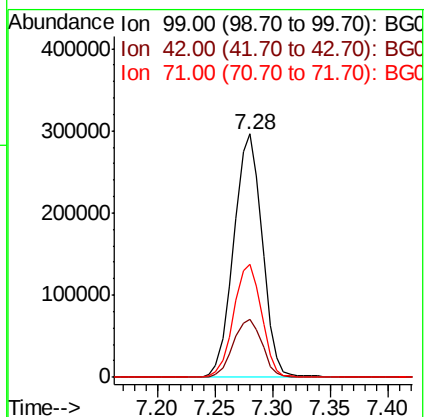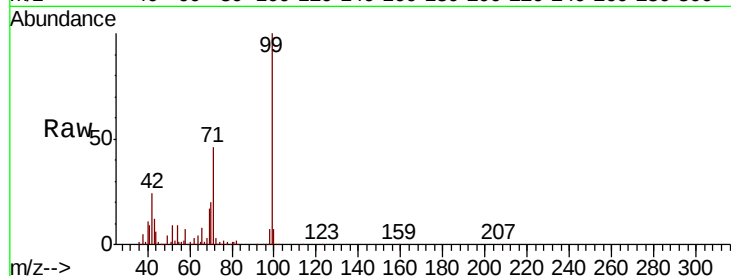

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.02 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29

Tgt Ion: 136 Resp: 170342




Ion Ratio Lower Upper

136 100

137 11.5 9.7 14.5

54 10.8 8.6 12.8

68 5.7 4.8 7.2

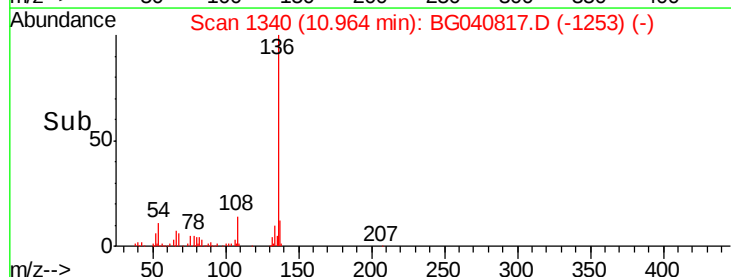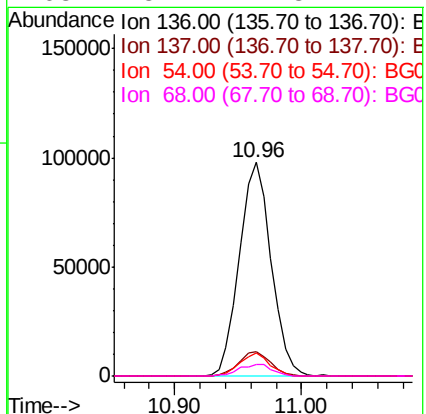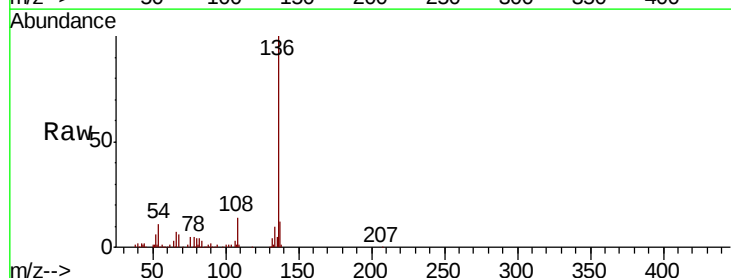







#23
Nitrobenzene-d5
Concen: 120.993 ng
RT: 9.32 min Scan# 1060
Delta R.T. -0.02 min
Lab File: BG040817.D
Acq: 9 May 2019 11:29

Instrument :
BNA_G
ClientSampleId :
PL-02-050719-D

Tot Ion	82	Resp	446049
Ion Ratio	Lower	Upper	
82	100		
128	36.0	28.9	43.3
54	55.1	47.2	70.8

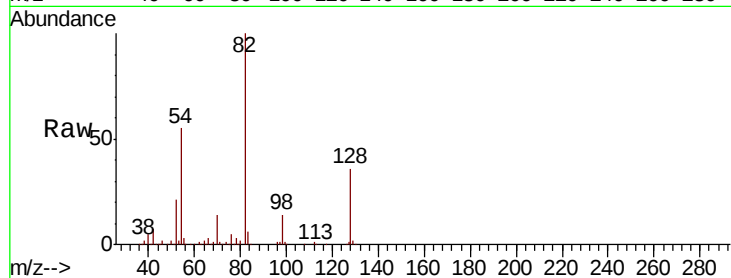


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

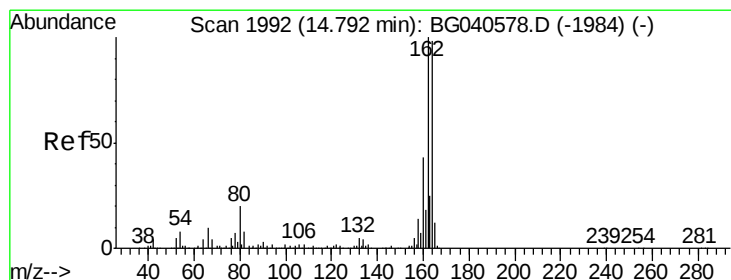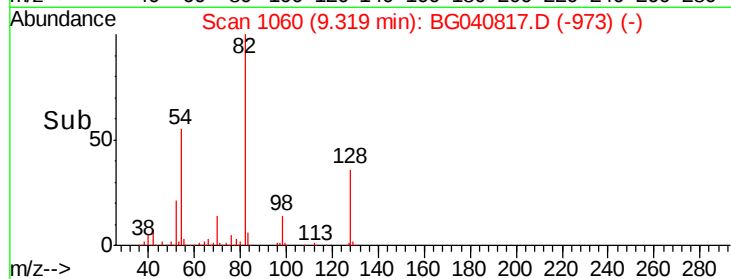
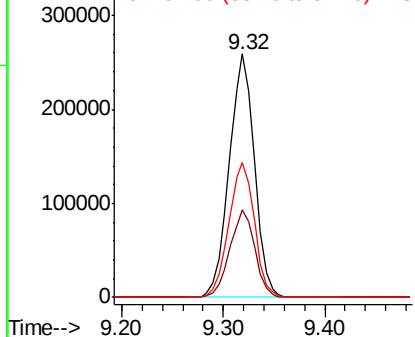


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1987
Delta R.T. -0.03 min
Lab File: BG040817.D
Acq: 9 May 2019 11:29

Tgt Ion	164	Resp	128881
Ion Ratio	Lower	Upper	
164	100		
162	98.7	81.9	122.9
160	45.5	35.4	53.2

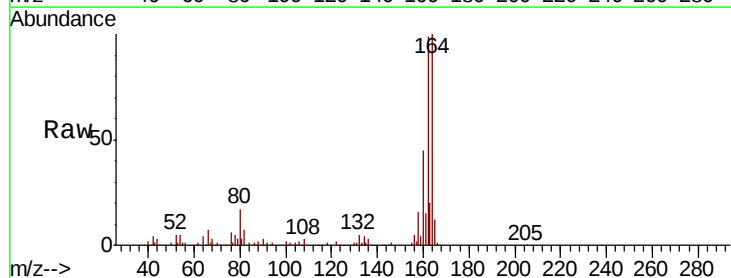

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

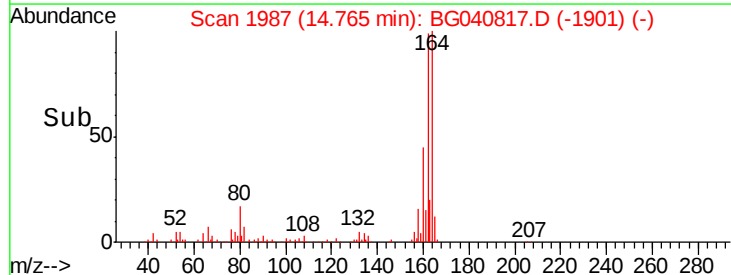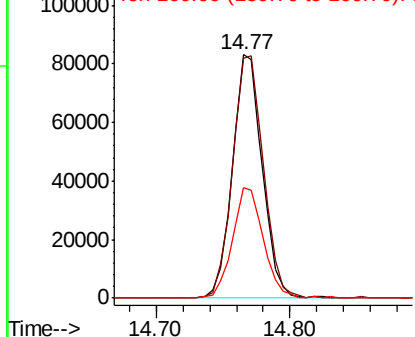




#42
 2,4,6-Tribromophenol
 Concen: 151.467 ng
 RT: 16.25 min Scan# 2240
 Delta R.T. -0.02 min
 Lab File: BG040817.D
 Acq: 9 May 2019 11:29

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-050719-D

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.4	75.9	113.9
141	35.9	32.4	48.6



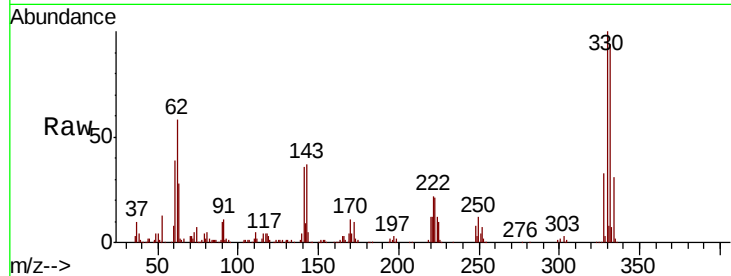


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

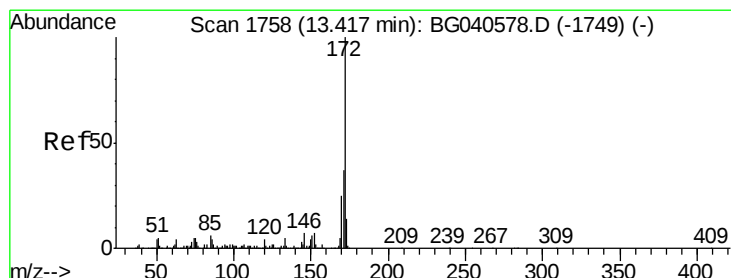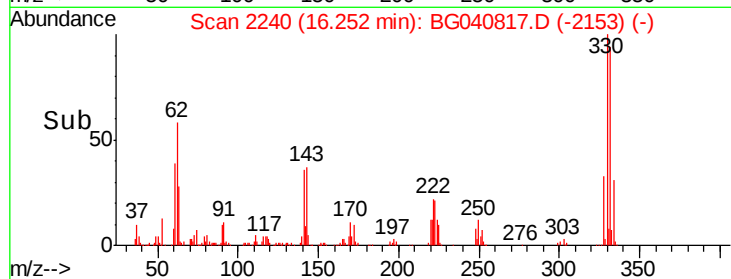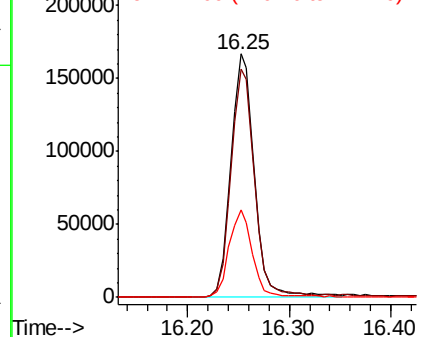

#45
 2-Fluorobiphenyl
 Concen: 110.454 ng
 RT: 13.39 min Scan# 1753
 Delta R.T. -0.03 min
 Lab File: BG040817.D
 Acq: 9 May 2019 11:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.0	29.4	44.2
170	25.5	19.9	29.9


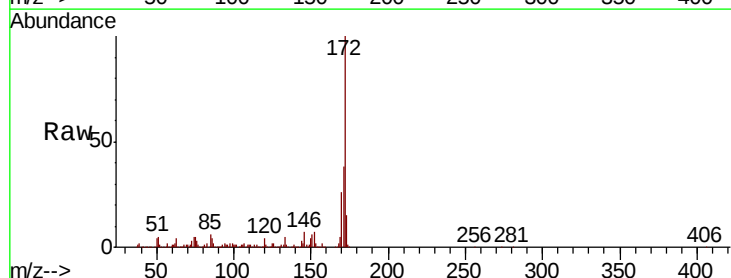



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

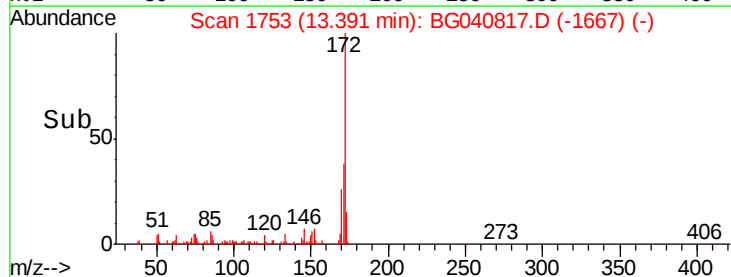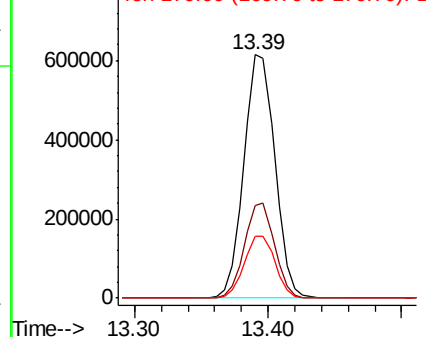

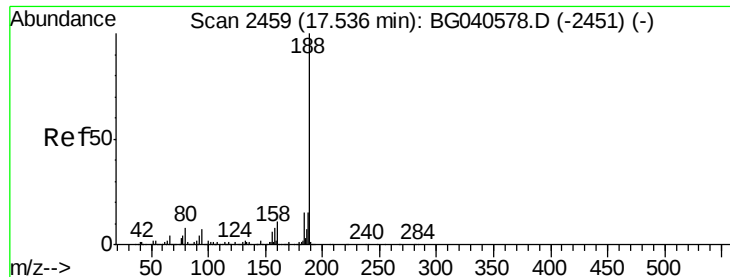

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2454

Delta R.T. -0.03 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29

Instrument :

BNA_G

ClientSampleId :

PL-02-050719-D


Tot Ion:188 Resp: 359002

Ion Ratio Lower Upper

188 100

94 5.6 5.6 8.4




80 7.0 6.4 9.6

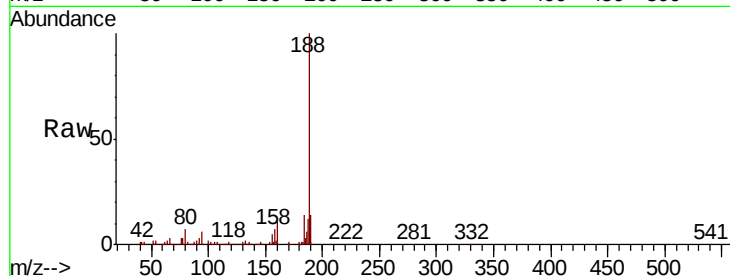

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

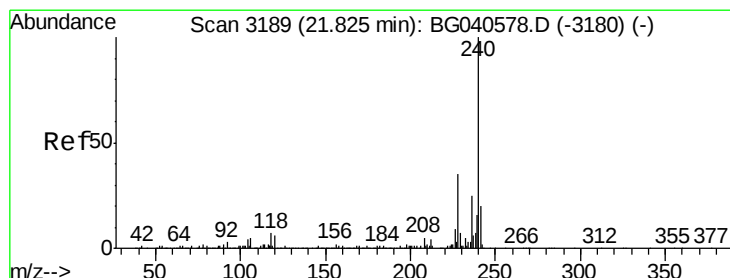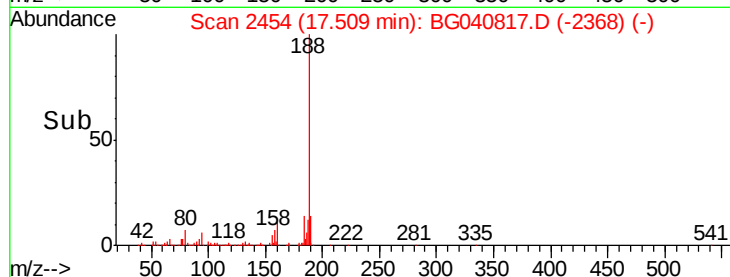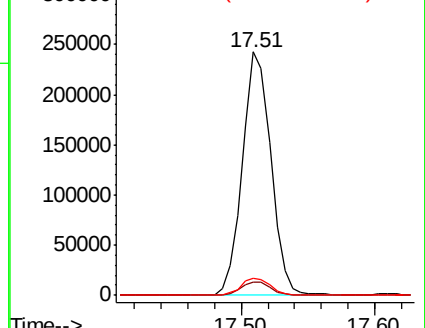

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.79 min Scan# 3183

Delta R.T. -0.03 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29


Tgt Ion:240 Resp: 329716

Ion Ratio Lower Upper

240 100

120 5.7 5.0 7.6



236 27.6 20.3 30.5

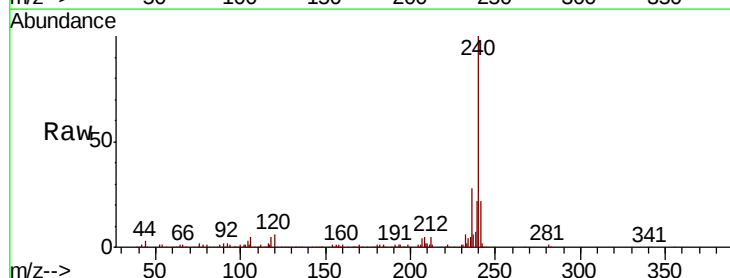


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

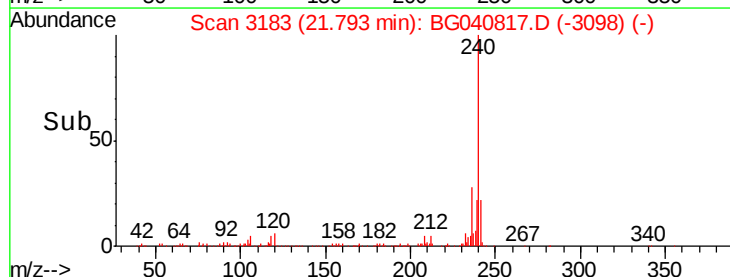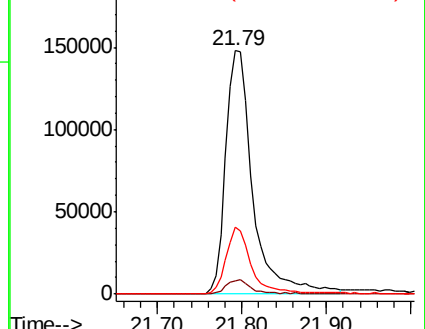

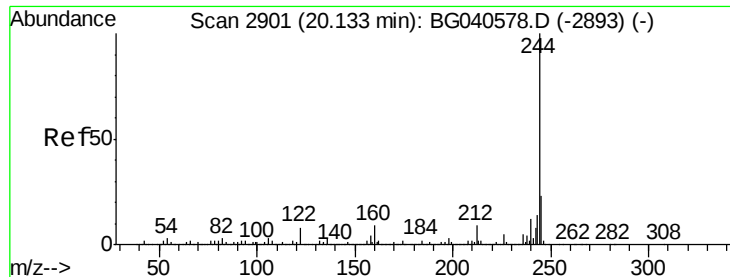

#79

Terphenyl-d14

Concen: 133.129 ng

RT: 20.11 min Scan# 2896

Delta R.T. -0.03 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29

Instrument :

BNA_G

ClientSampleId :

PL-02-050719-D


Tot Ion:244 Resp: 1981332

Ion Ratio Lower Upper

244 100

212 9.4 7.2 10.8




122 8.2 6.6 10.0

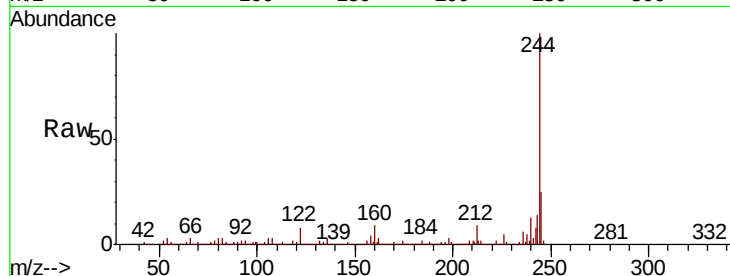

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

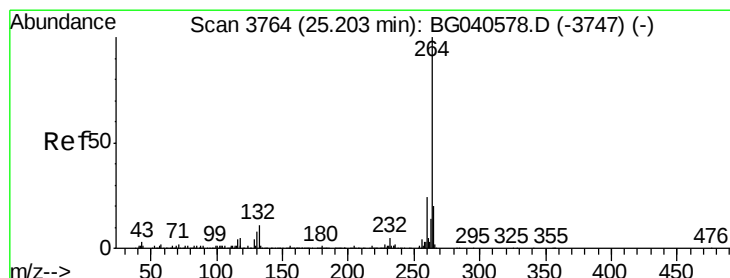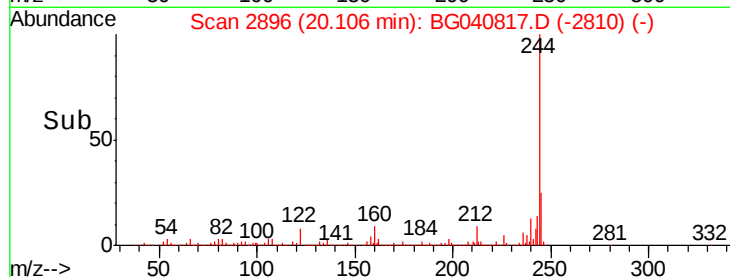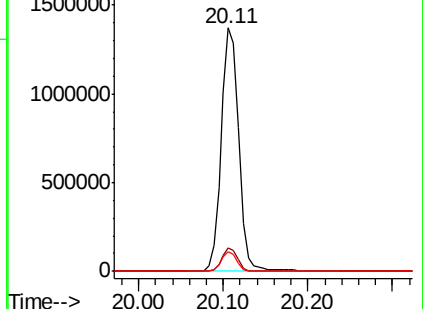

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3754

Delta R.T. -0.06 min

Lab File: BG040817.D

Acq: 9 May 2019 11:29


Tgt Ion:264 Resp: 234385

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 23.6 16.6 25.0

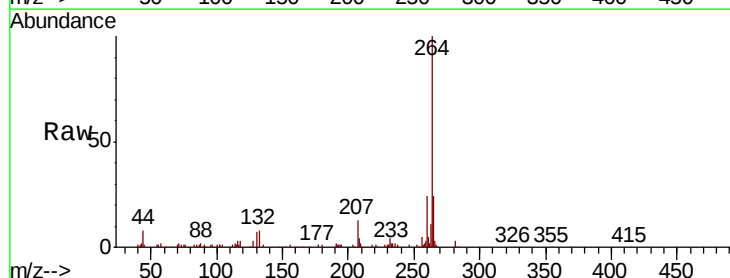

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

