


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG050819\
 Data File : BG040788.D
 Acq On : 8 May 2019 13:10
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

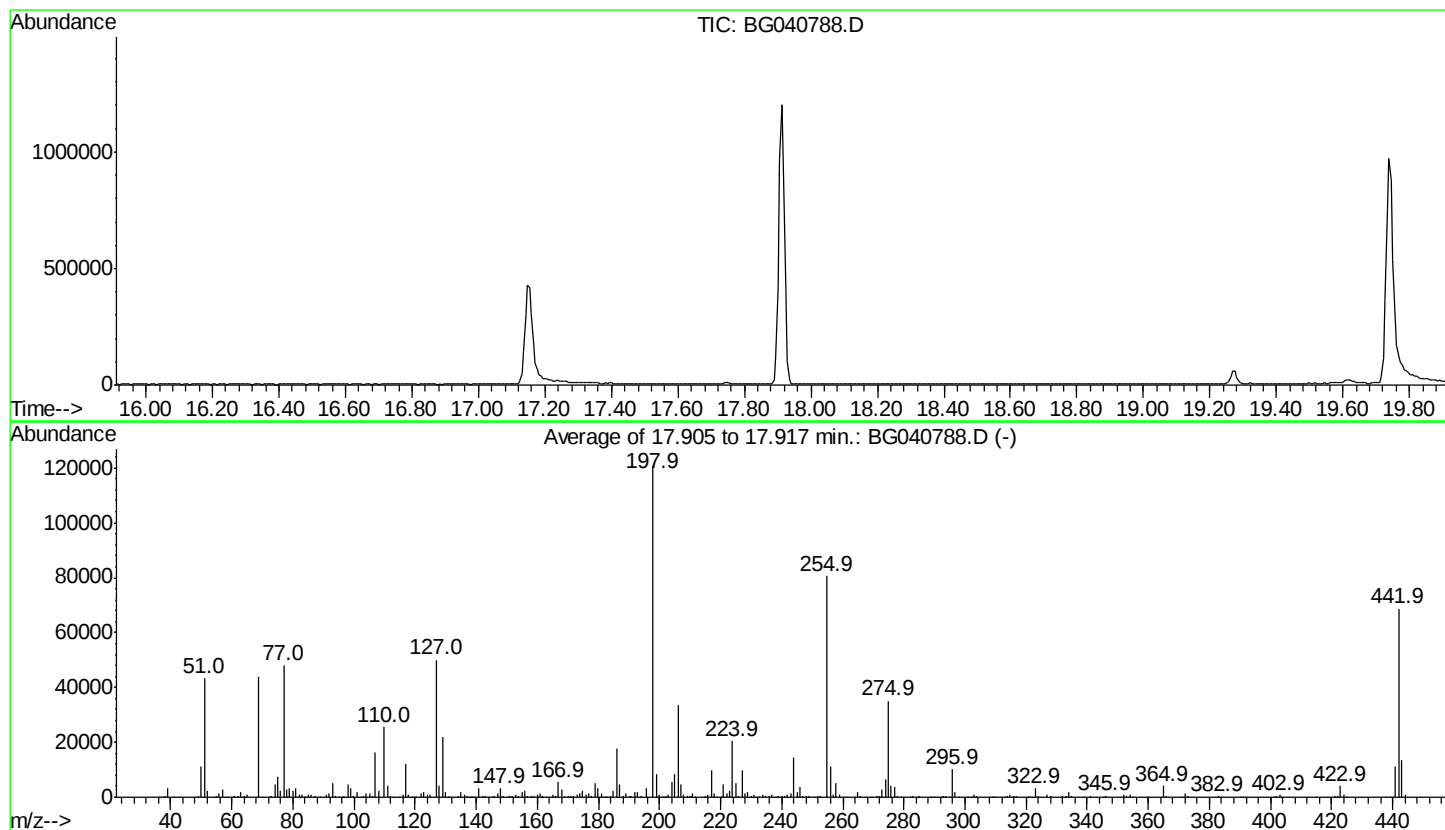

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	43365	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	44058	PASS
70	69	0.00	2	0.4	157	PASS
127	198	10	80	41.4	50013	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120837	PASS
199	198	5	9	6.8	8243	PASS
275	198	10	60	29.1	35173	PASS
365	198	1	100	3.3	3985	PASS
441	198	0.01	100	9.2	11062	PASS
442	198	50	100	56.8	68613	PASS
443	442	15	24	19.7	13488	PASS