


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG050819\
 Data File : BG040803.D
 Acq On : 9 May 2019 2:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

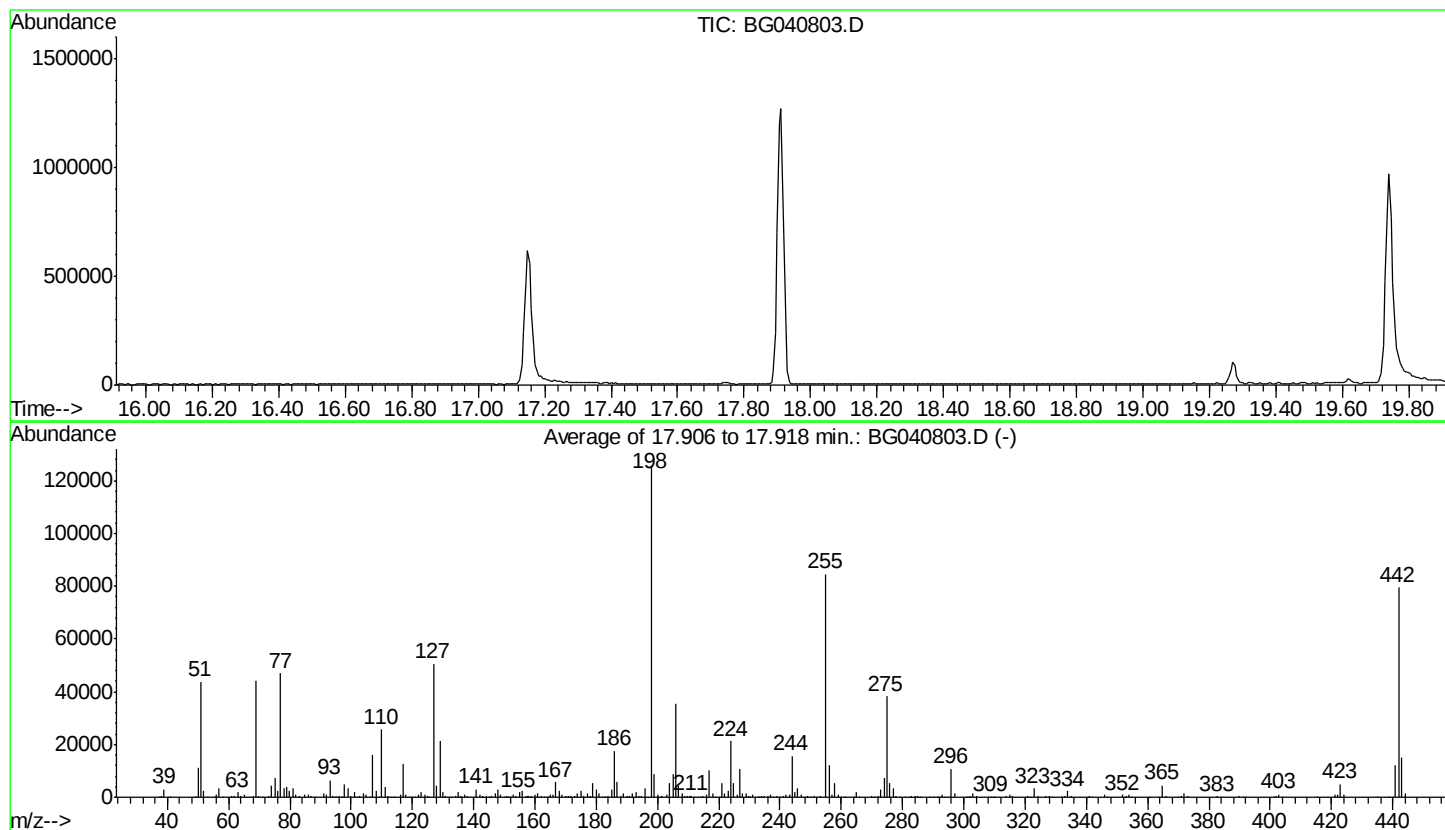

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	43687	PASS
68	69	0.00	2	0.8	363	PASS
69	198	0.00	100	35.3	44408	PASS
70	69	0.00	2	0.9	420	PASS
127	198	10	80	40.3	50650	PASS
197	198	0.00	2	0.2	248	PASS
198	198	100	100	100.0	125714	PASS
199	198	5	9	7.0	8745	PASS
275	198	10	60	30.3	38152	PASS
365	198	1	100	3.6	4576	PASS
441	198	0.01	100	9.6	12073	PASS
442	198	50	100	63.2	79501	PASS
443	442	15	24	18.9	14996	PASS