




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057335.D
Acq On : 8 May 2023 18:06
Operator : CG/JU
Sample : PB152663BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

Quant Time: May 09 00:11:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 08 11:47:25 2023
Response via : Initial Calibration

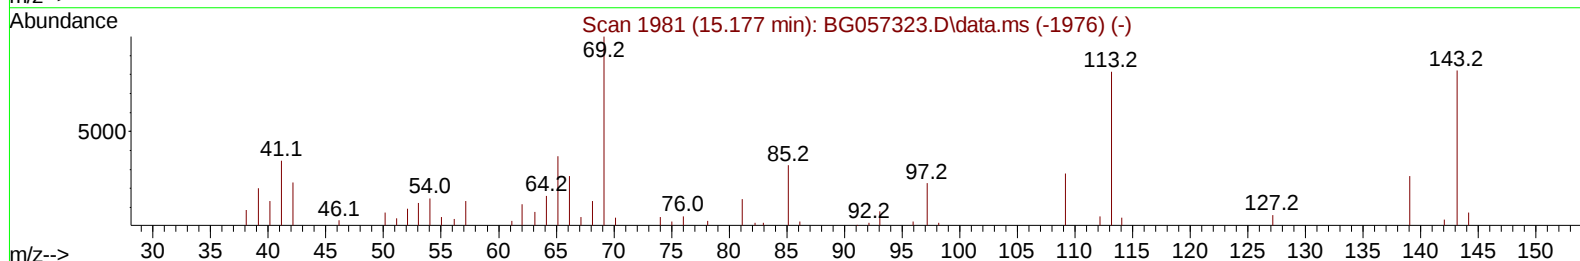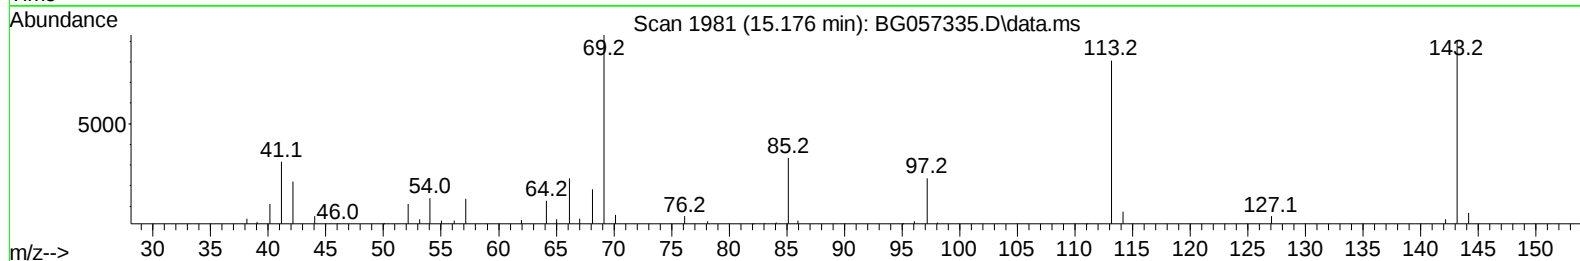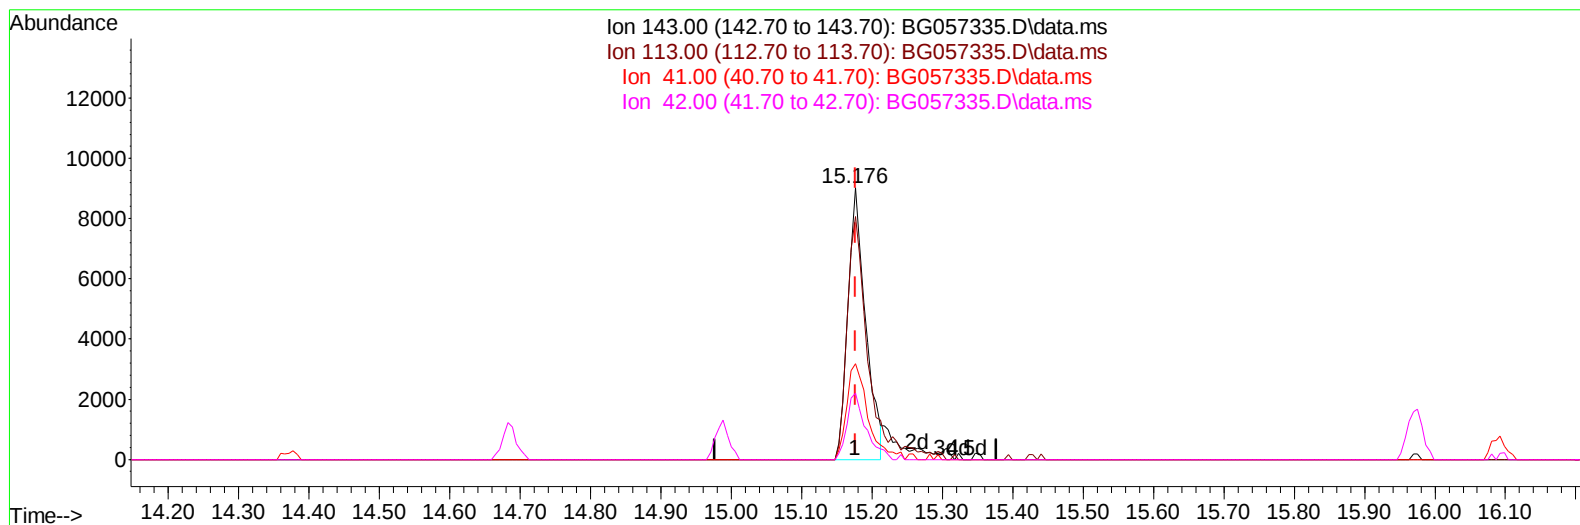

TIC: BG057335.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.176min (-0.001) 20.89 ng/u1

response 15701

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	89.48
41.00	44.40	35.18#
42.00	28.40	24.30




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057335.D
Acq On : 8 May 2023 18:06
Operator : CG/JU
Sample : PB152663BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

Quant Time: May 09 00:11:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 08 11:47:25 2023
Response via : Initial Calibration

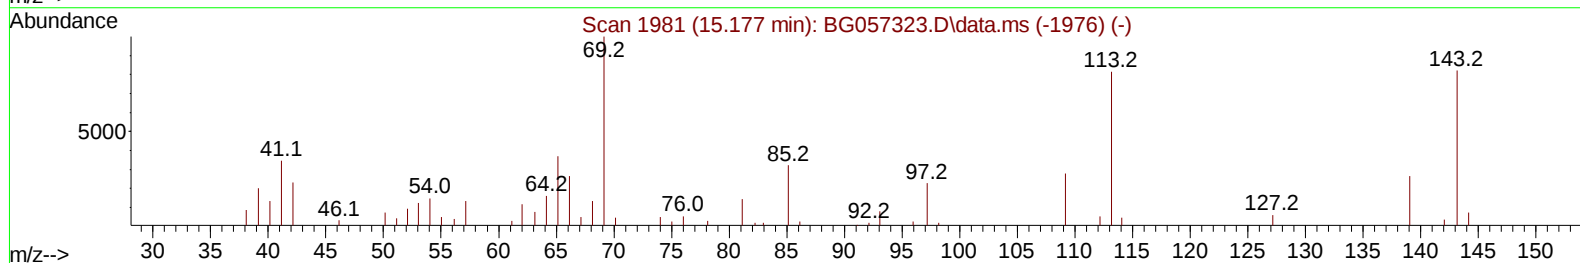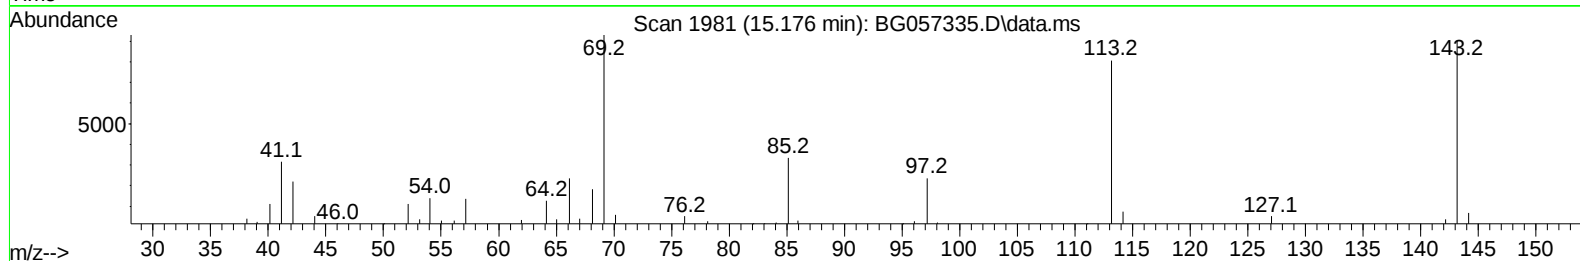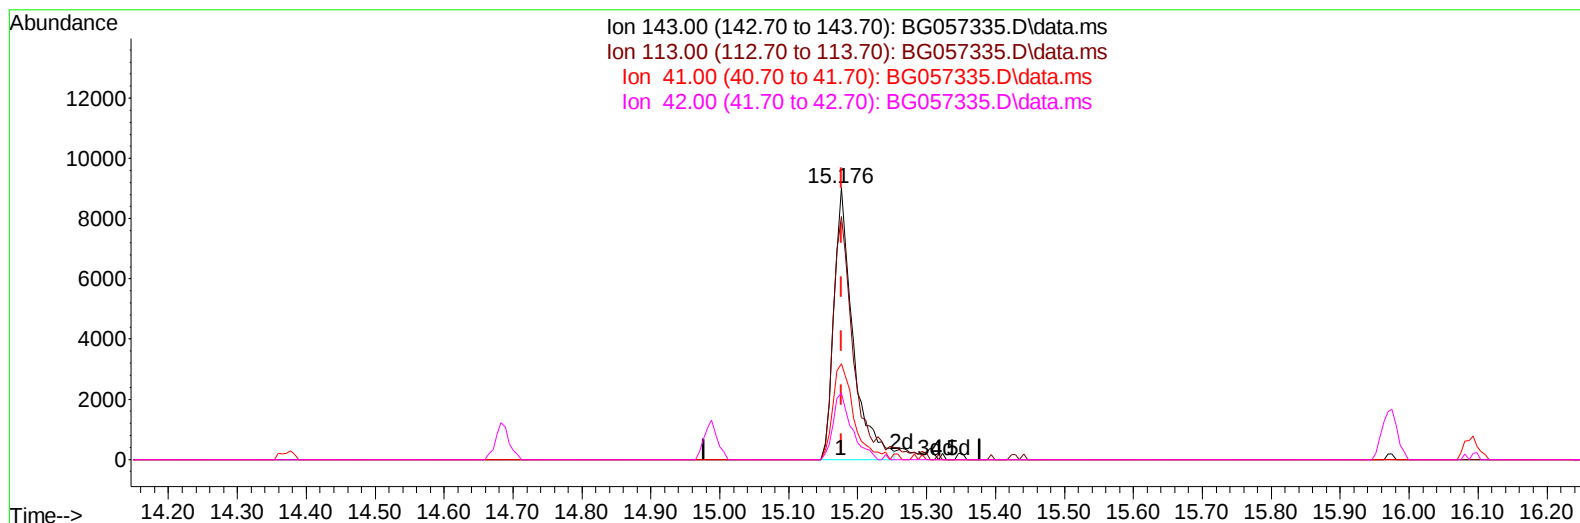

TIC: BG057335.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.176min (-0.001) 22.90 ng/ul m

response 17213

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.60	89.48
41.00	44.40	35.18#
42.00	28.40	24.30

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057335.D
 Acq On : 8 May 2023 18:06
 Operator : CG/JU
 Sample : PB152663BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK663

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/09/2023
 Supervised By :Jagrut Upadhyay 05/09/2023

Quant Time: May 09 00:42:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 08 11:47:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.374	152	18430	20.000	ng/ul	0.00
20) Naphthalene-d8	11.211	136	79270	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.988	164	65165	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.726	188	165830	20.000	ng/ul	0.00
79) Chrysene-d12	22.043	240	154763	20.000	ng/ul	# 0.00
88) Perylene-d12	25.562	264	157496	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.656	96	1757	4.195	ng/uL	0.01
4) Pyridine-d5	4.097	84	11015	8.342	ng/ul	0.00
7) Phenol-d5	7.510	99	41156	23.613	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.675	67	22246	21.700	ng/ul	0.00
11) 2-Chlorophenol-d4	7.898	132	29462	25.651	ng/ul	0.00
15) 4-Methylphenol-d8	9.073	113	32364	24.431	ng/ul	0.00
21) Nitrobenzene-d5	9.549	128	15800	25.029	ng/ul	0.00
24) 2-Nitrophenol-d4	10.277	143	18442	25.032	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.823	165	35231	24.787	ng/ul	0.00
31) 4-Chloroaniline-d4	11.340	131	14248	7.563	ng/ul	0.00
46) Dimethylphthalate-d6	14.371	166	133330	25.822	ng/ul	0.00
49) Acenaphthylene-d8	14.689	160	150451	25.925	ng/ul	0.00
54) 4-Nitrophenol-d4	15.176	143	17213m	22.902	ng/ul	0.00
60) Fluorene-d10	15.975	176	120824	25.118	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.093	200	20917	21.289	ng/ul	0.00
73) Anthracene-d10	17.826	188	208231	27.510	ng/ul	0.00
81) Pyrene-d10	20.093	212	246200	26.801	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.315	264	221268	27.576	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057335.D
Acq On : 8 May 2023 18:06
Operator : CG/JU
Sample : PB152663BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK663

Manual IntegrationsAPPROVED

Quant Time: May 09 00:42:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 08 11:47:25 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

