

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057324.D
 Acq On : 8 May 2023 9:50
 Operator : CG/JU
 Sample : PB152593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.650	13	19	26	rVB2	3663	5143	1.01%	0.101%
2	3.702	26	28	34	rVB2	514	790	0.16%	0.016%
3	3.979	74	75	79	rBB	623	515	0.10%	0.010%
4	4.090	91	94	111	rBV	36662	67281	13.25%	1.323%
5	4.449	152	155	158	rBB2	1016	1037	0.20%	0.020%
6	7.515	670	677	690	rBB	61495	109593	21.58%	2.155%
7	7.674	698	704	712	rBB	43395	73100	14.40%	1.437%
8	7.897	737	742	751	rBB	59952	102069	20.10%	2.007%
9	8.373	817	823	831	rBB	59979	97744	19.25%	1.922%
10	9.072	936	942	955	rBV2	77031	138713	27.32%	2.727%
11	9.553	1016	1024	1032	rBB	61563	109579	21.58%	2.155%
12	10.282	1141	1148	1155	rVB	57959	98275	19.35%	1.932%
13	10.828	1234	1241	1257	rVB2	81068	147341	29.01%	2.897%
14	11.210	1297	1306	1315	rVB	89146	158873	31.29%	3.124%
15	11.339	1321	1328	1339	rVB	76340	138600	27.29%	2.725%
16	12.767	1568	1571	1575	rBV2	1205	1789	0.35%	0.035%
17	14.370	1838	1844	1855	rVB	177543	251519	49.53%	4.945%
18	14.688	1890	1898	1909	rVB2	189664	302808	59.63%	5.954%
19	14.987	1943	1949	1958	rVB	171496	262854	51.76%	5.168%
20	15.175	1976	1981	1993	rBV2	42156	87784	17.29%	1.726%
21	15.281	1998	1999	2005	rVB2	905	1035	0.20%	0.020%
22	15.974	2110	2117	2125	rVB	246538	382951	75.41%	7.530%
23	16.092	2133	2137	2148	rBV	50059	81223	15.99%	1.597%
24	16.209	2155	2157	2162	rVB2	558	601	0.12%	0.012%
25	17.031	2294	2297	2302	rBV	570	894	0.18%	0.018%
26	17.507	2373	2378	2385	rVV	462	970	0.19%	0.019%
27	17.637	2395	2400	2401	rBV	487	555	0.11%	0.011%
28	17.725	2409	2415	2425	rVB	218413	339308	66.82%	6.672%
29	17.825	2425	2432	2440	rBV	284732	430630	84.80%	8.467%
30	18.324	2515	2517	2519	rBV	434	521	0.10%	0.010%
31	19.217	2667	2669	2672	rVB	694	814	0.16%	0.016%
32	19.305	2681	2684	2686	rVB2	957	986	0.19%	0.019%
33	19.510	2717	2719	2721	rVB2	1317	685	0.13%	0.013%
34	19.587	2731	2732	2735	rBV3	984	1113	0.22%	0.022%
35	19.622	2735	2738	2740	rVV	595	715	0.14%	0.014%
36	19.663	2740	2745	2748	rVB3	3353	4712	0.93%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057324.D
 Acq On : 8 May 2023 9:50
 Operator : CG/JU
 Sample : PB152593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	19.734	2753	2757	2760	rVB3	2829	3692	0.73%	0.073%
38	19.933	2790	2791	2793	rBV2	827	720	0.14%	0.014%
39	19.963	2793	2796	2800	rVB4	1349	2276	0.45%	0.045%
40	20.033	2806	2808	2810	rBV2	1108	904	0.18%	0.018%
41	20.092	2812	2818	2827	rVV	366886	507812	100.00%	9.985%
42	20.186	2832	2834	2835	rVV2	1119	666	0.13%	0.013%
43	20.221	2838	2840	2843	rVB4	1032	807	0.16%	0.016%
44	20.245	2843	2844	2847	rBV3	1399	1349	0.27%	0.027%
45	20.309	2854	2855	2857	rBV	1637	997	0.20%	0.020%
46	20.356	2861	2863	2865	rBV2	1603	1263	0.25%	0.025%
47	20.445	2876	2878	2884	rBV5	1121	2471	0.49%	0.049%
48	20.527	2890	2892	2893	rBV2	1070	931	0.18%	0.018%
49	20.815	2940	2941	2944	rBV3	1856	1987	0.39%	0.039%
50	21.097	2988	2989	2990	rBV	1412	601	0.12%	0.012%
51	21.285	3019	3021	3022	rBV2	2323	1373	0.27%	0.027%
52	21.337	3028	3030	3032	rBV3	2957	3402	0.67%	0.067%
53	22.042	3143	3150	3156	rBV2	193298	356107	70.13%	7.002%
54	22.783	3274	3276	3279	rBV4	2214	2067	0.41%	0.041%
55	22.877	3290	3292	3294	rBV3	2195	1896	0.37%	0.037%
56	23.053	3320	3322	3324	rBV3	2425	2120	0.42%	0.042%
57	23.106	3330	3331	3334	rBV3	2198	1287	0.25%	0.025%
58	23.147	3336	3338	3340	rBV3	2495	2912	0.57%	0.057%
59	23.241	3353	3354	3358	rBV4	2536	3227	0.64%	0.063%
60	23.446	3387	3389	3393	rBV4	2614	2716	0.53%	0.053%
61	25.250	3694	3696	3697	rBV2	2778	2546	0.50%	0.050%
62	25.314	3698	3707	3719	rVB2	156852	448872	88.39%	8.826%
63	25.420	3724	3725	3726	rBV	2463	1079	0.21%	0.021%
64	25.561	3739	3749	3759	rVB	104910	313007	61.64%	6.154%
65	26.037	3828	3830	3833	rBV4	2303	1914	0.38%	0.038%
66	27.758	4121	4123	4124	rVB2	2285	1447	0.28%	0.028%
67	28.069	4174	4176	4177	rVB2	2654	1254	0.25%	0.025%
68	28.586	4262	4264	4265	rBV2	2419	1652	0.33%	0.032%
69	30.419	4574	4576	4578	rBV3	2154	1589	0.31%	0.031%
70	31.518	4761	4763	4764	rBV2	2113	1034	0.20%	0.020%
71	31.905	4826	4829	4830	rBV3	3100	3455	0.68%	0.068%
72	32.076	4856	4858	4859	rBV	2329	1340	0.26%	0.026%



Sum of corrected areas: 5085892

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057324.D
Acq On : 8 May 2023 9:50
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

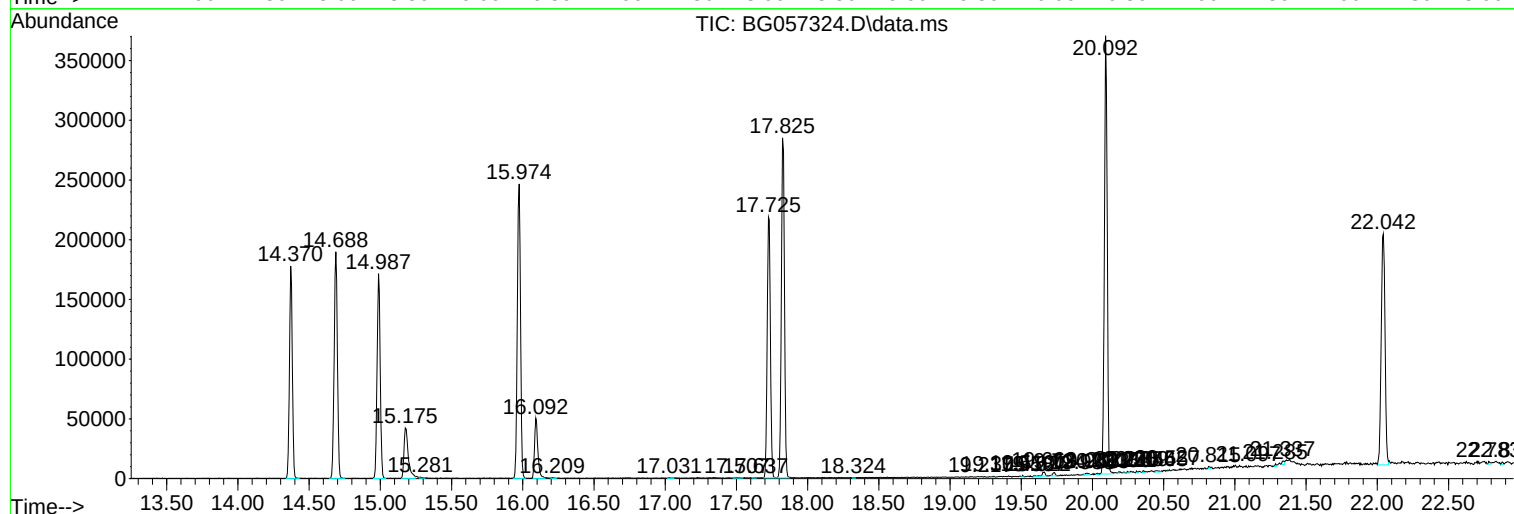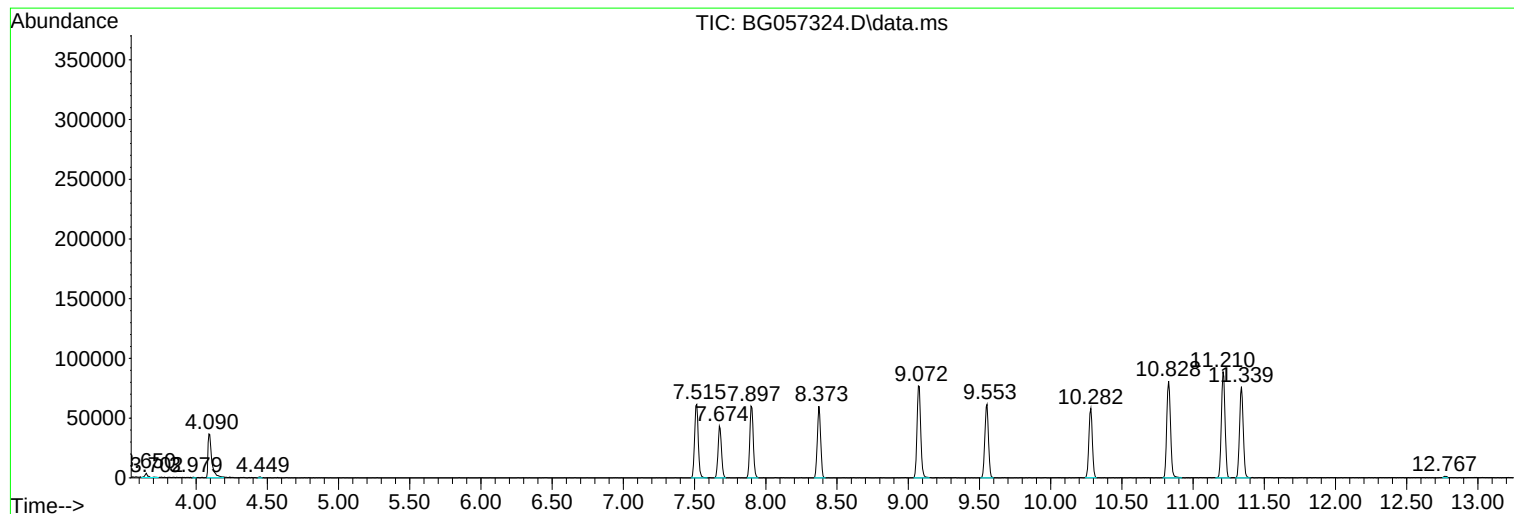

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057324.D
Acq On : 8 May 2023 9:50
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057324.D
Acq On : 8 May 2023 9:50
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------