

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057344.D
 Acq On : 9 May 2023 00:20
 Operator : CG/JU
 Sample : 02619-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFZD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.655	17	20	25	rVB3	3160	3968	0.59%	0.074%
2	3.755	35	37	39	rBV2	1044	1155	0.17%	0.021%
3	4.102	94	96	104	rVB2	4982	7275	1.08%	0.135%
4	4.260	122	123	126	rVB3	1212	931	0.14%	0.017%
5	4.442	151	154	159	rBV4	1579	1804	0.27%	0.034%
6	4.724	199	202	203	rVB2	830	691	0.10%	0.013%
7	4.748	203	206	207	rBV2	743	783	0.12%	0.015%
8	6.751	543	547	552	rBV2	573	1138	0.17%	0.021%
9	7.515	671	677	684	rVB2	10848	18627	2.77%	0.347%
10	7.673	697	704	711	rBV	47812	79386	11.81%	1.478%
11	7.896	736	742	750	rBV	44477	77592	11.55%	1.444%
12	8.372	817	823	830	rBB2	57455	96688	14.39%	1.800%
13	9.071	935	942	952	rBB	36046	61951	9.22%	1.153%
14	9.547	1016	1023	1031	rBB	67298	117298	17.45%	2.183%
15	10.276	1140	1147	1155	rBB	54228	97578	14.52%	1.816%
16	10.828	1233	1241	1252	rBV	76943	135547	20.17%	2.523%
17	11.210	1298	1306	1315	rVB	87938	152679	22.72%	2.842%
18	11.339	1321	1328	1335	rBV	46636	83820	12.47%	1.560%
19	11.386	1335	1336	1342	rVB	526	802	0.12%	0.015%
20	12.766	1566	1571	1572	rBV3	1201	1626	0.24%	0.030%
21	13.841	1750	1754	1758	rVB2	1430	1895	0.28%	0.035%
22	14.370	1838	1844	1854	rVB	192968	280709	41.77%	5.225%
23	14.681	1890	1897	1905	rBV2	203725	325821	48.48%	6.065%
24	14.987	1942	1949	1957	rVB	162906	256580	38.18%	4.776%
25	15.187	1979	1983	1992	rBV3	6103	12572	1.87%	0.234%
26	15.968	2110	2116	2125	rBV	301149	449926	66.95%	8.375%
27	16.085	2132	2136	2147	rBV	71729	114066	16.97%	2.123%
28	16.209	2154	2157	2159	rVB2	727	801	0.12%	0.015%
29	17.724	2409	2415	2422	rVV	228799	340050	50.60%	6.329%
30	17.824	2425	2432	2441	rVV	377667	560174	83.36%	10.427%
31	18.182	2488	2493	2496	rBV2	536	753	0.11%	0.014%
32	19.657	2740	2744	2748	rVV3	4492	6049	0.90%	0.113%
33	19.727	2751	2756	2761	rBV3	3976	5794	0.86%	0.108%
34	19.915	2787	2788	2792	rBV3	548	709	0.11%	0.013%
35	19.951	2792	2794	2796	rVV2	1080	1044	0.16%	0.019%
36	20.027	2805	2807	2810	rBV2	1125	1370	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057344.D
 Acq On : 9 May 2023 00:20
 Operator : CG/JU
 Sample : 02619-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFZD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	20.092	2811	2818	2827	rVV	468940	672025	100.00%	12.509%
38	20.180	2831	2833	2834	rVB2	1312	791	0.12%	0.015%
39	20.315	2854	2856	2858	rBV3	1169	837	0.12%	0.016%
40	20.380	2865	2867	2870	rVB3	1395	1012	0.15%	0.019%
41	20.591	2899	2903	2905	rVB4	1037	1120	0.17%	0.021%
42	20.667	2914	2916	2919	rVB4	1473	1063	0.16%	0.020%
43	20.773	2932	2934	2937	rBV3	905	811	0.12%	0.015%
44	20.996	2970	2972	2976	rVB5	2730	2697	0.40%	0.050%
45	21.184	3000	3004	3006	rBV3	1480	1933	0.29%	0.036%
46	21.231	3010	3012	3014	rVV3	1594	1416	0.21%	0.026%
47	21.455	3049	3050	3052	rBV2	2430	1398	0.21%	0.026%
48	21.590	3071	3073	3074	rBV2	1314	759	0.11%	0.014%
49	21.678	3086	3088	3091	rBV3	1317	1303	0.19%	0.024%
50	21.707	3091	3093	3096	rVB4	1436	1160	0.17%	0.022%
51	21.736	3096	3098	3099	rBV2	1590	1032	0.15%	0.019%
52	21.784	3105	3106	3110	rBV4	1578	2113	0.31%	0.039%
53	22.036	3142	3149	3159	rBV	216246	368069	54.77%	6.851%
54	22.218	3178	3180	3181	rBV2	1625	1484	0.22%	0.028%
55	22.324	3196	3198	3202	rVB4	1766	2222	0.33%	0.041%
56	22.371	3202	3206	3209	rBV5	2009	2808	0.42%	0.052%
57	22.676	3256	3258	3259	rBV2	2243	1856	0.28%	0.035%
58	22.700	3259	3262	3263	rVV2	2016	2379	0.35%	0.044%
59	23.005	3312	3314	3315	rBV2	1622	1384	0.21%	0.026%
60	23.287	3360	3362	3364	rVB3	2122	1352	0.20%	0.025%
61	23.405	3381	3382	3384	rVB2	2013	1020	0.15%	0.019%
62	23.428	3384	3386	3387	rBV2	1471	779	0.12%	0.014%
63	23.475	3393	3394	3398	rBV5	1817	2117	0.32%	0.039%
64	23.563	3407	3409	3411	rBV4	1881	1202	0.18%	0.022%
65	23.757	3440	3442	3443	rBV2	1544	1354	0.20%	0.025%
66	23.887	3462	3464	3466	rBV3	1678	1620	0.24%	0.030%
67	24.251	3524	3526	3528	rVB2	2426	1815	0.27%	0.034%
68	25.067	3663	3665	3669	rBV5	1820	2523	0.38%	0.047%
69	25.314	3695	3707	3719	rBV2	213311	612585	91.16%	11.402%
70	25.467	3731	3733	3735	rBV3	2178	1953	0.29%	0.036%
71	25.555	3739	3748	3761	rVB2	112107	342289	50.93%	6.371%
72	26.025	3826	3828	3830	rVB3	2662	1517	0.23%	0.028%
73	26.677	3935	3939	3940	rBV3	3354	3829	0.57%	0.071%
74	26.994	3992	3993	3995	rBV2	1702	1355	0.20%	0.025%
75	27.200	4026	4028	4030	rBV3	1714	2006	0.30%	0.037%
76	27.311	4046	4047	4048	rVB	2089	736	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057344.D
Acq On : 9 May 2023 00:20
Operator : CG/JU
Sample : 02619-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Title : SVOA CALIBRATION

77	27.576	4090	4092	4096	rBV5	2045	2130	0.32%	0.040%
78	27.781	4126	4127	4130	rBV3	1855	2094	0.31%	0.039%
79	27.840	4135	4137	4138	rBV2	1742	857	0.13%	0.016%
80	29.085	4347	4349	4352	rBV4	2436	1928	0.29%	0.036%
81	29.573	4430	4432	4434	rBV2	1930	1459	0.22%	0.027%
82	30.601	4605	4607	4608	rVB2	2344	1228	0.18%	0.023%
83	30.619	4608	4610	4611	rBV2	2554	2334	0.35%	0.043%
84	30.871	4651	4653	4655	rBV3	1994	2002	0.30%	0.037%
85	30.918	4659	4661	4663	rBV3	2195	2486	0.37%	0.046%
86	31.811	4812	4813	4815	rBV2	1751	1631	0.24%	0.030%
87	31.876	4822	4824	4825	rVB2	2045	997	0.15%	0.019%
88	32.357	4904	4906	4908	rBV2	2584	1942	0.29%	0.036%



Sum of corrected areas: 5372464

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057344.D
Acq On : 9 May 2023 00:20
Operator : CG/JU
Sample : 02619-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

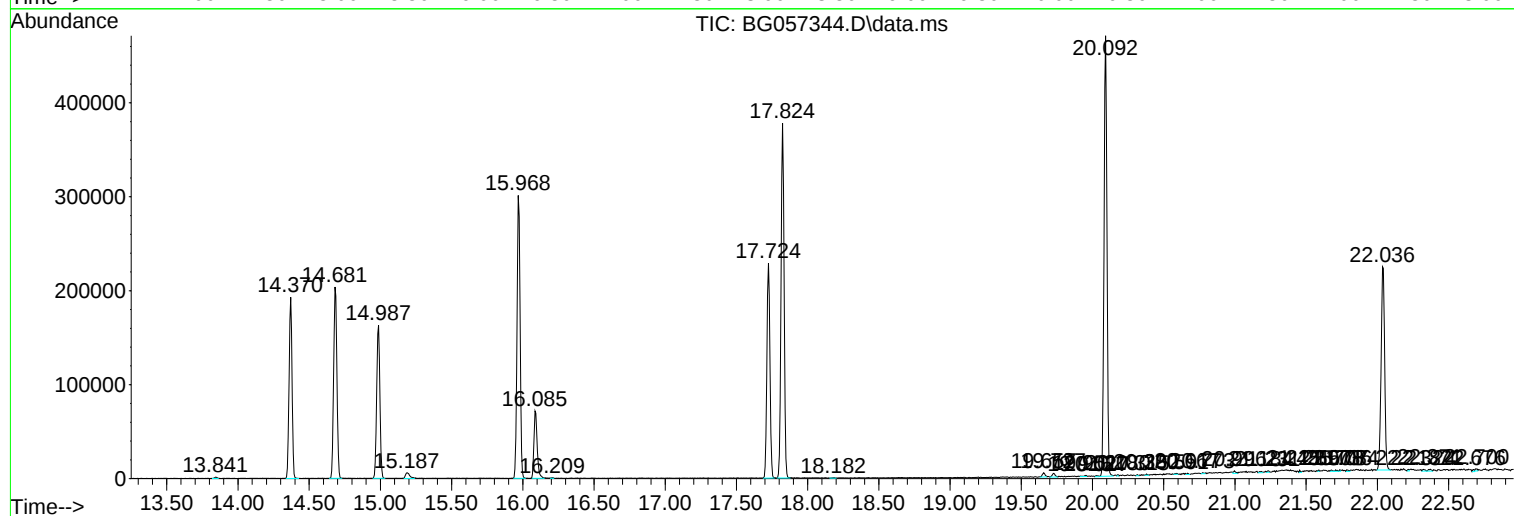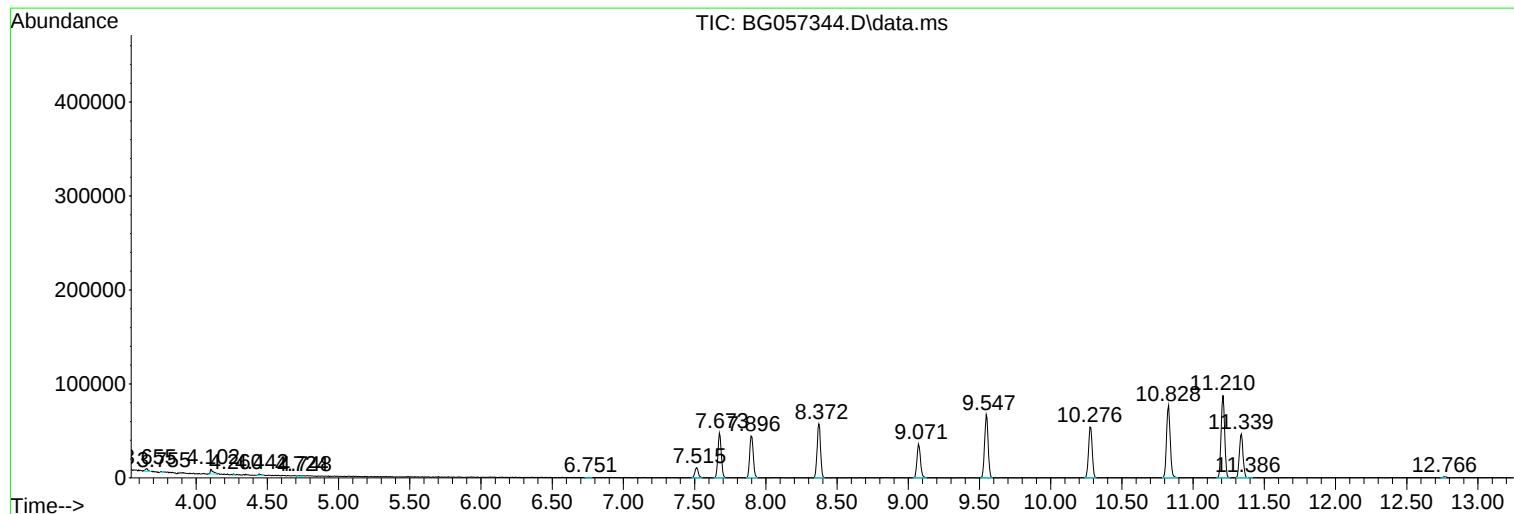

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057344.D
Acq On : 9 May 2023 00:20
Operator : CG/JU
Sample : 02619-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057344.D
Acq On : 9 May 2023 00:20
Operator : CG/JU
Sample : 02619-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------