

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057345.D
 Acq On : 9 May 2023 1:02
 Operator : CG/JU
 Sample : 02619-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFZE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.652	15	19	22	rBV	2243	2987	0.42%	0.053%
2	3.864	51	55	57	rBV	716	753	0.10%	0.013%
3	3.964	67	72	77	rBV2	430	740	0.10%	0.013%
4	4.104	94	96	103	rBV3	3330	5982	0.83%	0.105%
5	4.181	107	109	112	rVB	914	782	0.11%	0.014%
6	4.451	151	155	156	rBV2	999	1149	0.16%	0.020%
7	7.512	671	676	684	rBB2	13649	22608	3.15%	0.399%
8	7.676	698	704	712	rBB	51334	86525	12.06%	1.526%
9	7.899	736	742	751	rBB	52106	89034	12.41%	1.570%
10	8.369	816	822	830	rBB	54102	87746	12.23%	1.548%
11	9.074	935	942	950	rBV	43115	74883	10.44%	1.321%
12	9.550	1015	1023	1030	rBV	75620	131469	18.32%	2.319%
13	10.279	1140	1147	1154	rVB	64558	110577	15.41%	1.950%
14	10.825	1234	1240	1253	rBB	86140	155285	21.64%	2.739%
15	11.207	1299	1305	1315	rVB	78020	140652	19.60%	2.481%
16	11.336	1321	1327	1335	rBV	45392	80381	11.20%	1.418%
17	12.769	1566	1571	1577	rVB3	1280	2351	0.33%	0.041%
18	13.850	1750	1755	1760	rVB2	783	1035	0.14%	0.018%
19	14.367	1837	1843	1850	rBV	217431	311956	43.48%	5.502%
20	14.684	1890	1897	1907	rBV	239493	373335	52.03%	6.584%
21	14.984	1941	1948	1956	rVB	158324	237300	33.07%	4.185%
22	15.184	1977	1982	1989	rBV4	8269	15438	2.15%	0.272%
23	15.236	1989	1991	1995	rVB2	814	755	0.11%	0.013%
24	15.971	2109	2116	2123	rBV	333164	498691	69.50%	8.795%
25	16.088	2131	2136	2148	rVB	81399	129548	18.06%	2.285%
26	16.212	2154	2157	2159	rVB2	849	882	0.12%	0.016%
27	16.317	2172	2175	2179	rVB2	2294	3014	0.42%	0.053%
28	17.439	2363	2366	2368	rVB2	1209	1004	0.14%	0.018%
29	17.727	2408	2415	2421	rBV	213907	318080	44.33%	5.610%
30	17.827	2425	2432	2444	rVB	399509	607812	84.71%	10.719%
31	18.626	2566	2568	2571	rBV2	704	724	0.10%	0.013%
32	19.472	2708	2712	2715	rBV2	907	1394	0.19%	0.025%
33	19.625	2734	2738	2740	rBV3	612	779	0.11%	0.014%
34	19.654	2740	2743	2747	rVB3	5341	7643	1.07%	0.135%
35	19.725	2751	2755	2760	rBV	4671	7283	1.02%	0.128%
36	19.954	2791	2794	2796	rBV5	1761	1429	0.20%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
 Data File : BG057345.D
 Acq On : 9 May 2023 1:02
 Operator : CG/JU
 Sample : 02619-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFZE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	20.089	2811	2817	2823	rBV	496190	717514	100.00%	12.654%
38	20.324	2854	2857	2860	rVB3	1241	1616	0.23%	0.028%
39	20.359	2860	2863	2864	rBV	1310	1178	0.16%	0.021%
40	20.559	2895	2897	2899	rVB3	1394	891	0.12%	0.016%
41	20.794	2935	2937	2939	rVB3	1374	1446	0.20%	0.026%
42	20.999	2968	2972	2975	rBV6	1916	2389	0.33%	0.042%
43	21.311	3023	3025	3026	rBV2	1653	843	0.12%	0.015%
44	21.328	3026	3028	3029	rBV2	1486	827	0.12%	0.015%
45	21.522	3059	3061	3063	rVB3	2158	1519	0.21%	0.027%
46	21.546	3063	3065	3066	rBV	2242	1422	0.20%	0.025%
47	21.563	3066	3068	3069	rVB	1630	974	0.14%	0.017%
48	21.851	3115	3117	3120	rBV4	1758	2513	0.35%	0.044%
49	22.039	3142	3149	3159	rVB	204426	344544	48.02%	6.076%
50	22.151	3166	3168	3169	rBV2	1479	823	0.11%	0.015%
51	22.233	3181	3182	3184	rVB2	1730	1174	0.16%	0.021%
52	23.337	3368	3370	3371	rBV	1348	1027	0.14%	0.018%
53	23.566	3406	3409	3414	rVB6	3400	5526	0.77%	0.097%
54	24.448	3552	3559	3567	rVB6	4302	11426	1.59%	0.202%
55	24.565	3577	3579	3582	rBV3	1585	2342	0.33%	0.041%
56	25.311	3693	3706	3719	rBV2	218781	669182	93.26%	11.802%
57	25.476	3728	3734	3737	rBV8	4266	9688	1.35%	0.171%
58	25.552	3737	3747	3761	rVB2	108673	332193	46.30%	5.859%
59	25.869	3799	3801	3804	rBV3	1344	1046	0.15%	0.018%
60	25.904	3806	3807	3811	rBV4	2430	2399	0.33%	0.042%
61	26.421	3893	3895	3896	rBV2	1667	965	0.13%	0.017%
62	26.627	3929	3930	3932	rBV	1770	1230	0.17%	0.022%
63	26.656	3932	3935	3936	rBV2	2151	2161	0.30%	0.038%
64	26.709	3938	3944	3948	rVV7	3751	8080	1.13%	0.142%
65	26.833	3963	3965	3967	rVB3	1716	1446	0.20%	0.026%
66	26.885	3973	3974	3978	rBV4	2118	1340	0.19%	0.024%
67	27.485	4075	4076	4078	rBV2	1667	1389	0.19%	0.024%
68	27.508	4078	4080	4081	rVV	2421	1354	0.19%	0.024%
69	27.526	4081	4083	4086	rVB4	1656	1218	0.17%	0.021%
70	27.955	4154	4156	4159	rBV4	1403	1404	0.20%	0.025%
71	28.107	4180	4182	4184	rBV2	2037	1835	0.26%	0.032%
72	28.824	4302	4304	4305	rBV2	1608	913	0.13%	0.016%
73	29.124	4354	4355	4357	rBV2	2426	1240	0.17%	0.022%
74	29.282	4380	4382	4385	rVB3	2405	2519	0.35%	0.044%
75	29.306	4385	4386	4388	rBV2	2306	1841	0.26%	0.032%
76	29.406	4401	4403	4405	rBV2	1508	1223	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057345.D
Acq On : 9 May 2023 1:02
Operator : CG/JU
Sample : 02619-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Title : SVOA CALIBRATION

77	29.717	4455	4456	4460	rBV3	1754	2164	0.30%	0.038%
78	29.764	4462	4464	4466	rBV3	1455	1109	0.15%	0.020%
79	30.187	4535	4536	4539	rVB3	2215	1441	0.20%	0.025%
80	30.234	4542	4544	4545	rBV2	1745	990	0.14%	0.017%
81	30.639	4611	4613	4616	rBV4	2013	2033	0.28%	0.036%
82	30.663	4616	4617	4618	rBV	1810	837	0.12%	0.015%
83	31.467	4752	4754	4755	rBV	1848	922	0.13%	0.016%
84	31.826	4813	4815	4818	rVB4	2016	2320	0.32%	0.041%
85	32.437	4917	4919	4920	rBV2	1662	976	0.14%	0.017%
86	32.584	4942	4944	4945	rBV2	1314	718	0.10%	0.013%




Sum of corrected areas: 5670176

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057345.D
Acq On : 9 May 2023 1:02
Operator : CG/JU
Sample : 02619-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

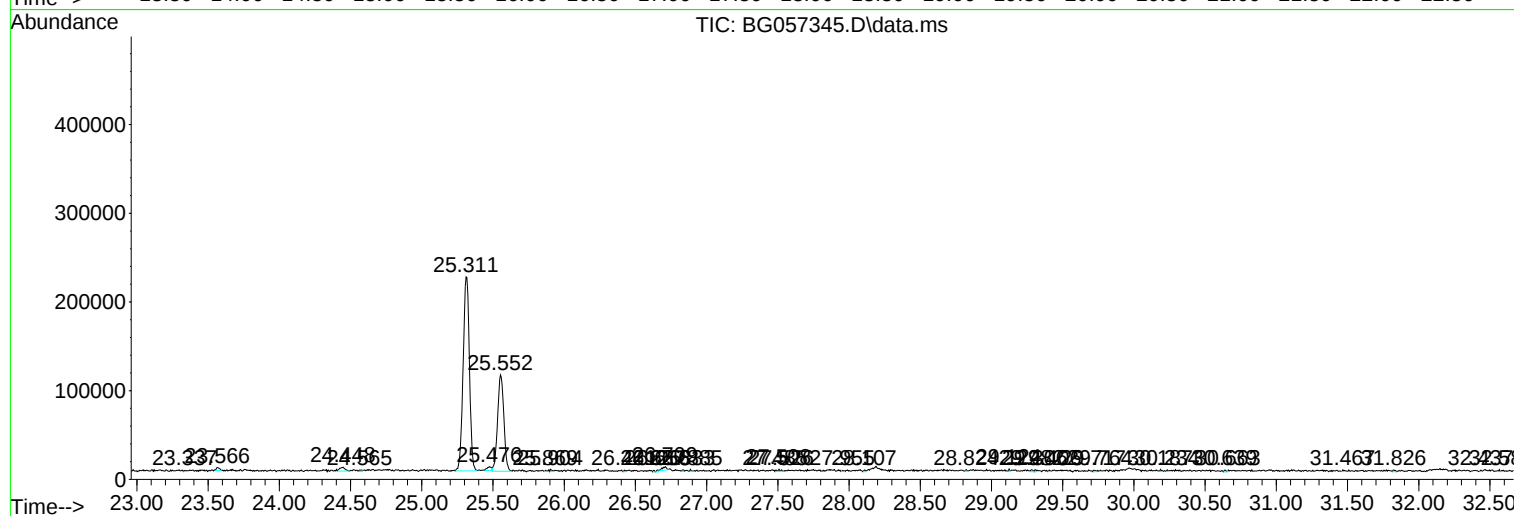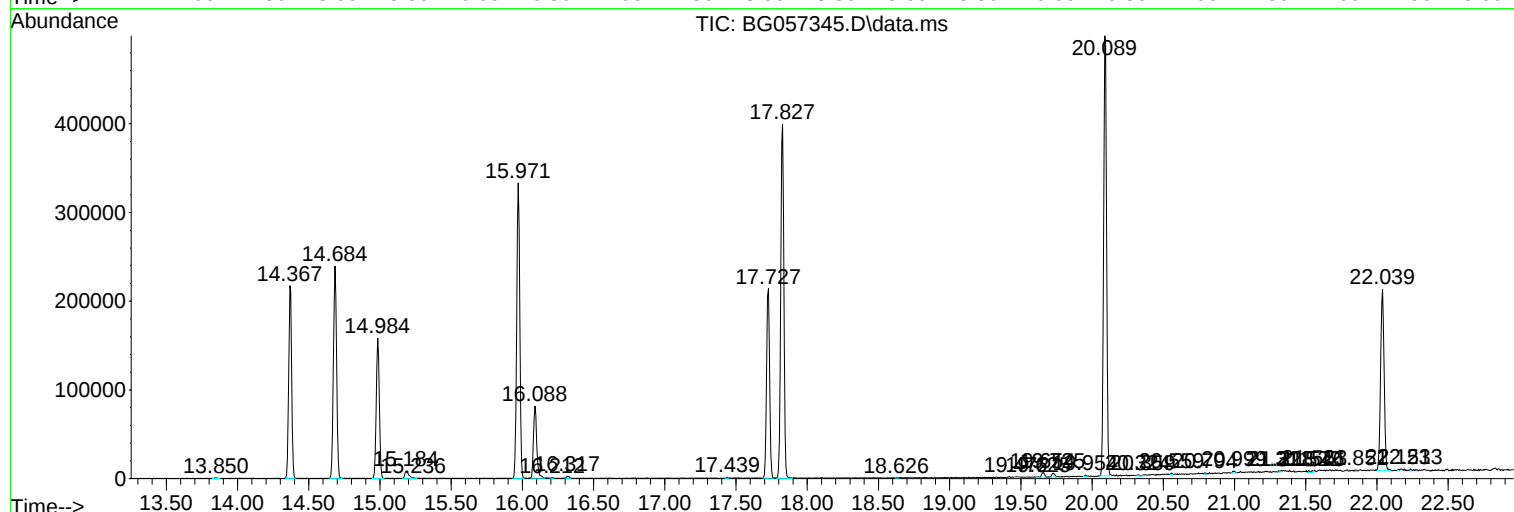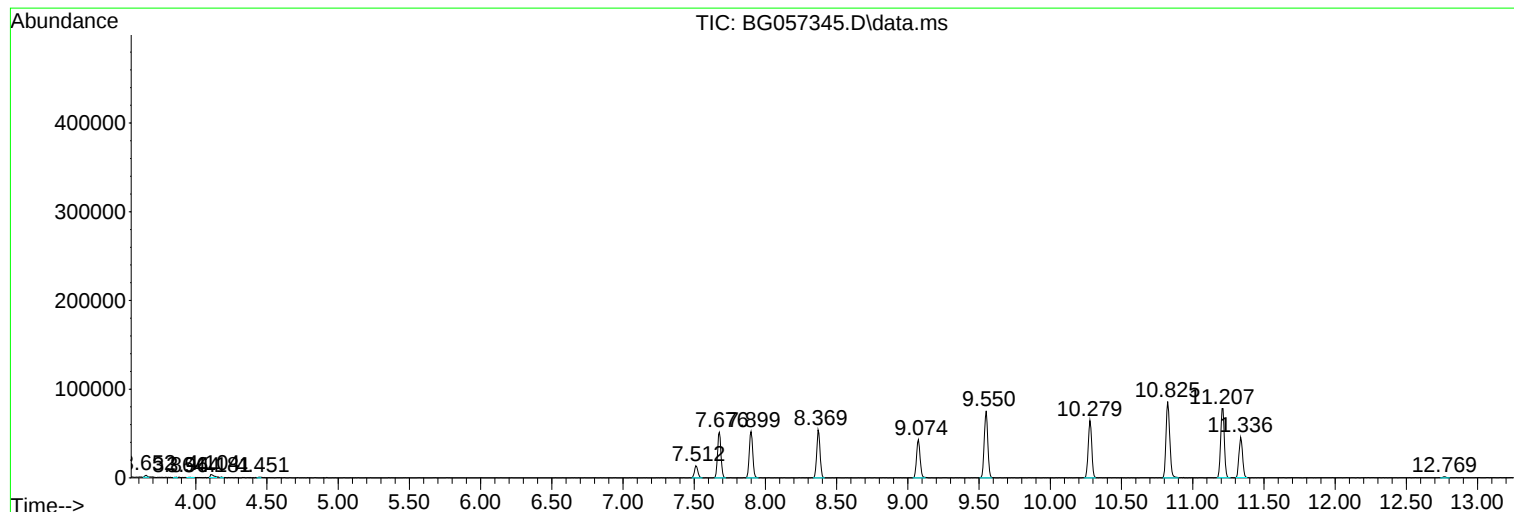

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057345.D
Acq On : 9 May 2023 1:02
Operator : CG/JU
Sample : 02619-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050823\
Data File : BG057345.D
Acq On : 9 May 2023 1:02
Operator : CG/JU
Sample : 02619-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFZE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc