

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG016996.D
 Acq On : 9 May 2015 19:13
 Operator : TP/IZ
 Sample : G2183-02
 Misc : 625 SURR ADDED
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-1

Quant Time: May 19 07:29:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 05 16:13:58 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	54208	20.00	ng	-0.02
21) Naphthalene-d8	10.58	136	253379	20.00	ng	-0.02
38) Acenaphthene-d10	14.43	164	179735	20.00	ng	-0.02
63) Phenanthrene-d10	17.17	188	422215	20.00	ng	-0.02
75) Chrysene-d12	21.34	240	407299	20.00	ng	-0.02
86) Perylene-d12	23.64	264	399719	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	154265	49.55	ng	-0.01
7) Phenol-d6	6.95	99	140910	31.68	ng	-0.01
23) Nitrobenzene-d5	8.95	82	592709	114.28	ng	-0.01
41) 2,4,6-Tribromophenol	15.91	330	227407	126.03	ng	-0.02
44) 2-Fluorobiphenyl	13.05	172	1244301	104.47	ng	-0.02
78) Terphenyl-d14	19.80	244	2095069	120.58	ng	-0.02
Target Compounds						
32) Benzoic acid	9.83	122	88	Below Cal	Qvalue #	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG016996.D
Acq On : 9 May 2015 19:13
Operator : TP/IZ
Sample : G2183-02
Misc : 625 SURR ADDED
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1

Quant Time: May 19 07:29:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 16:13:58 2015
Response via : Initial Calibration

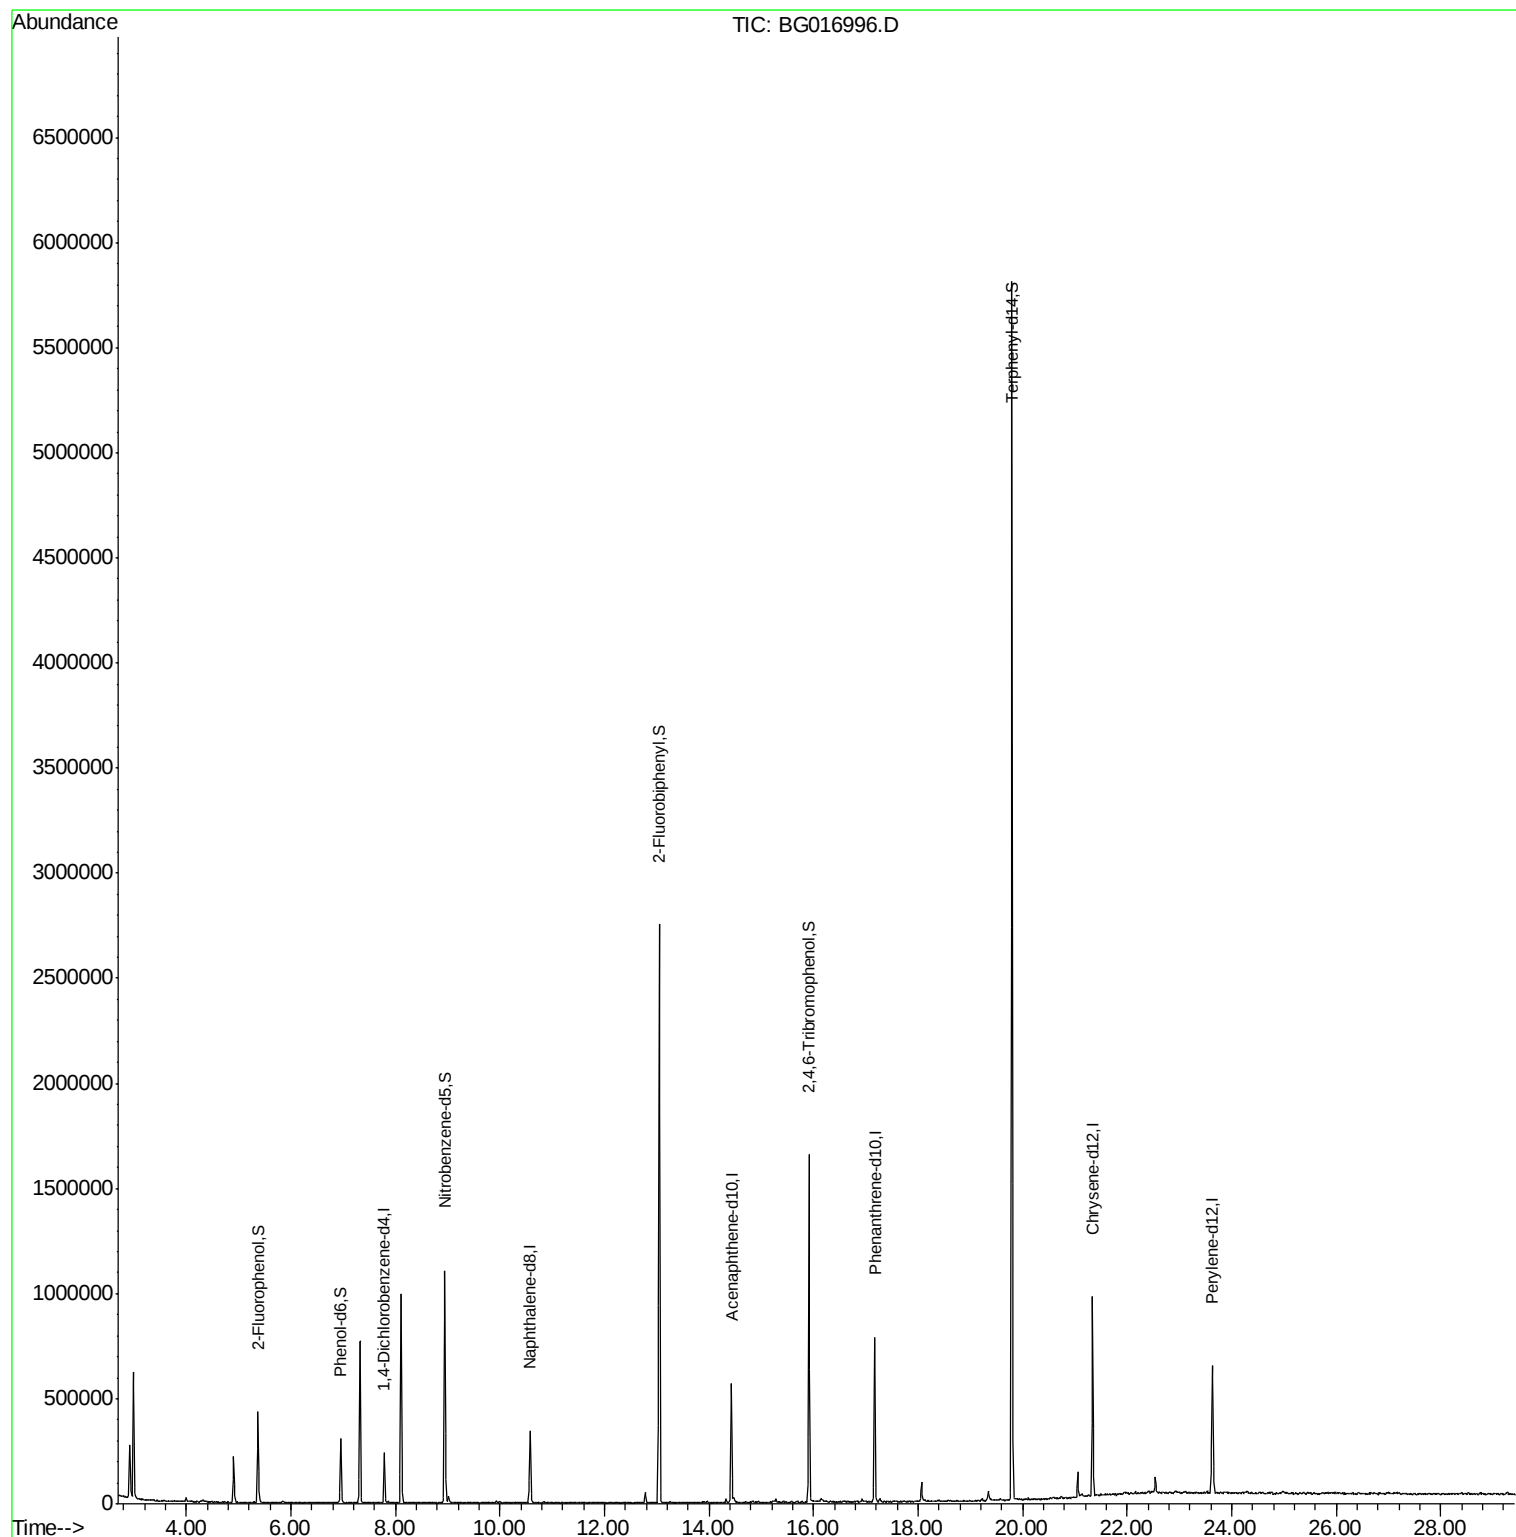

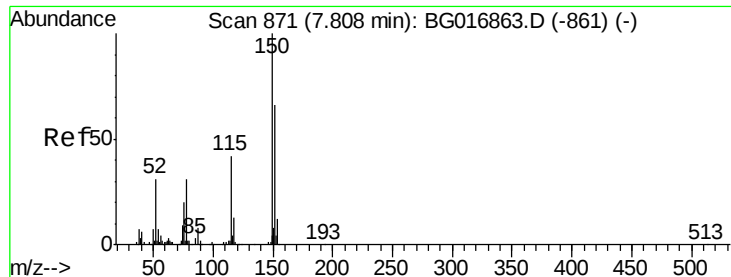

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 868

Delta R.T. -0.02 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13

Instrument :

BNA_G

ClientSampleId :

SB-1


Tgt Ion:152 Resp: 54208

Ion Ratio Lower Upper

152 100

150 148.7 121.0 181.4



115 63.8 50.5 75.7

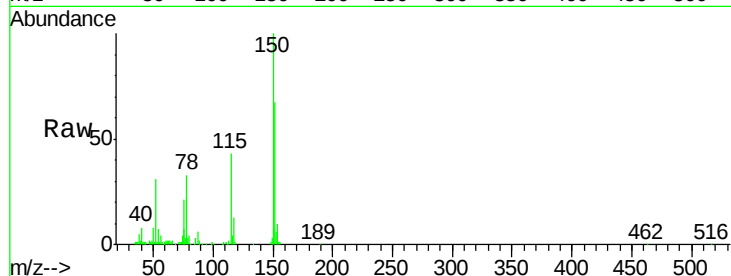

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

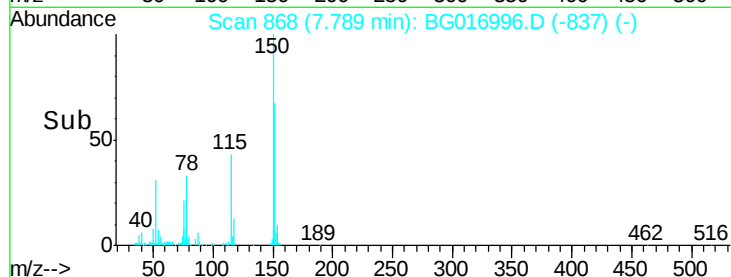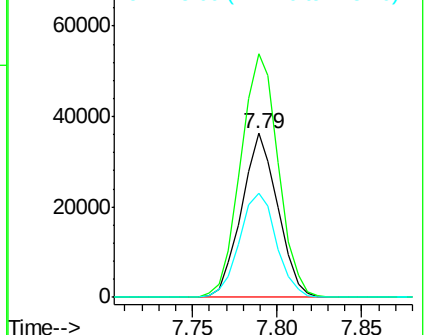

#5

2-Fluorophenol

Concen: 49.55 ng

RT: 5.37 min Scan# 457

Delta R.T. -0.01 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13


Tgt Ion:112 Resp: 154265

Ion Ratio Lower Upper

112 100

64 67.3 51.4 77.2



63 36.4 28.1 42.1

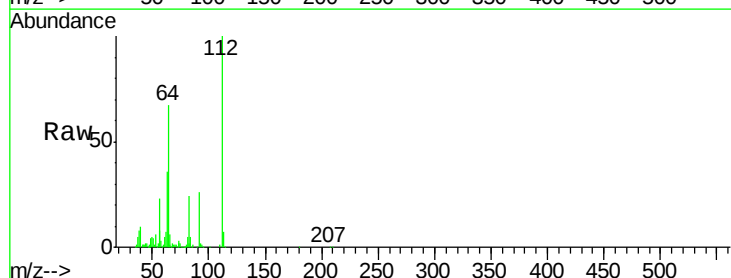


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

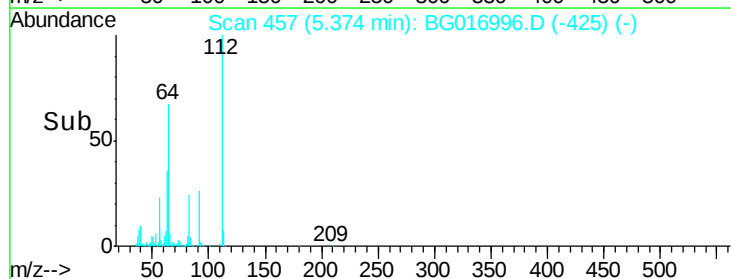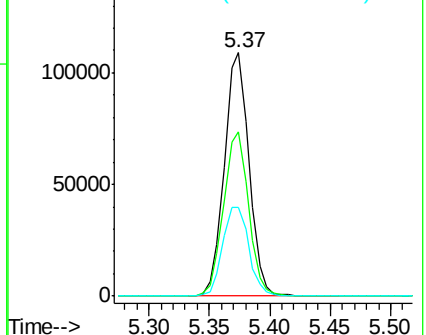

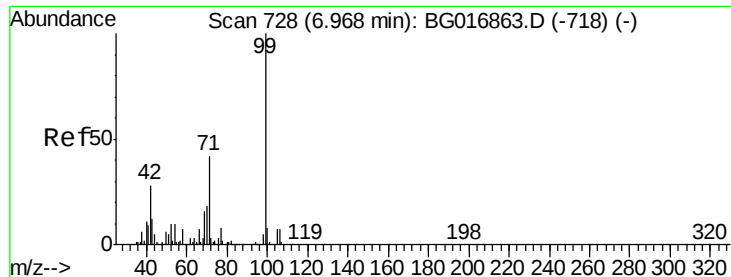

#7

Phenol-d6

Concen: 31.68 ng

RT: 6.95 min Scan# 726

Delta R.T. -0.01 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13

Instrument :

BNA_G

ClientSampleId :

SB-1


Tgt Ion: 99 Resp: 140910

Ion Ratio Lower Upper




99 100

42 26.9 22.1 33.1

71 41.8 33.4 50.0

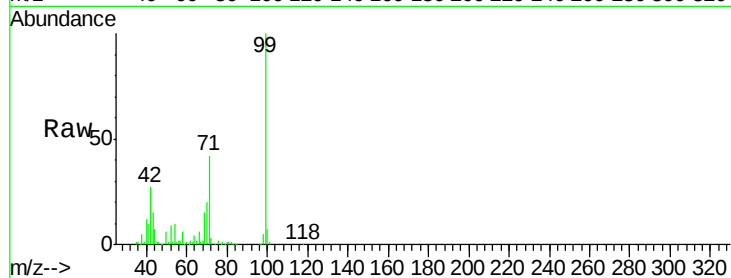

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

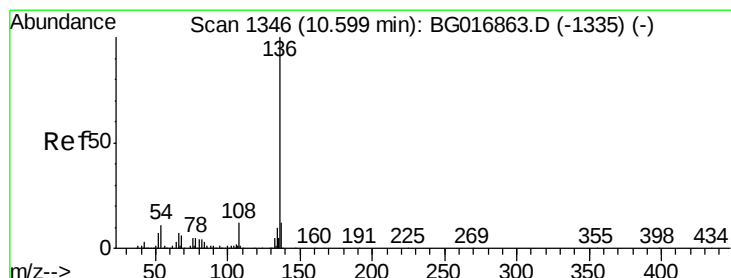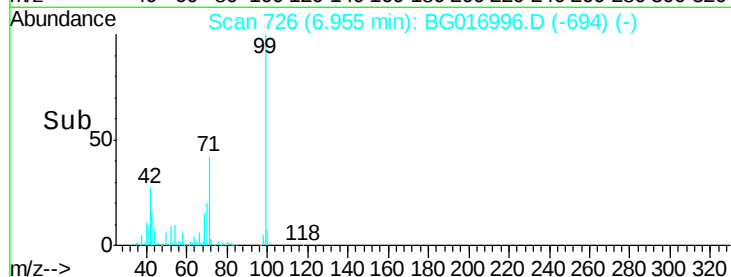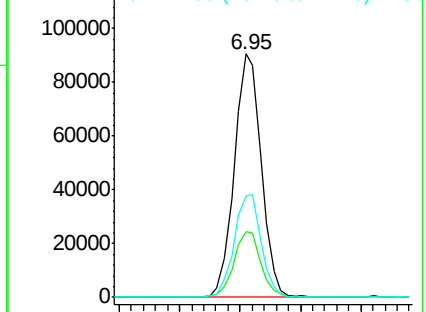

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1343

Delta R.T. -0.02 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13

Tgt Ion: 136 Resp: 253379


Ion Ratio Lower Upper

136 100



137 10.3 9.8 14.8

54 9.2 8.7 13.1

68 7.1 5.0 7.4

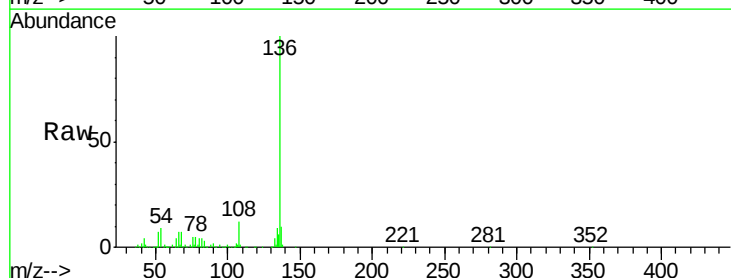

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



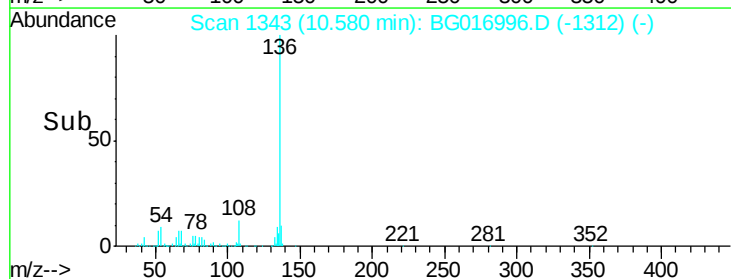
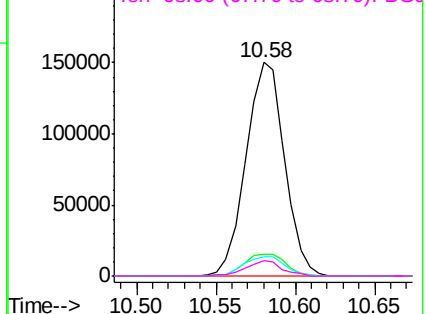




#23
 Nitrobenzene-d5
 Concen: 114.28 ng
 RT: 8.95 min Scan# 1066
 Delta R.T. -0.01 min
 Lab File: BG016996.D
 Acq: 9 May 2015 19:13




Instrument :
 BNA_G
 ClientSampleID :
 SB-1


Tgt Ion: 82 Resp: 592709
 Ion Ratio Lower Upper
 82 100
 128 40.3 33.2 49.8
 54 54.6 48.6 72.8

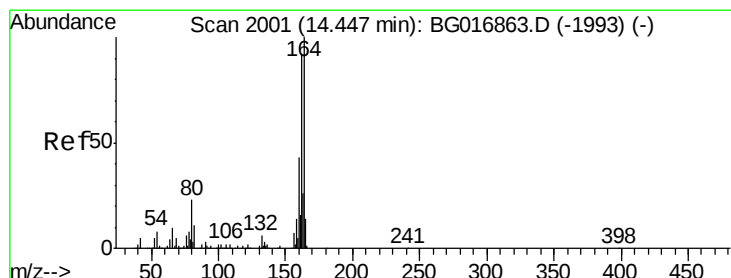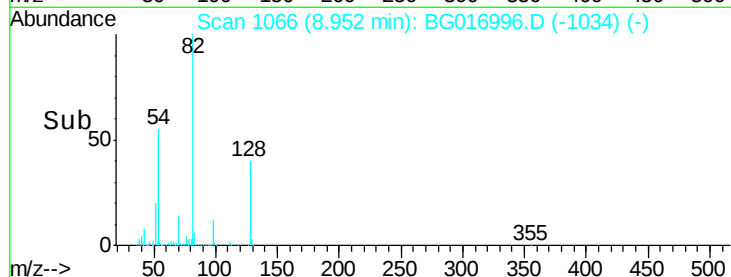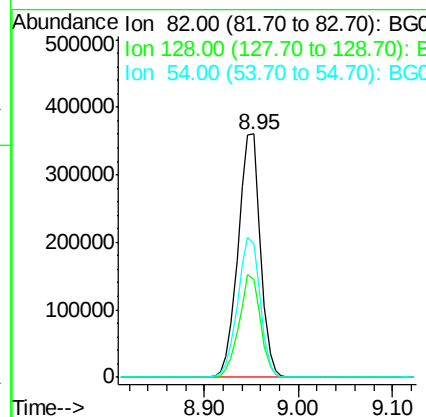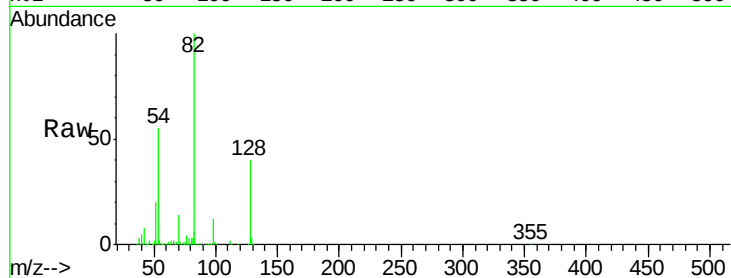

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. -0.02 min
 Lab File: BG016996.D
 Acq: 9 May 2015 19:13

Tgt Ion: 164 Resp: 179735
 Ion Ratio Lower Upper
 164 100
 162 96.3 74.0 111.0
 160 45.3 34.7 52.1

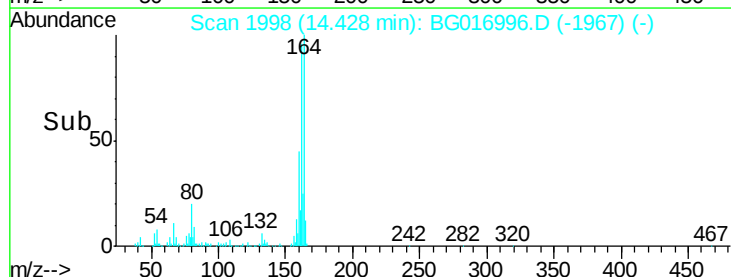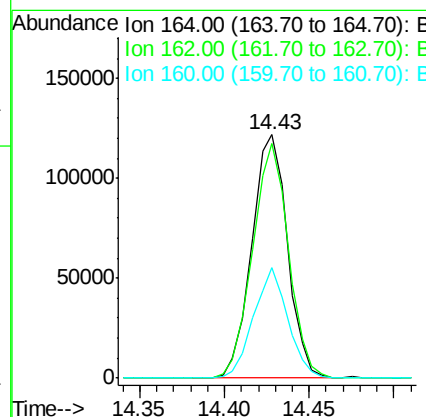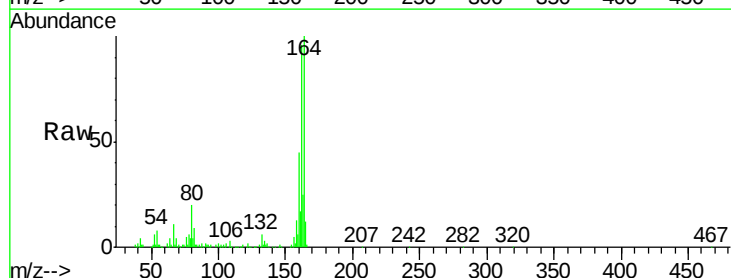


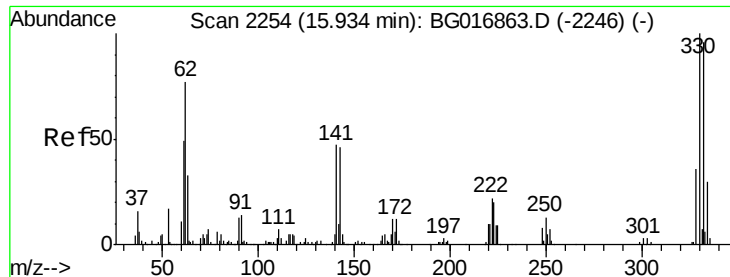




#41
 2,4,6-Tribromophenol
 Concen: 126.03 ng
 RT: 15.91 min Scan# 2251
 Delta R.T. -0.02 min
 Lab File: BG016996.D
 Acq: 9 May 2015 19:13

Instrument :
 BNA_G
 ClientSampleID :
 SB-1

Tgt Ion:330 Resp: 227407
 Ion Ratio Lower Upper
 330 100
 332 95.6 0.0 0.0#
 141 50.2 0.0 0.0#

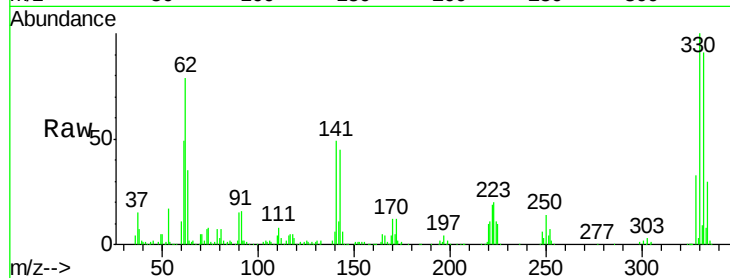


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

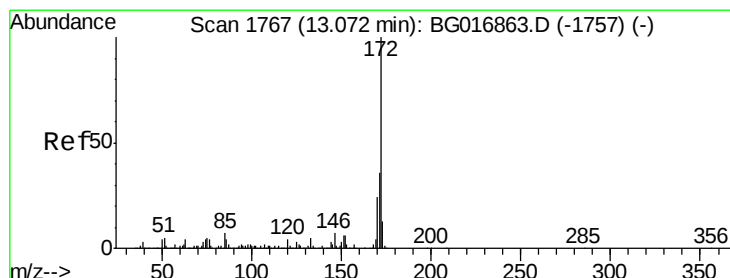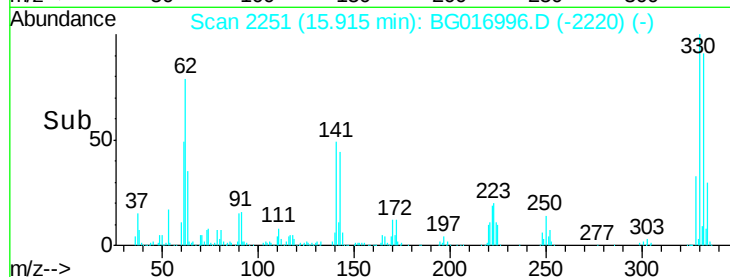
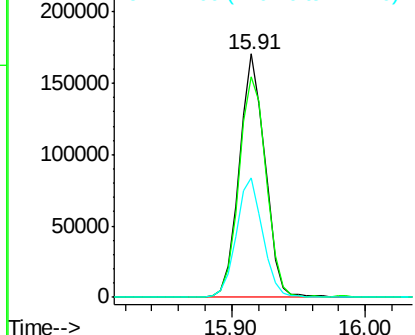



#44
 2-Fluorobiphenyl
 Concen: 104.47 ng
 RT: 13.05 min Scan# 1764
 Delta R.T. -0.02 min
 Lab File: BG016996.D
 Acq: 9 May 2015 19:13

Tgt Ion:172 Resp: 1244301
 Ion Ratio Lower Upper
 172 100
 171 38.3 29.0 43.4
 170 24.0 19.0 28.4

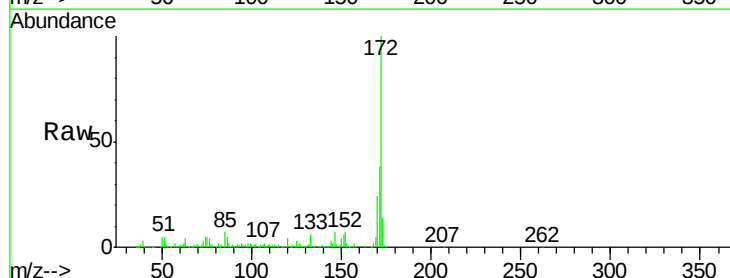

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

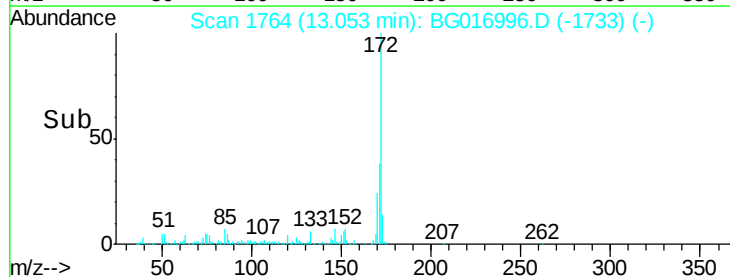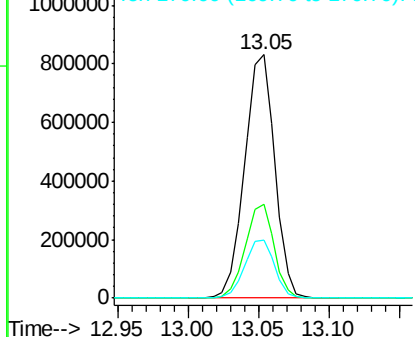

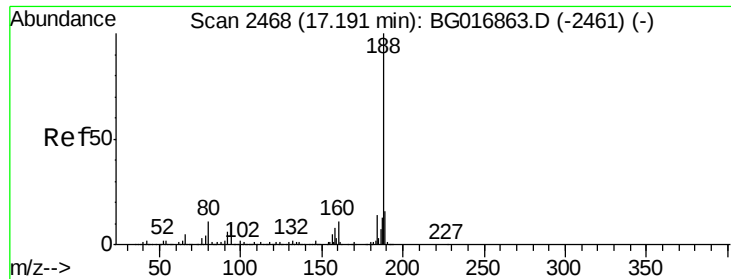

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2465

Delta R.T. -0.02 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13

Instrument :

BNA_G

ClientSampleId :

SB-1


Tgt Ion:188 Resp: 422215

Ion Ratio Lower Upper

188 100

94 9.4 8.2 12.4




80 10.3 8.8 13.2

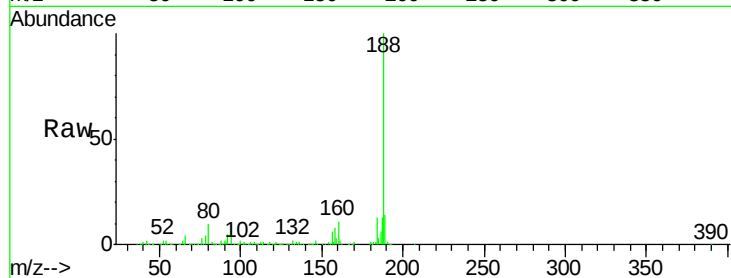

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

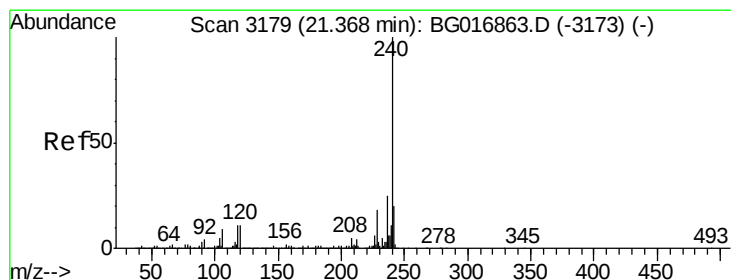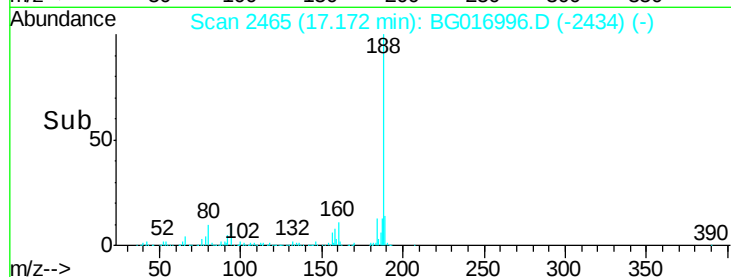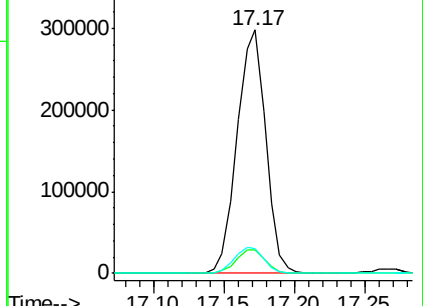

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.34 min Scan# 3175

Delta R.T. -0.02 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13


Tgt Ion:240 Resp: 407299

Ion Ratio Lower Upper

240 100

120 11.4 9.1 13.7



236 26.5 20.2 30.4

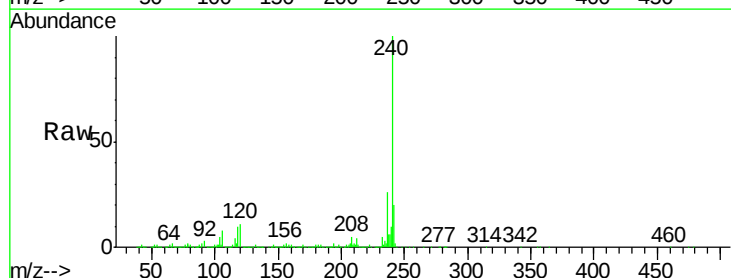


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

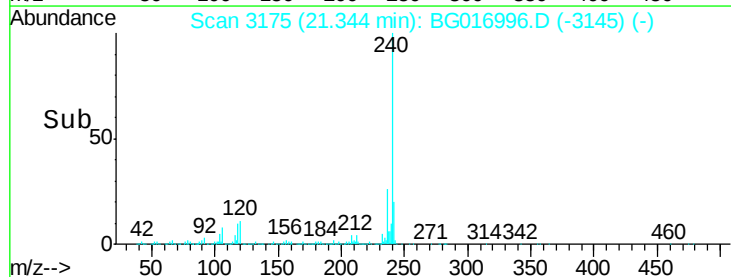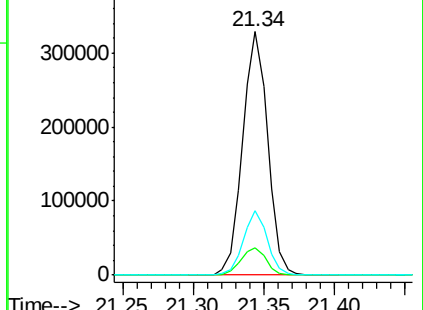

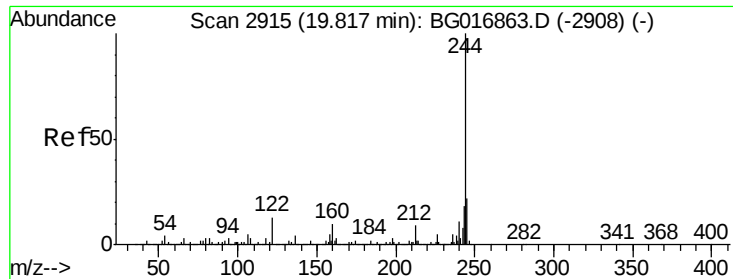

#78

Terphenyl-d14

Concen: 120.58 ng

RT: 19.80 min Scan# 2912

Delta R.T. -0.02 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13

Instrument :

BNA_G

ClientSampleId :

SB-1


Tgt Ion:244 Resp: 2095069

Ion Ratio Lower Upper

244 100

212 10.4 7.0 10.6




122 15.3 10.4 15.6

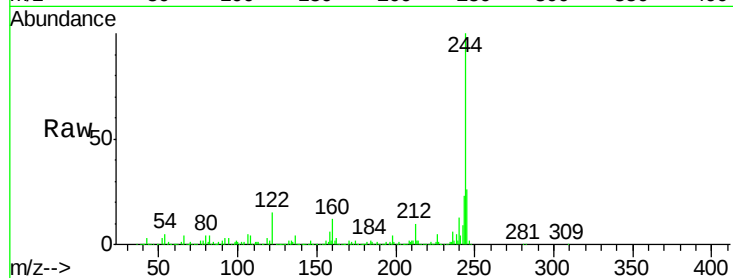

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

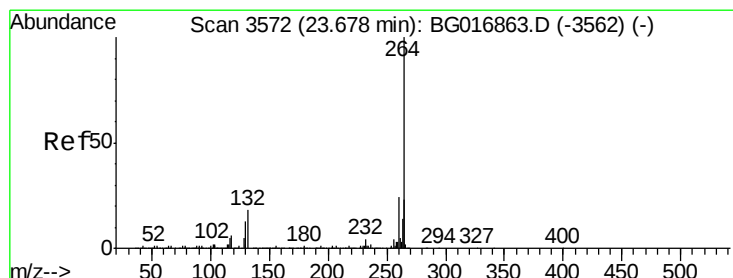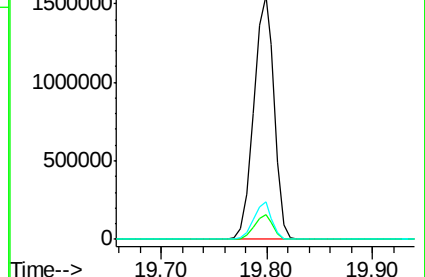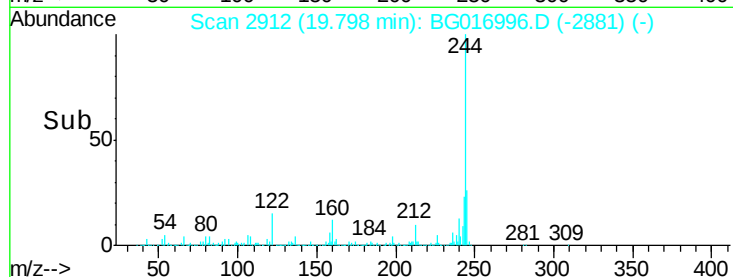

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.64 min Scan# 3565

Delta R.T. -0.04 min

Lab File: BG016996.D

Acq: 9 May 2015 19:13


Tgt Ion:264 Resp: 399719

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 20.9 18.5 27.7

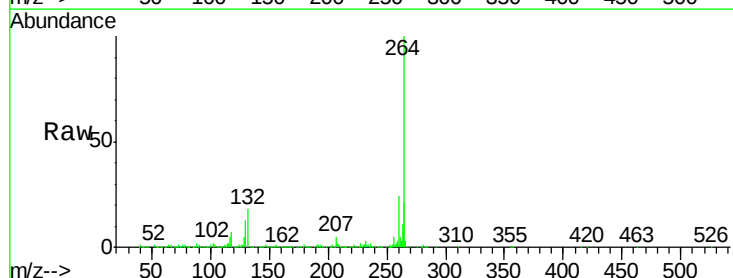

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

