

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG017007.D
 Acq On : 10 May 2015 1:35
 Operator : TP/IZ
 Sample : G2104-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-101

Quant Time: May 19 07:31:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 05 16:13:58 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	79281	20.00	ng	-0.02
21) Naphthalene-d8	10.58	136	394914	20.00	ng	-0.02
38) Acenaphthene-d10	14.43	164	273852	20.00	ng	-0.02
63) Phenanthrene-d10	17.17	188	616133	20.00	ng	-0.02
75) Chrysene-d12	21.35	240	596980	20.00	ng	-0.02
86) Perylene-d12	23.64	264	592987	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	215234	47.27	ng	-0.02
7) Phenol-d6	6.96	99	218466	33.58	ng	-0.01
23) Nitrobenzene-d5	8.95	82	461635	57.11	ng	-0.02
41) 2,4,6-Tribromophenol	15.92	330	307134	111.72	ng	-0.02
44) 2-Fluorobiphenyl	13.05	172	1035343	57.05	ng	-0.02
78) Terphenyl-d14	19.79	244	1544797	60.66	ng	-0.02
Target Compounds						
32) Benzoic acid	9.82	122	125	Below Cal	Qvalue #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG017007.D
Acq On : 10 May 2015 1:35
Operator : TP/IZ
Sample : G2104-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-101

Quant Time: May 19 07:31:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 16:13:58 2015
Response via : Initial Calibration

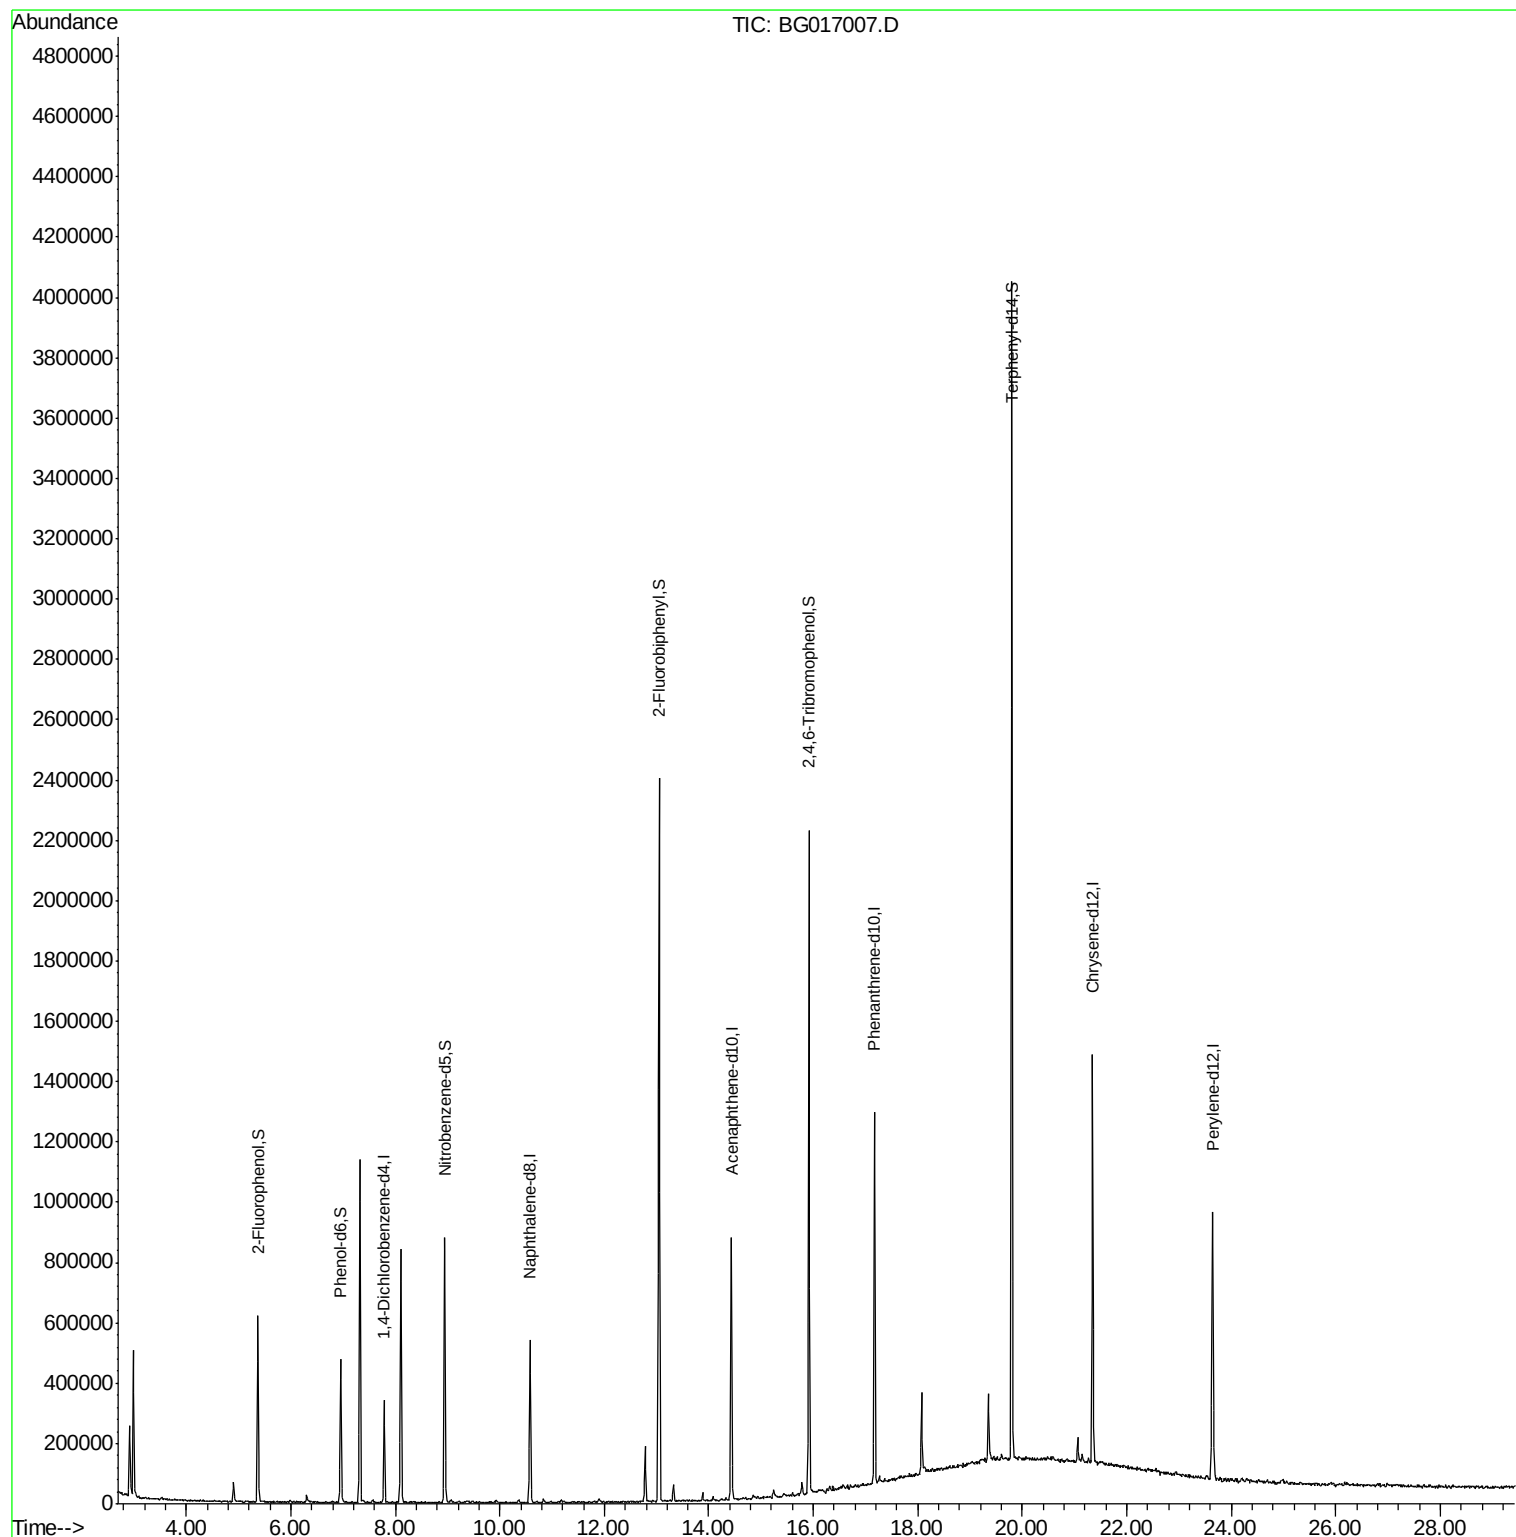

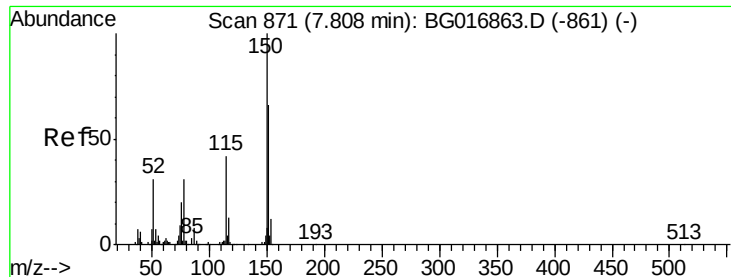


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.79 min Scan# 867
Delta R.T. -0.02 min
Lab File: BG017007.D
Acq: 10 May 2015 1:35

Instrument :
BNA_G
ClientSampleId :
MW-101

Tgt Ion:152 Resp: 79281
Ion Ratio Lower Upper
152 100
150 151.5 121.0 181.4
115 64.1 50.5 75.7

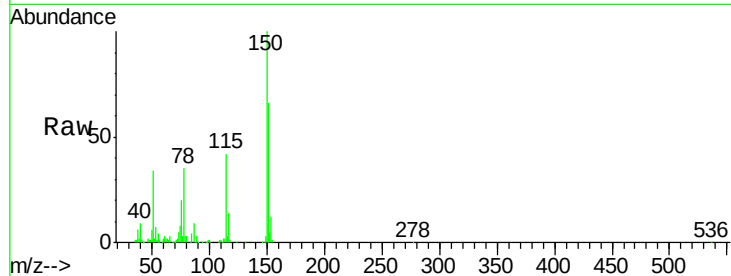


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

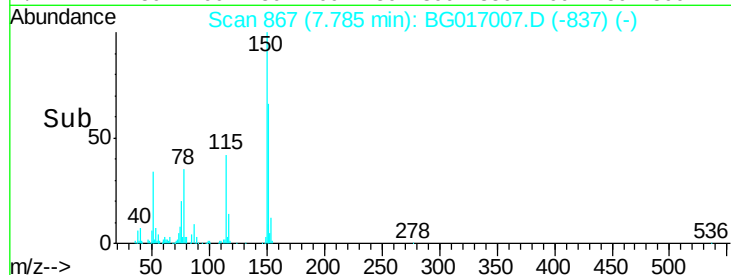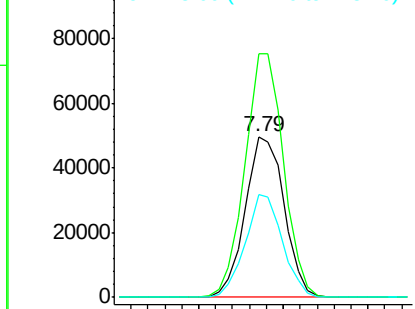



#5


2-Fluorophenol
Concen: 47.27 ng
RT: 5.37 min Scan# 456
Delta R.T. -0.02 min
Lab File: BG017007.D
Acq: 10 May 2015 1:35

Tgt Ion:112 Resp: 215234
Ion Ratio Lower Upper
112 100
64 72.4 51.4 77.2
63 39.3 28.1 42.1

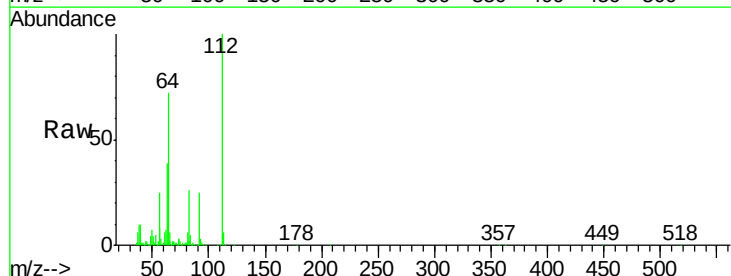

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

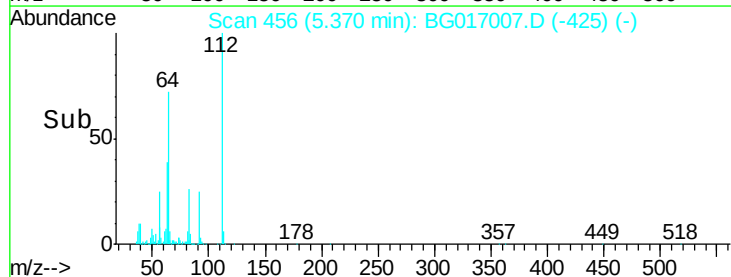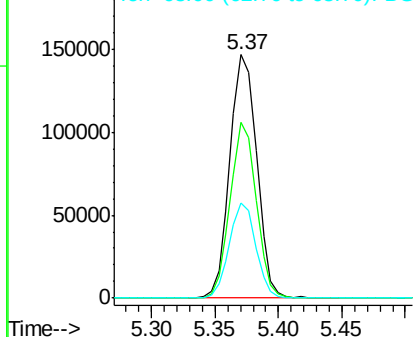

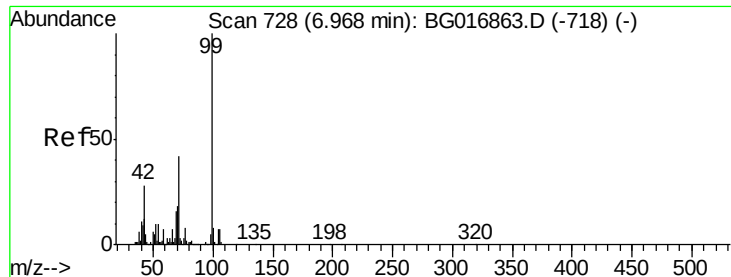

#7

Phenol-d6

Concen: 33.58 ng

RT: 6.96 min Scan# 726

Delta R.T. -0.01 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35

Instrument :

BNA_G

ClientSampleId :

MW-101


Tgt Ion: 99 Resp: 218466

Ion Ratio Lower Upper




99 100

42 27.6 22.1 33.1

71 42.6 33.4 50.0

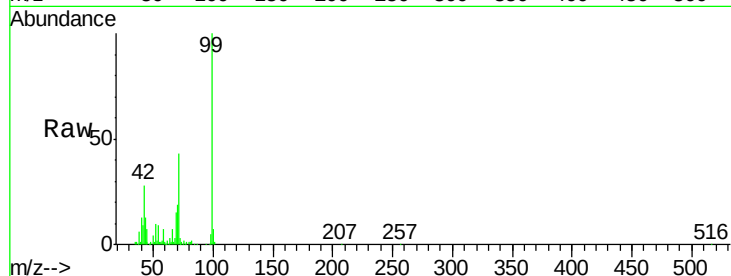

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

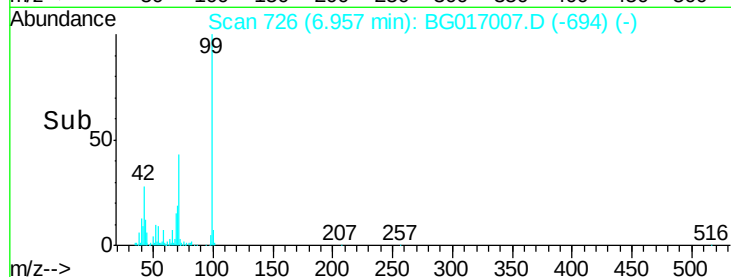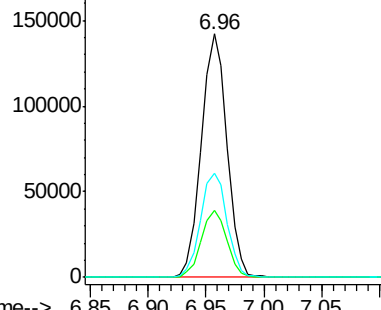

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1343

Delta R.T. -0.02 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35

Tgt Ion: 136 Resp: 394914


Ion Ratio Lower Upper

136 100



137 11.4 9.8 14.8


54 9.5 8.7 13.1

68 6.1 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



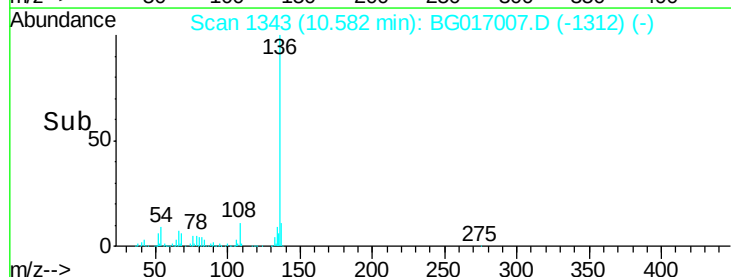
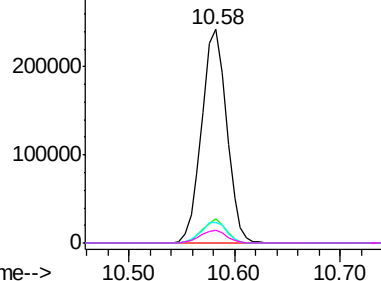


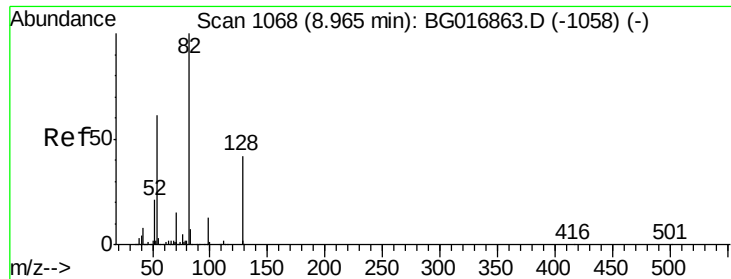

#23
 Nitrobenzene-d5
 Concen: 57.11 ng
 RT: 8.95 min Scan# 1065
 Delta R.T. -0.02 min
 Lab File: BG017007.D
 Acq: 10 May 2015 1:35




Instrument :
 BNA_G
 ClientSampleId :
 MW-101


Tgt Ion	Ratio	Lower	Upper
82	100		
128	42.7	33.2	49.8
54	60.4	48.6	72.8

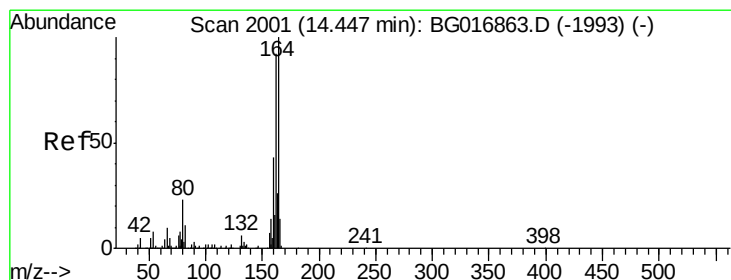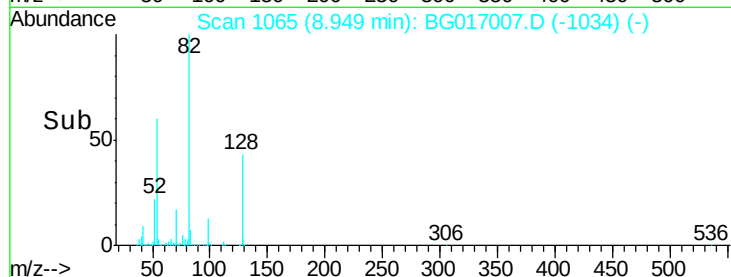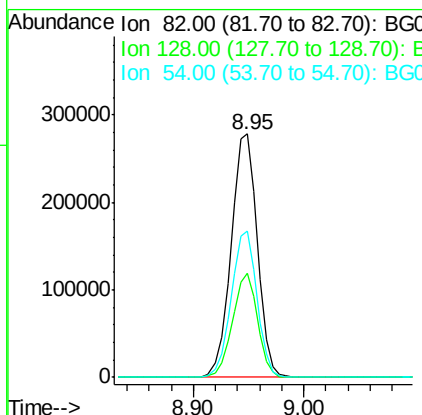

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. -0.02 min
 Lab File: BG017007.D
 Acq: 10 May 2015 1:35

Tgt Ion	Ratio	Lower	Upper
164	100		
162	93.6	74.0	111.0
160	42.8	34.7	52.1

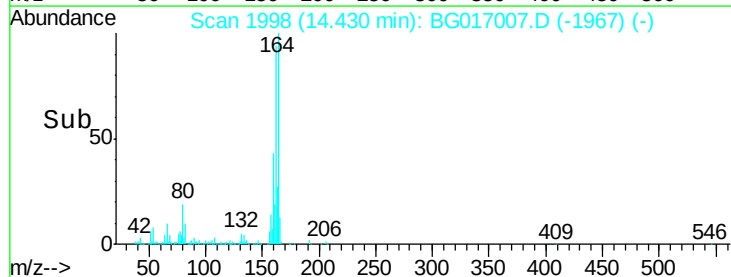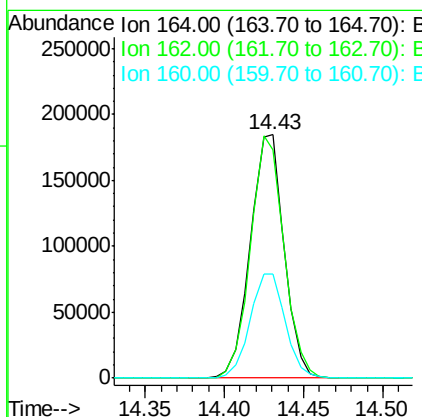


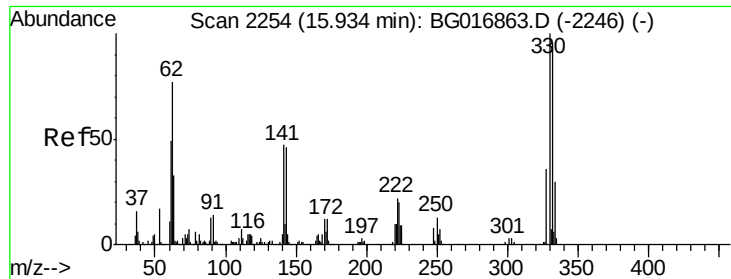




#41
 2,4,6-Tribromophenol
 Concen: 111.72 ng
 RT: 15.92 min Scan# 2251
 Delta R.T. -0.02 min
 Lab File: BG017007.D
 Acq: 10 May 2015 1:35

Instrument :
 BNA_G
 ClientSampleId :
 MW-101

Tgt Ion:330 Resp: 307134
 Ion Ratio Lower Upper
 330 100
 332 95.0 0.0 0.0#
 141 51.0 0.0 0.0#

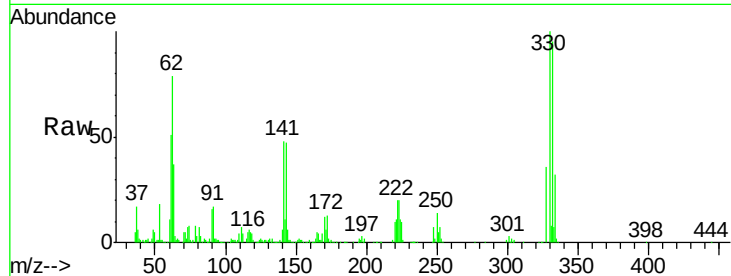


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

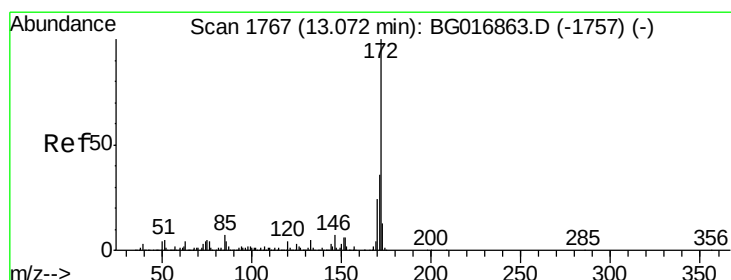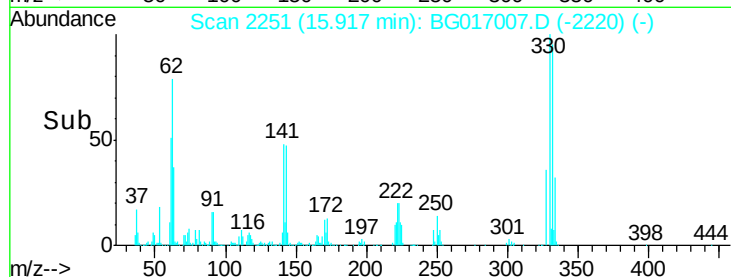
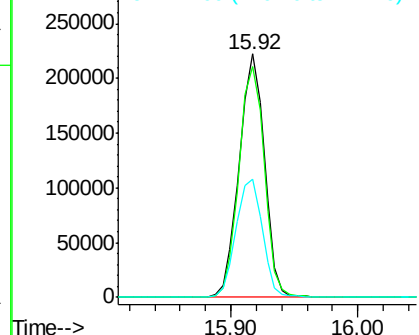



#44
 2-Fluorobiphenyl
 Concen: 57.05 ng
 RT: 13.05 min Scan# 1763
 Delta R.T. -0.02 min
 Lab File: BG017007.D
 Acq: 10 May 2015 1:35

Tgt Ion:172 Resp: 1035343
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.0 43.4
 170 24.0 19.0 28.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

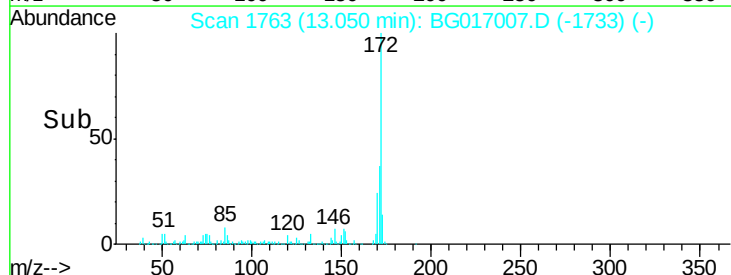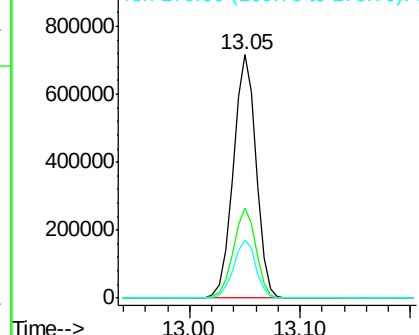

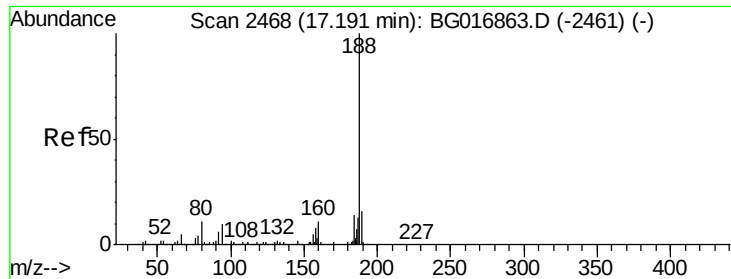

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2464

Delta R.T. -0.02 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35

Instrument :

BNA_G

ClientSampleId :

MW-101


Tgt Ion:188 Resp: 616133

Ion Ratio Lower Upper

188 100

94 10.5 8.2 12.4




80 10.9 8.8 13.2

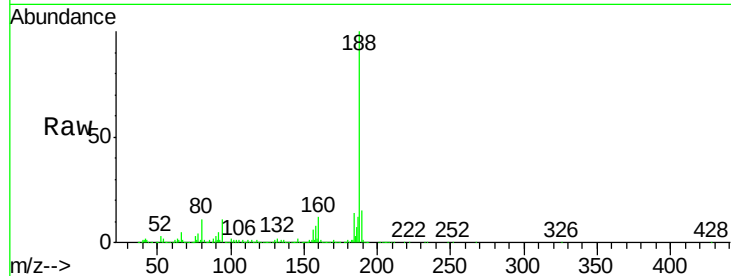

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

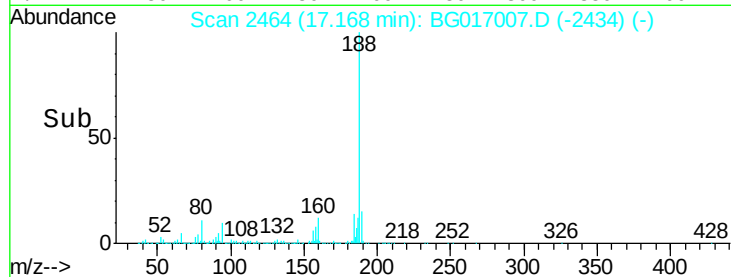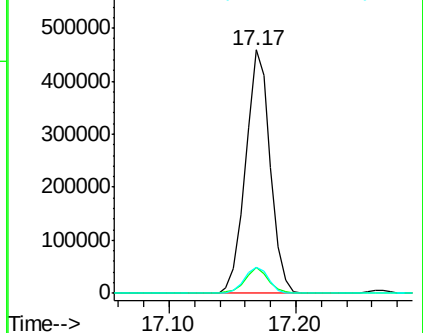

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.35 min Scan# 3175

Delta R.T. -0.02 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35


Tgt Ion:240 Resp: 596980

Ion Ratio Lower Upper

240 100

120 11.1 9.1 13.7



236 25.0 20.2 30.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

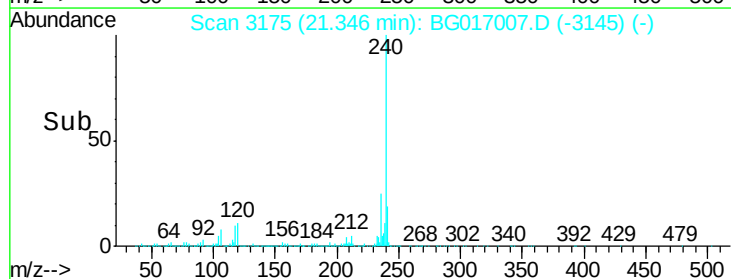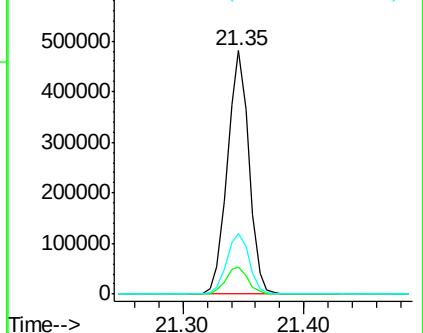

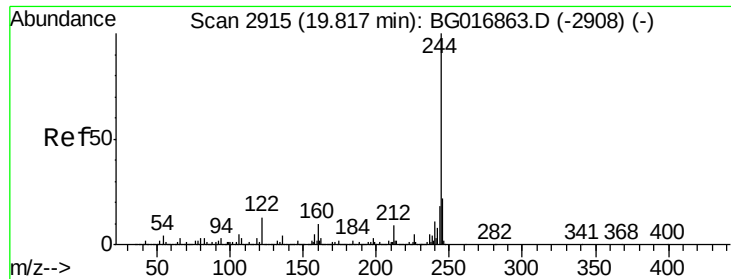

#78

Terphenyl-d14

Concen: 60.66 ng

RT: 19.79 min Scan# 2911

Delta R.T. -0.02 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35

Instrument :


BNA_G

ClientSampleId :

MW-101

Tgt Ion:244 Resp: 1544797

Ion	Ratio	Lower	Upper
244	100		
212	9.2	7.0	10.6
122	13.8	10.4	15.6



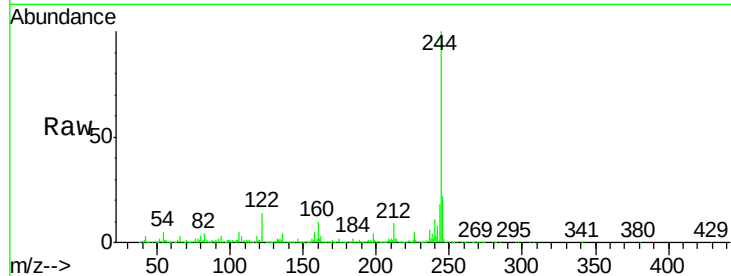


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

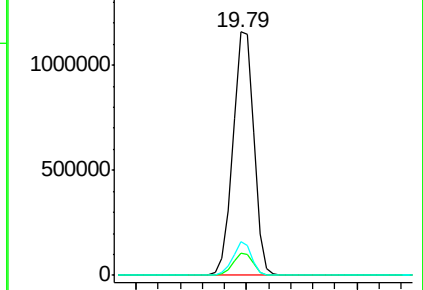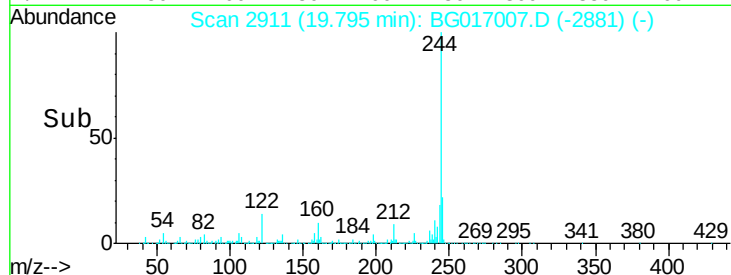

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.64 min Scan# 3566


Delta R.T. -0.03 min

Lab File: BG017007.D

Acq: 10 May 2015 1:35

Tgt Ion:264 Resp: 592987

Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.5	29.3
265	23.3	18.5	27.7



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

