
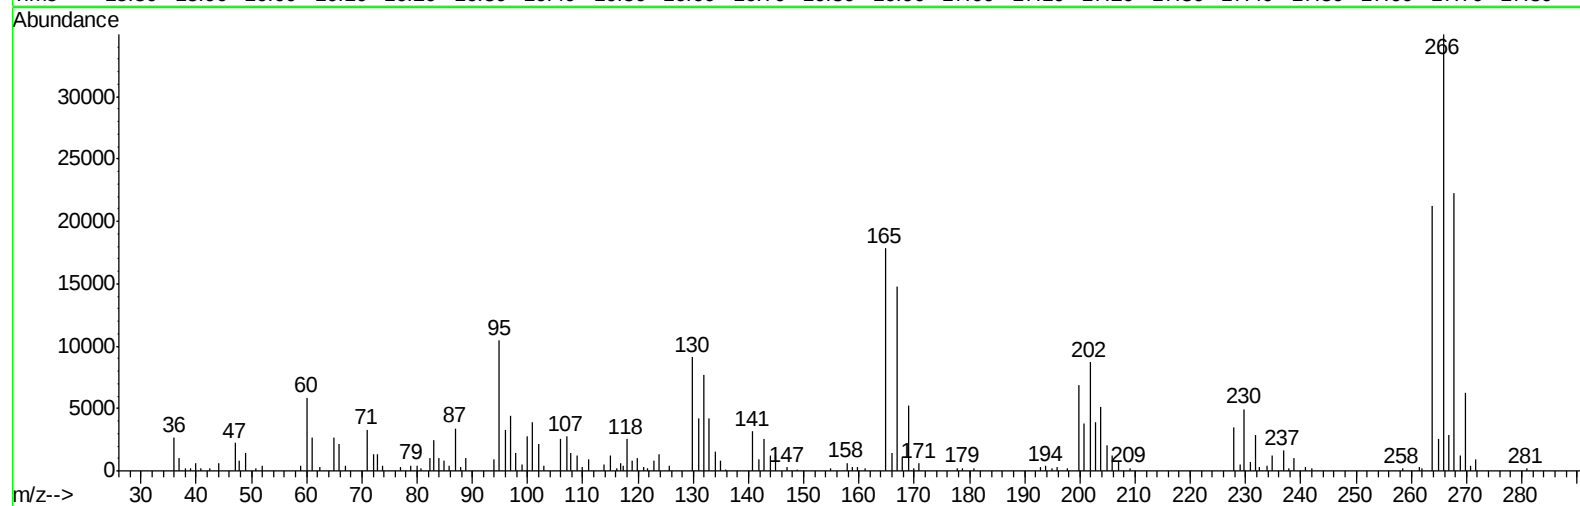


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016987.D
Acq On : 9 May 2015 12:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:06:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

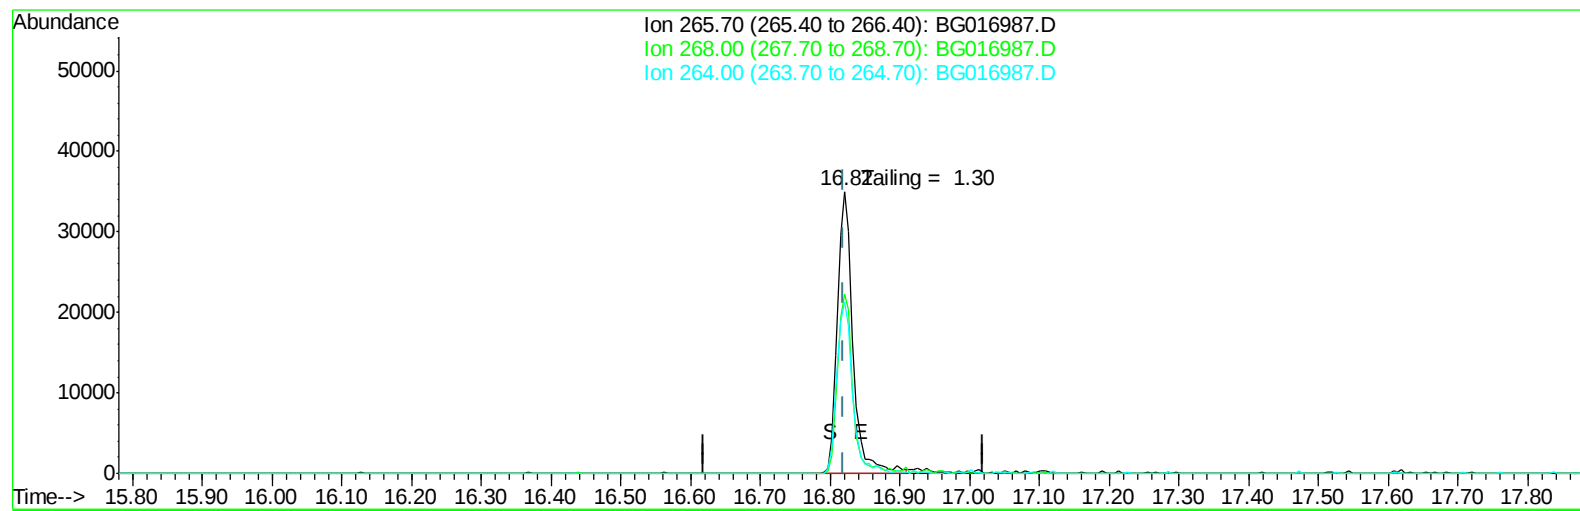

TIC: BG016987.D

(69) Pentachlorophenol (C)



16.820min (-0.000) 83559.04ng

response 53402

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	63.68
264.00	64.20	60.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG016987.D
Acq On : 9 May 2015 12:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 07:06:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 11 06:04:58 2015
Response via : Initial Calibration

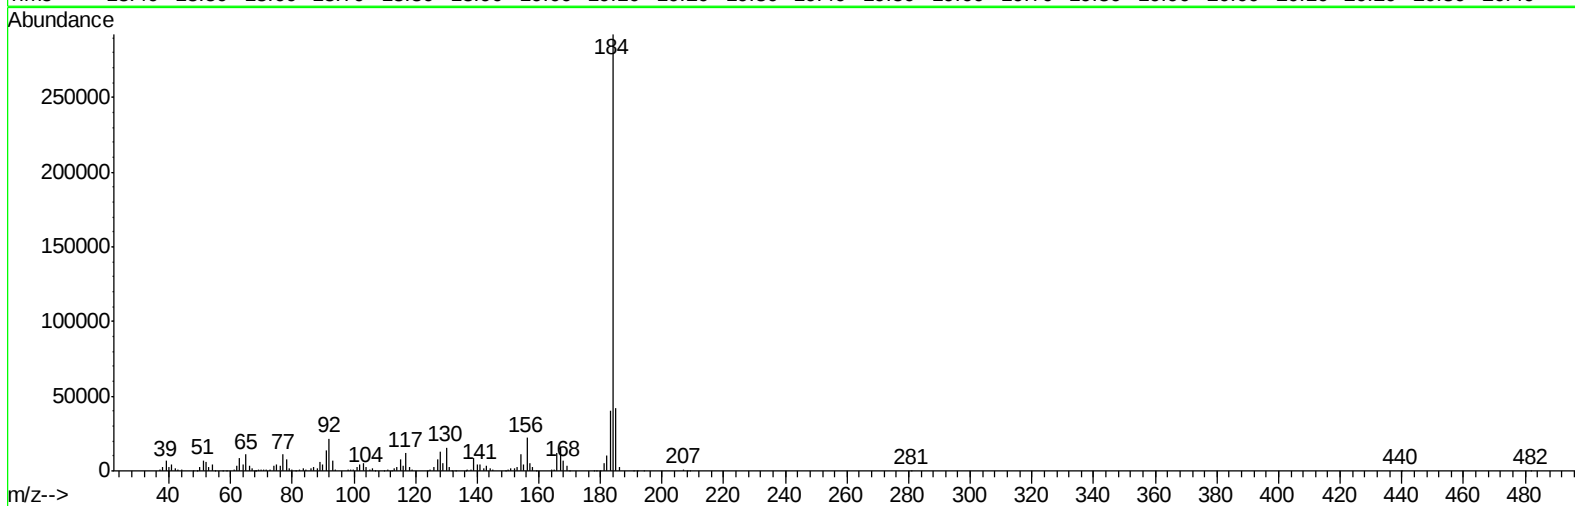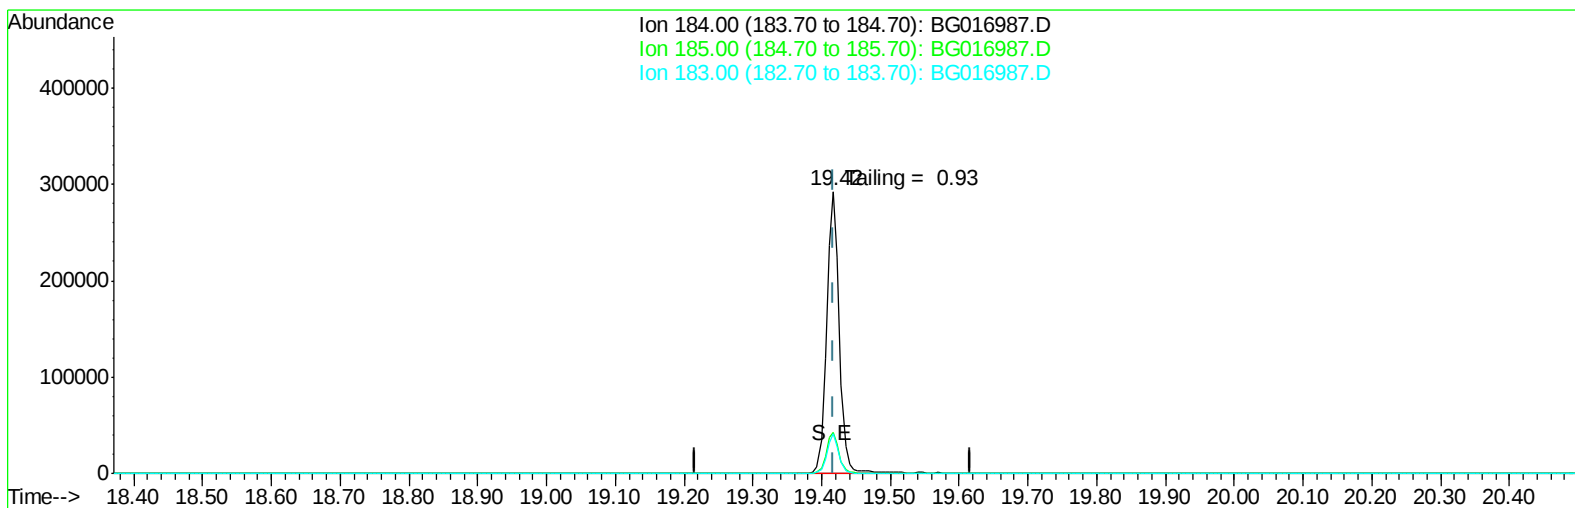

TIC: BG016987.D

(76) Benzidine

19.417min (-0.000) 0.00ng

response 375792

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.41
183.00	13.20	13.93
0.00	0.00	0.00