

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG016992.D
 Acq On : 9 May 2015 16:54
 Operator : TP/IZ
 Sample : G2180-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-CW-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.917	34	39	47	rBV	304786	470143	6.50%	1.278%
2	2.993	47	52	66	rVB	639835	820731	11.34%	2.231%
3	4.908	372	378	386	rBV	226502	310976	4.30%	0.845%
4	5.373	451	457	467	rVB	411784	585858	8.09%	1.592%
5	6.959	720	727	736	rVB	280493	445024	6.15%	1.210%
6	7.323	779	789	798	rBV	799774	1251629	17.29%	3.402%
7	7.787	861	868	874	rBV	240218	379608	5.25%	1.032%
8	7.852	874	879	886	rVB	175835	265523	3.67%	0.722%
9	8.111	916	923	930	rBV	1026045	1627088	22.48%	4.423%
10	8.469	978	984	993	rVB	152211	236153	3.26%	0.642%
11	8.951	1058	1066	1074	rBV	1121861	1875395	25.91%	5.098%
12	9.632	1177	1182	1191	rBV5	33791	80001	1.11%	0.217%
13	9.767	1200	1205	1212	rVB4	91903	150422	2.08%	0.409%
14	10.584	1336	1344	1350	rBV	343521	585700	8.09%	1.592%
15	10.937	1395	1404	1410	rBV2	258886	422207	5.83%	1.148%
16	11.189	1440	1447	1456	rVB	982183	1575534	21.77%	4.283%
17	11.289	1456	1464	1473	rVB3	104390	205539	2.84%	0.559%
18	11.965	1572	1579	1587	rVB	240482	384720	5.32%	1.046%
19	12.247	1623	1627	1632	rVB3	54602	87366	1.21%	0.237%
20	12.464	1656	1664	1670	rBV7	41767	106568	1.47%	0.290%
21	12.564	1675	1681	1688	rVB8	42850	112162	1.55%	0.305%
22	12.641	1688	1694	1700	rBV3	75254	153497	2.12%	0.417%
23	13.052	1756	1764	1770	rBV	2843625	4077305	56.34%	11.083%
24	13.551	1842	1849	1853	rBV2	98639	171892	2.38%	0.467%
25	13.592	1853	1856	1860	rVV3	84675	120456	1.66%	0.327%
26	13.886	1898	1906	1912	rBV3	68171	134389	1.86%	0.365%
27	14.427	1992	1998	2005	rBV2	569305	871153	12.04%	2.368%
28	14.609	2023	2029	2034	rBV6	44274	80296	1.11%	0.218%
29	14.744	2047	2052	2062	rVB8	72451	141843	1.96%	0.386%
30	15.349	2148	2155	2165	rVB	256735	397760	5.50%	1.081%
31	15.602	2193	2198	2205	rBV8	49180	92372	1.28%	0.251%
32	15.913	2245	2251	2259	rBV	1508070	2206106	30.48%	5.997%
33	16.142	2279	2290	2298	rBV2	1922023	2977821	41.14%	8.094%
34	16.789	2396	2400	2414	rVB	225865	374110	5.17%	1.017%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG016992.D
 Acq On : 9 May 2015 16:54
 Operator : TP/IZ
 Sample : G2180-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-CW-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.171	2460	2465	2471	rVB	808611	1089552	15.05%	2.962%
36	17.370	2492	2499	2505	rBV2	61001	120089	1.66%	0.326%
37	17.529	2521	2526	2535	rBV4	85075	160212	2.21%	0.435%
38	17.834	2574	2578	2583	rVB	113012	154958	2.14%	0.421%
39	18.069	2613	2618	2632	rBV	279185	471742	6.52%	1.282%
40	18.246	2641	2648	2652	rVB	83672	137587	1.90%	0.374%
41	19.227	2806	2815	2820	rBV	192688	292017	4.03%	0.794%
42	19.350	2832	2836	2843	rVB2	136321	185703	2.57%	0.505%
43	19.591	2872	2877	2885	rVB	185068	276156	3.82%	0.751%
44	19.803	2906	2913	2918	rBV	5615721	7237518	100.00%	19.673%
45	21.060	3123	3127	3136	rBV	236995	317984	4.39%	0.864%
46	21.266	3158	3162	3165	rVB	72382	83501	1.15%	0.227%
47	21.348	3170	3176	3181	rBV	1025106	1203042	16.62%	3.270%
48	22.547	3376	3380	3386	rVB	103000	141336	1.95%	0.384%
49	23.645	3560	3567	3575	rBV2	579340	1140027	15.75%	3.099%


Sum of corrected areas: 36788771

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG016992.D
Acq On : 9 May 2015 16:54
Operator : TP/IZ
Sample : G2180-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-CW-02

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

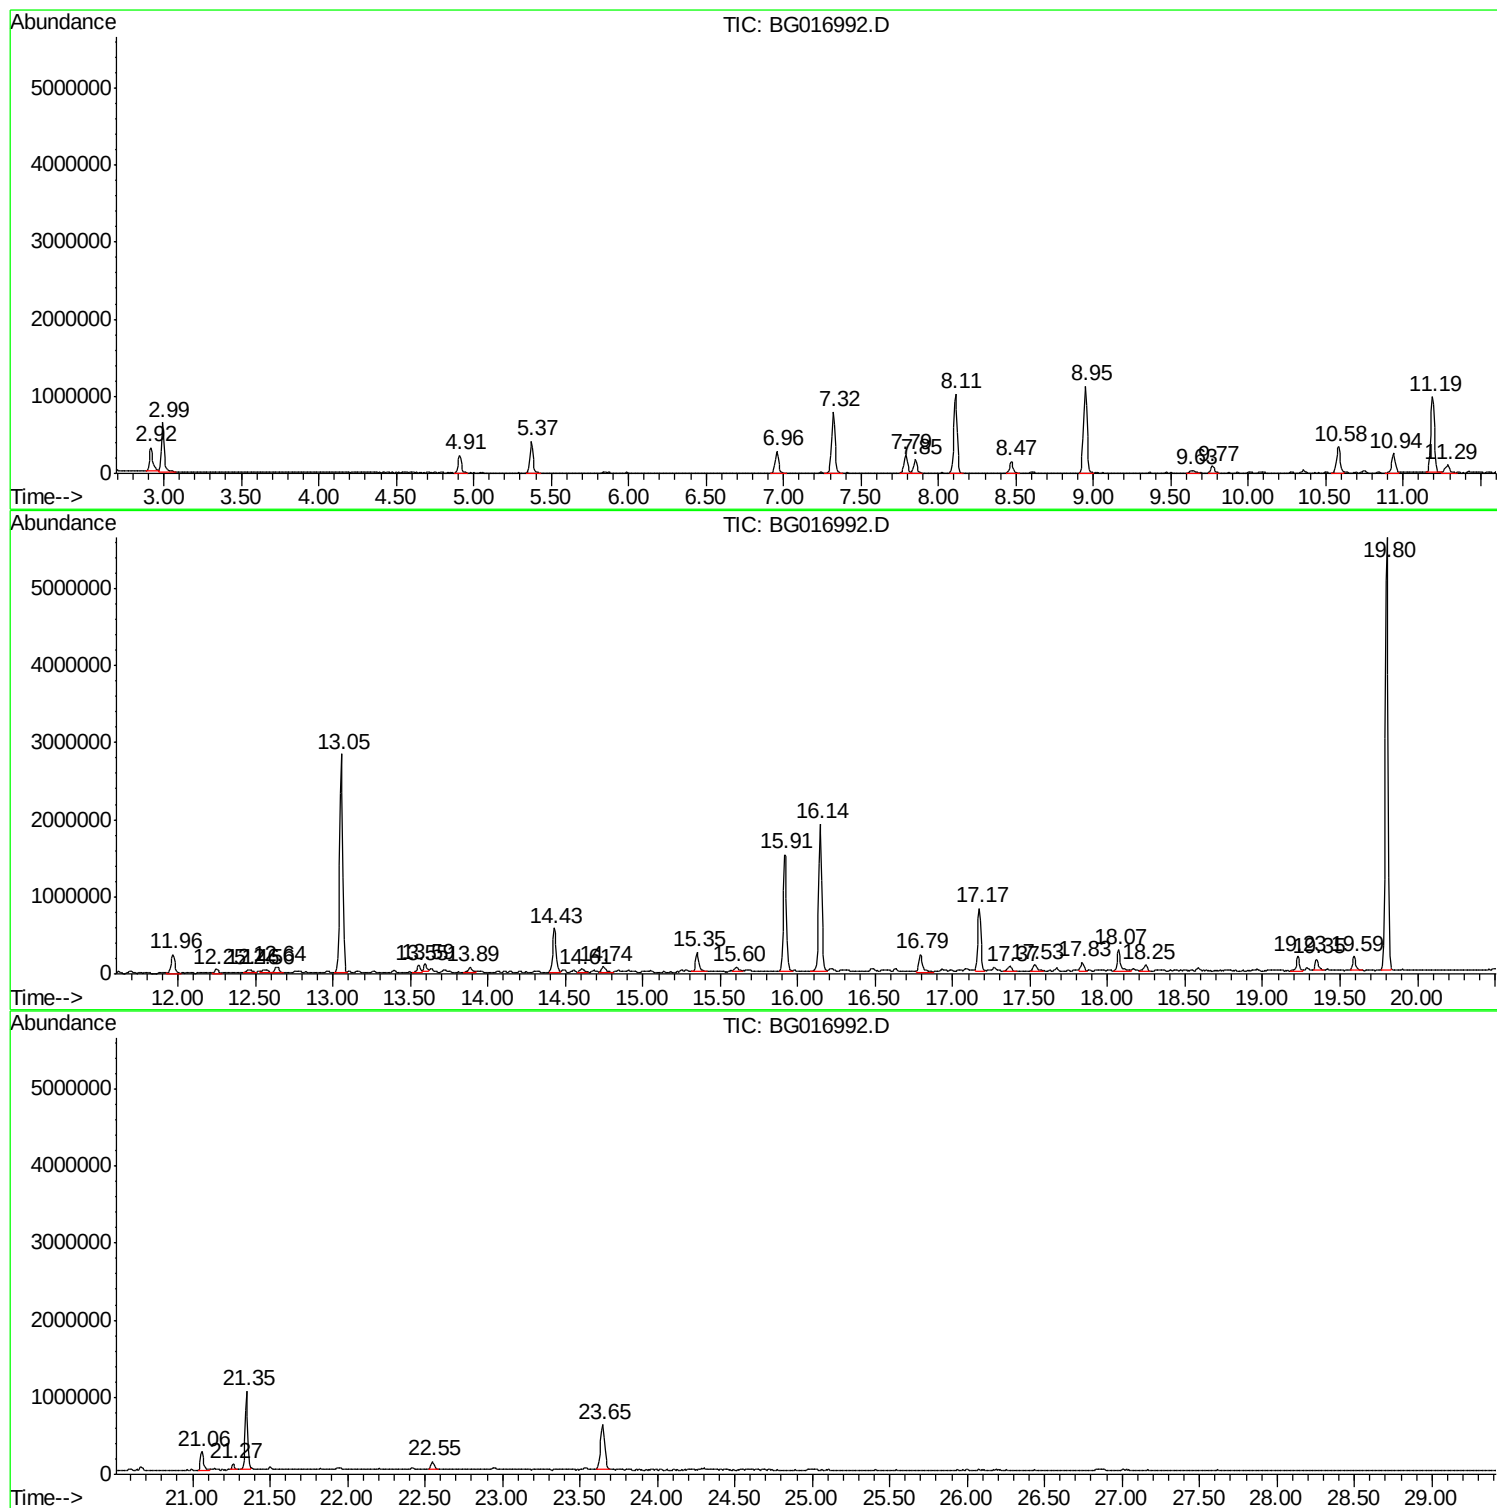

DbaaaPath::ZZ\NRPBHHM1BBAAGCDBAAAB00000155\
 DbaaaFile::BB0000922DD
 AcqQOn :: 99May2005 166534
 Operator::TPPZZ
 Sample::G0280001
 Misc::
 ASSVal::337 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleID :
 WC-CW-02

QqantMebdd::ZZ\NRPBHHM1BBAAGCMEEH00S8270BB0000155MM
 QqantTitle::ASBPBNASSANDABBSF00R55P000NTC6AIBRATION

TICLibrary::CC\DATAABSENDS002LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
