

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG017015.D
 Acq On : 10 May 2015 8:31
 Operator : TP/IZ
 Sample : G2139-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.911	31	38	43	rBV	253518	397914	2.48%	0.843%
2	3.005	50	54	60	rVB	752765	901417	5.61%	1.909%
3	4.697	337	342	351	rVB	141648	198573	1.24%	0.421%
4	4.915	369	379	385	rBV	202223	294444	1.83%	0.624%
5	5.379	452	458	466	rBV	1378067	1962230	12.21%	4.156%
6	5.872	534	542	550	rBV	720187	998616	6.21%	2.115%
7	6.971	718	729	737	rBV	1353118	2126741	13.23%	4.504%
8	7.324	782	789	797	rBV	1450702	2292790	14.26%	4.856%
9	7.788	860	868	875	rBV	279471	424233	2.64%	0.898%
10	8.111	914	923	929	rBV	991815	1536392	9.56%	3.254%
11	8.945	1058	1065	1074	rBV	920664	1494656	9.30%	3.166%
12	9.380	1082	1139	1142	rBV2	1798523	16072841	100.00%	34.041%
13	9.932	1221	1233	1244	rBV3	149202	369897	2.30%	0.783%
14	10.579	1336	1343	1350	rBV	365468	612952	3.81%	1.298%
15	10.755	1365	1373	1380	rBV	228828	377282	2.35%	0.799%
16	13.046	1752	1763	1772	rBV	2113033	3302423	20.55%	6.994%
17	13.781	1885	1888	1901	rBV2	65047	179312	1.12%	0.380%
18	14.427	1992	1998	2006	rVB2	598162	892497	5.55%	1.890%
19	15.913	2245	2251	2262	rBV	2314242	3202278	19.92%	6.782%
20	17.171	2456	2465	2472	rBV2	832102	1223440	7.61%	2.591%
21	19.797	2905	2912	2920	rBV	4600835	5758453	35.83%	12.196%
22	21.342	3170	3175	3183	rBV	1059655	1317578	8.20%	2.791%
23	23.640	3558	3566	3578	rBV	607432	1279261	7.96%	2.709%


Sum of corrected areas: 47216220

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG017015.D
Acq On : 10 May 2015 8:31
Operator : TP/IZ
Sample : G2139-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LAR9794-B

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

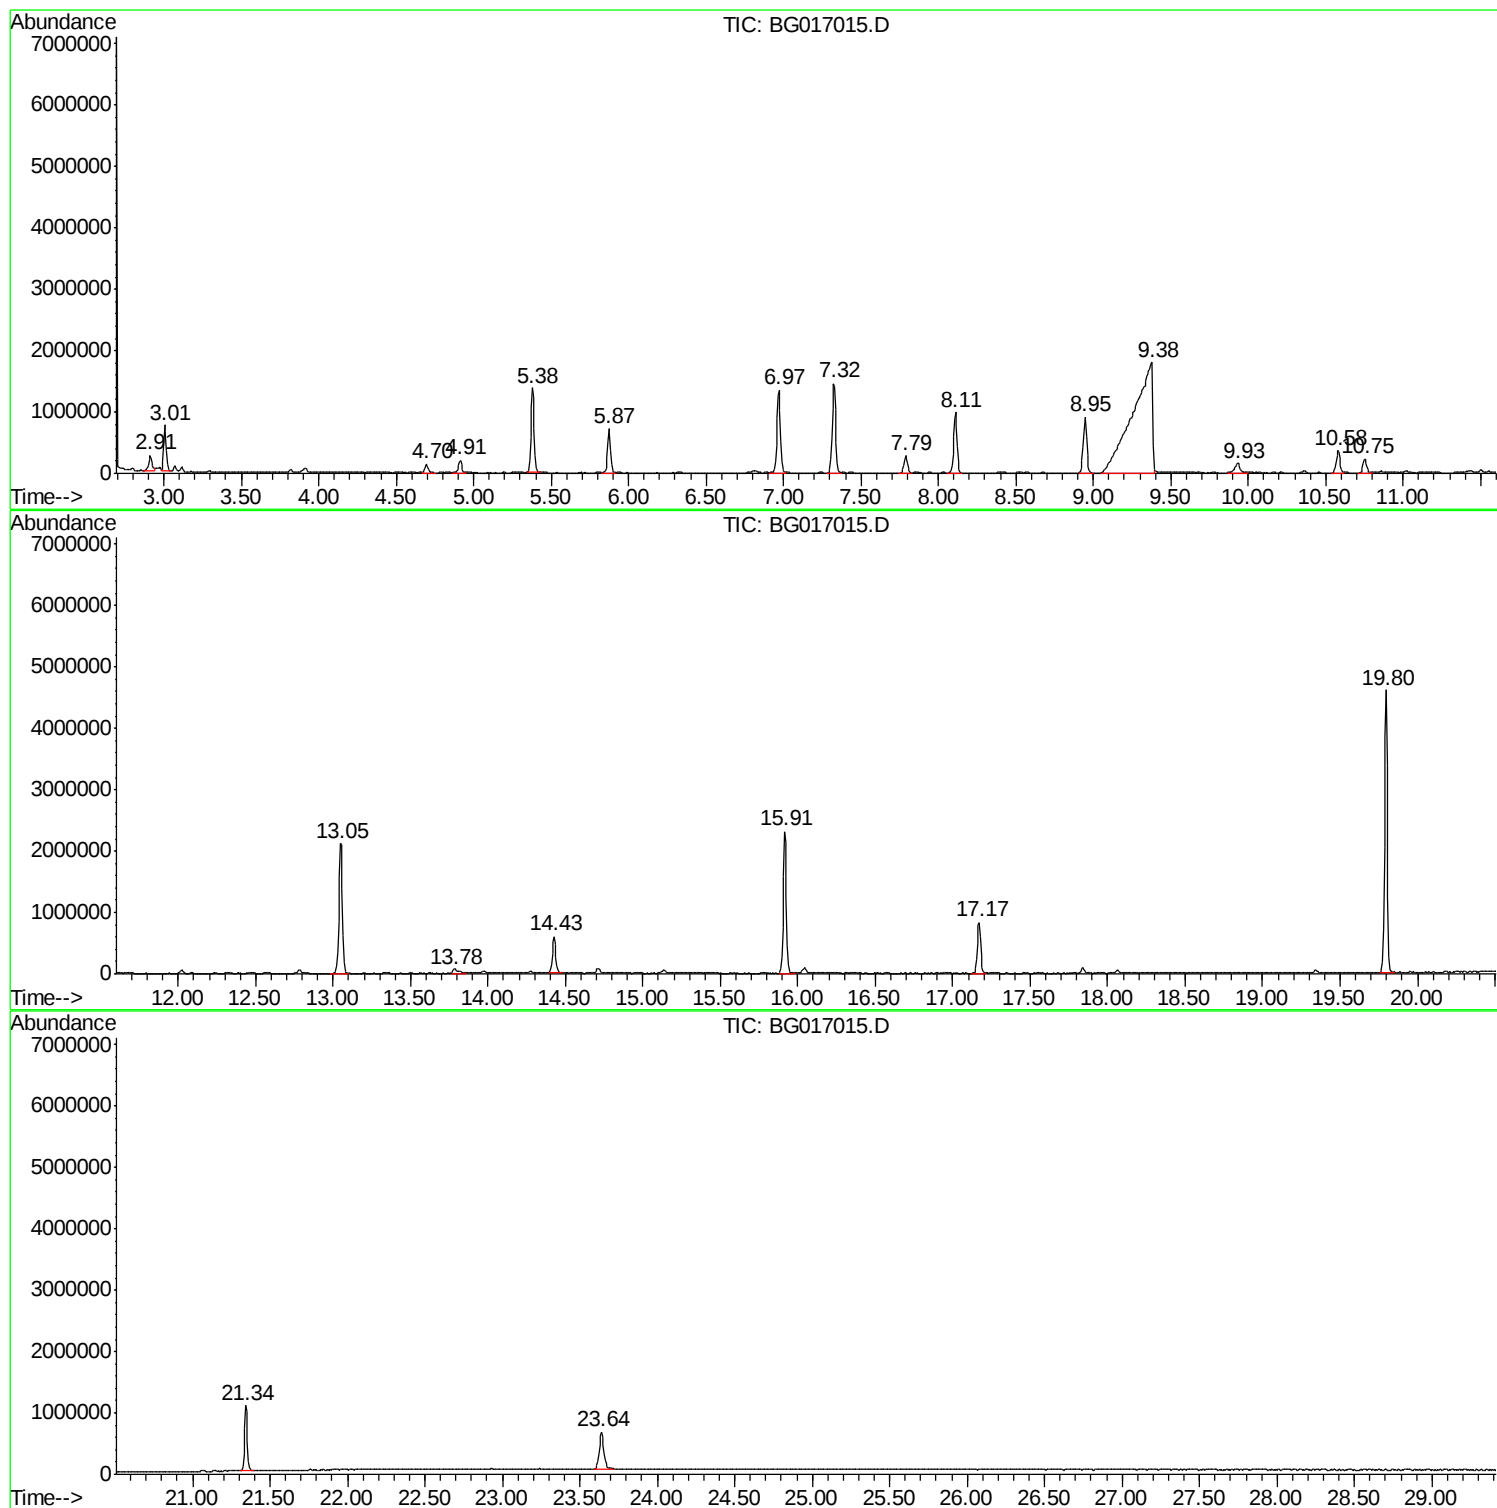

DbaaaPathh::ZZ\NRPBHHM1BBAAGCDBAAABBB0000155\
 DbaaaFile::BB00I0055DD
 Aeqq00n ::100MMay20055 88331
 Oppaaaor ::TPPIZZ
 Samplee ::G02399002
 Misc ::
 AASSVaal ::537 SampleeMMultiplicier:11

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-B

QQaantMebbdd::ZZ\NRPBHHM1BBAAGCMEEH00S88200BB000055MM
 QQaantTife ::ASBPBBNASSANDBBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DATAABBS6EN055002LL
 TICInteggaionPaaaess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
