

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG017016.D
 Acq On : 10 May 2015 9:06
 Operator : TP/IZ
 Sample : G2139-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.914	33	38	49	rVV	250189	435959	7.38%	0.660%
2	3.008	49	54	63	rVB	693391	851846	14.42%	1.289%
3	4.911	371	378	384	rBV2	189674	275451	4.66%	0.417%
4	5.381	451	458	465	rBV	1464357	2096867	35.48%	3.173%
5	5.881	535	543	550	rBV	1875885	2667965	45.15%	4.037%
6	6.815	690	702	709	rBV2	45037	100116	1.69%	0.151%
7	6.968	719	728	742	rVB	1436425	2433132	41.17%	3.682%
8	7.326	781	789	796	rBV	1587925	2465012	41.71%	3.730%
9	7.438	801	808	813	rVB4	41891	78869	1.33%	0.119%
10	7.696	846	852	859	rBV3	31577	66393	1.12%	0.100%
11	7.790	859	868	874	rBV	310346	481382	8.15%	0.728%
12	7.855	874	879	884	rBV	227222	328818	5.56%	0.498%
13	8.037	905	910	917	rBV	264447	465697	7.88%	0.705%
14	8.107	917	922	929	rVB	1041283	1664976	28.18%	2.519%
15	8.372	963	967	972	rVB2	44027	62871	1.06%	0.095%
16	8.442	972	979	986	rBV5	35311	80442	1.36%	0.122%
17	8.766	1025	1034	1046	rBV	250750	557183	9.43%	0.843%
18	8.889	1050	1055	1059	rVV4	70429	111599	1.89%	0.169%
19	8.948	1059	1065	1071	rVV	1006518	1612353	27.29%	2.440%
20	9.012	1071	1076	1081	rVB2	271547	387476	6.56%	0.586%
21	9.089	1084	1089	1095	rBV3	62377	109746	1.86%	0.166%
22	9.659	1179	1186	1191	rBV5	34974	73890	1.25%	0.112%
23	9.764	1199	1204	1207	rBV5	45180	70912	1.20%	0.107%
24	9.858	1211	1220	1224	rVV4	214007	576922	9.76%	0.873%
25	9.929	1224	1232	1236	rVV3	372466	1188403	20.11%	1.798%
26	9.976	1238	1240	1243	rVV2	474521	531517	8.99%	0.804%
27	10.005	1243	1245	1254	rVV	205073	306410	5.19%	0.464%
28	10.111	1258	1263	1267	rVB2	135903	206564	3.50%	0.313%
29	10.358	1300	1305	1310	rBV2	97142	148420	2.51%	0.225%
30	10.558	1332	1339	1349	rBV2	834917	1890152	31.99%	2.860%
31	10.746	1366	1371	1377	rVB2	431064	663608	11.23%	1.004%
32	10.804	1377	1381	1386	rBV5	47465	91326	1.55%	0.138%
33	11.063	1420	1425	1430	rBV8	34609	69976	1.18%	0.106%
34	11.339	1464	1472	1479	rBV3	393924	913630	15.46%	1.382%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG017016.D
 Acq On : 10 May 2015 9:06
 Operator : TP/IZ
 Sample : G2139-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.498	1494	1499	1506	rVB2	133939	214933	3.64%	0.325%
36	11.603	1511	1517	1522	rBV2	118277	200207	3.39%	0.303%
37	11.686	1527	1531	1539	rVB4	86114	170523	2.89%	0.258%
38	11.768	1539	1545	1548	rBV	157423	242402	4.10%	0.367%
39	11.809	1548	1552	1554	rVV2	176727	270575	4.58%	0.409%
40	11.833	1554	1556	1560	rVV	187846	252764	4.28%	0.382%
41	11.874	1560	1563	1568	rVB	174054	250145	4.23%	0.379%
42	12.003	1581	1585	1590	rVB	243045	308447	5.22%	0.467%
43	12.109	1597	1603	1607	rBV	54243	94998	1.61%	0.144%
44	12.238	1616	1625	1632	rVB5	44456	106591	1.80%	0.161%
45	12.549	1675	1678	1686	rVB9	31327	61338	1.04%	0.093%
46	12.784	1710	1718	1722	rBV4	55839	117771	1.99%	0.178%
47	13.049	1752	1763	1770	rBV	2650438	3899329	65.99%	5.900%
48	13.172	1778	1784	1790	rBV8	29046	71256	1.21%	0.108%
49	13.249	1794	1797	1804	rVB3	43100	69252	1.17%	0.105%
50	13.566	1844	1851	1859	rBV	1297636	1992749	33.72%	3.015%
51	13.783	1882	1888	1898	rBV	2312376	4128515	69.86%	6.247%
52	13.971	1916	1920	1927	rBV3	103972	164746	2.79%	0.249%
53	14.053	1930	1934	1942	rBV3	168690	355309	6.01%	0.538%
54	14.277	1969	1972	1977	rVB3	75571	99338	1.68%	0.150%
55	14.324	1977	1980	1986	rVB3	54050	83082	1.41%	0.126%
56	14.429	1992	1998	2008	rVB2	706201	1127148	19.07%	1.706%
57	14.647	2033	2035	2041	rVB7	39714	65149	1.10%	0.099%
58	15.058	2101	2105	2112	rVB2	133867	177127	3.00%	0.268%
59	15.146	2116	2120	2127	rVB3	65324	109427	1.85%	0.166%
60	15.246	2133	2137	2140	rBV	109162	149106	2.52%	0.226%
61	15.276	2140	2142	2146	rVB	148308	159170	2.69%	0.241%
62	15.375	2155	2159	2165	rVB8	51520	92557	1.57%	0.140%
63	15.916	2245	2251	2258	rBV	2333295	3291413	55.70%	4.981%
64	16.045	2265	2273	2278	rVB	505660	842773	14.26%	1.275%
65	16.116	2280	2285	2296	rBV2	207669	390853	6.61%	0.591%
66	16.216	2296	2302	2309	rVV6	111621	261096	4.42%	0.395%
67	16.427	2333	2338	2344	rBV	954128	1178819	19.95%	1.784%
68	16.539	2353	2357	2359	rBV	202031	270181	4.57%	0.409%
69	16.568	2359	2362	2363	rBV	370269	369602	6.25%	0.559%
70	16.633	2370	2373	2377	rVB	118031	144462	2.44%	0.219%
71	16.739	2387	2391	2400	rVB	114883	164137	2.78%	0.248%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
 Data File : BG017016.D
 Acq On : 10 May 2015 9:06
 Operator : TP/IZ
 Sample : G2139-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	16.903	2415	2419	2421	rBV3	90103	116656	1.97%	0.177%
73	16.927	2421	2423	2427	rVB	93334	116402	1.97%	0.176%
74	17.173	2459	2465	2470	rBV	861451	1232240	20.85%	1.865%
75	17.291	2482	2485	2490	rVB2	125817	147519	2.50%	0.223%
76	17.455	2510	2513	2520	rVB2	130787	182788	3.09%	0.277%
77	17.667	2546	2549	2553	rBV	94696	106628	1.80%	0.161%
78	17.843	2574	2579	2583	rVB	475348	604361	10.23%	0.915%
79	18.066	2614	2617	2622	rBV	215557	251198	4.25%	0.380%
80	18.360	2663	2667	2671	rBV	156667	200225	3.39%	0.303%
81	18.824	2743	2746	2753	rBV3	120975	184829	3.13%	0.280%
82	18.995	2772	2775	2780	rBV	151152	236440	4.00%	0.358%
83	19.153	2799	2802	2805	rBV2	173190	186646	3.16%	0.282%
84	19.230	2809	2815	2818	rBV3	287084	556018	9.41%	0.841%
85	19.283	2822	2824	2829	rVB3	174751	207661	3.51%	0.314%
86	19.341	2829	2834	2836	rBV4	173151	342046	5.79%	0.518%
87	19.747	2900	2903	2904	rBV3	218694	242737	4.11%	0.367%
88	19.800	2905	2912	2917	rVB	4192301	5909280	100.00%	8.942%
89	20.105	2962	2964	2968	rVB	361436	413162	6.99%	0.625%
90	20.287	2991	2995	3001	rBV2	653121	1358282	22.99%	2.055%
91	20.769	3074	3077	3081	rBV2	555853	736884	12.47%	1.115%
92	21.216	3149	3153	3158	rBV	1471240	2507264	42.43%	3.794%
93	21.345	3172	3175	3184	rVB	1074355	1668992	28.24%	2.525%
94	21.645	3222	3226	3233	rVB2	1375481	2564326	43.39%	3.880%


Sum of corrected areas: 66085757

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG017016.D
Acq On : 10 May 2015 9:06
Operator : TP/IZ
Sample : G2139-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LAR9794-C

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

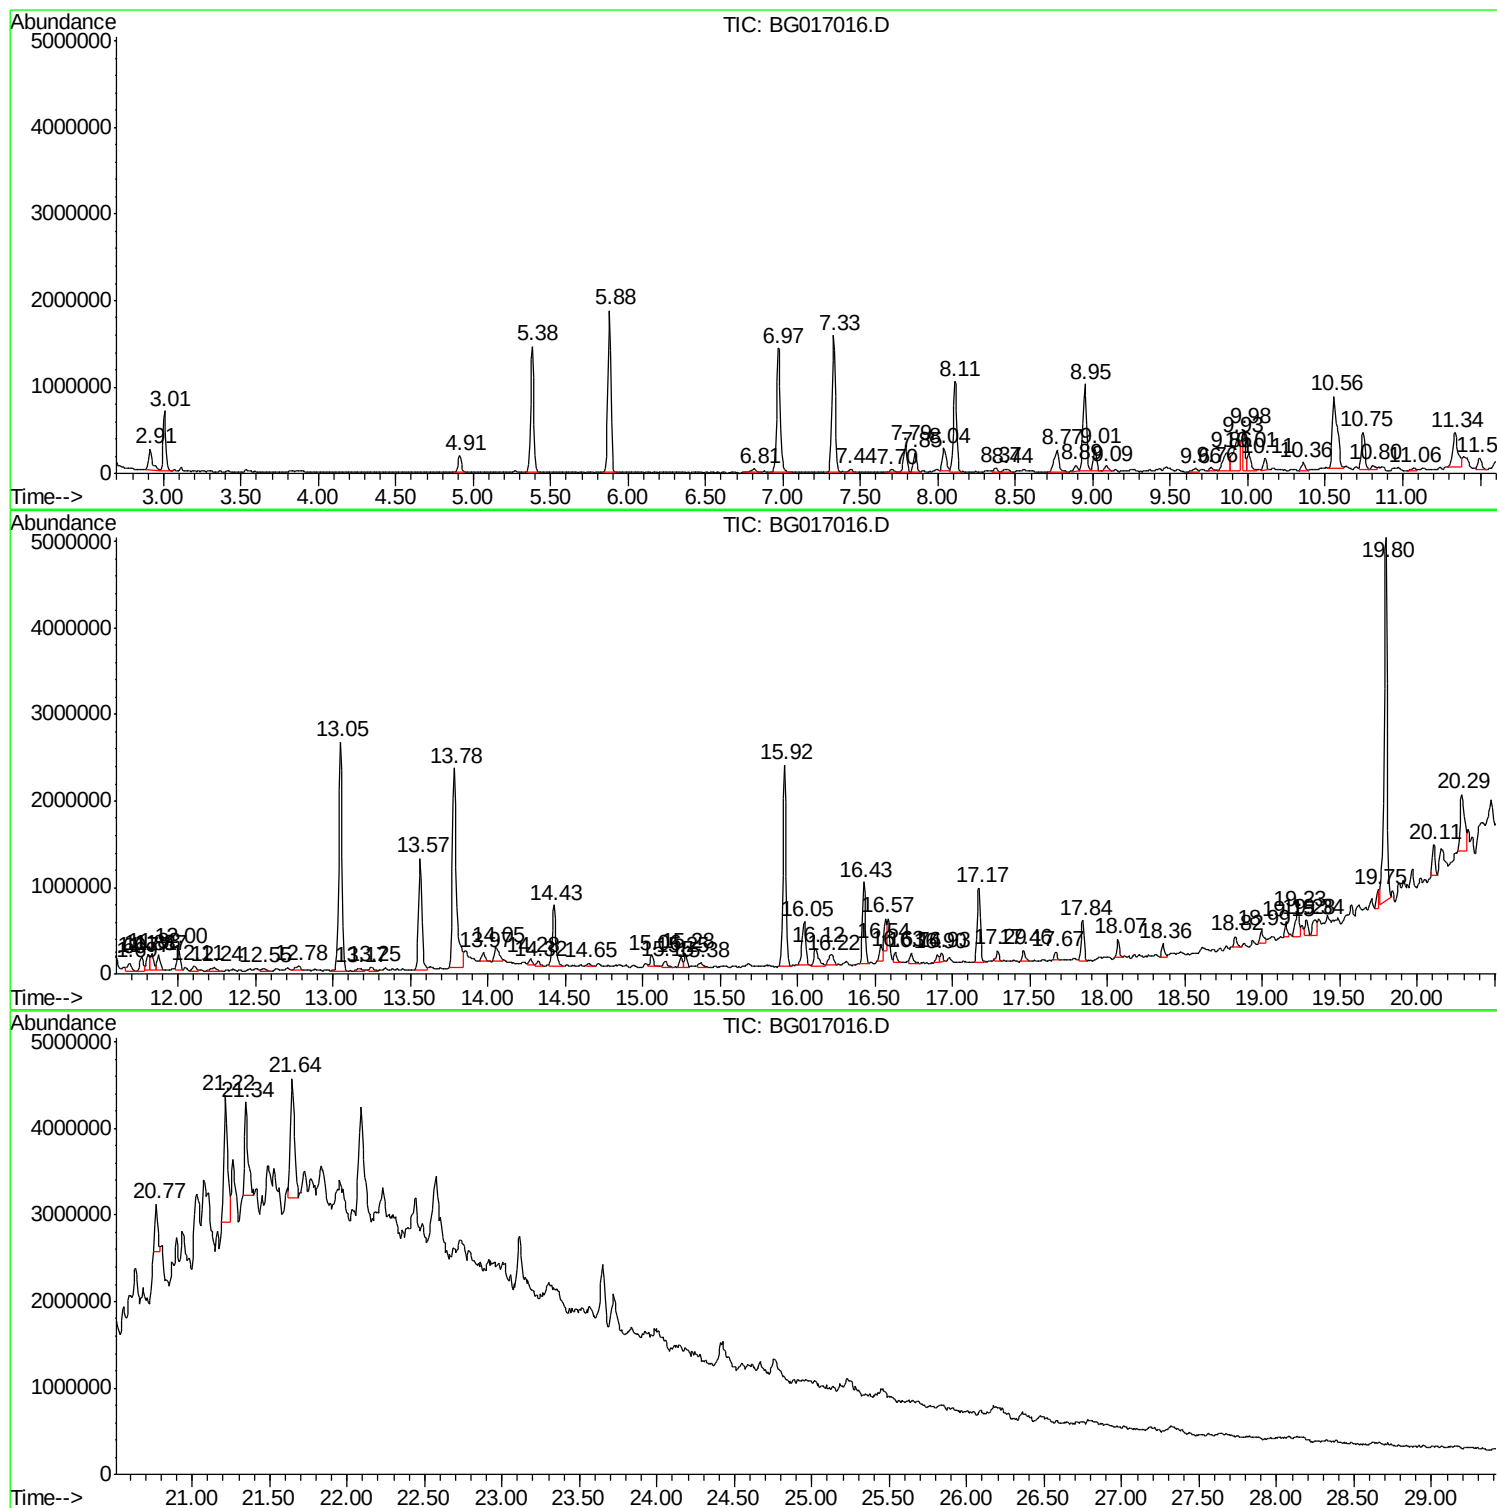

DbaaaPath::ZZ\NRPBHHM1BBAAGCDBAA\BB0000015\
 DbaaaFile::BB00I0066DD
 AcqQOn::100MHz20055 99006
 Operator::TPP11Z
 Sample::G02399003
 Misc::
 ASSVAl::588 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 LAR9794-C

QqantMebdd::ZZ\NRPBHHM1BBAAGCMEEH00S82Z00BB000015MM
 QqantTitle::ASBPBNASSANDARBSF00R55P000NTC6AIBRATION

TICLibrary::CC\DATA\BBS6EN0\$S002LL
 TICIntegratIonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
