


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050915\
Data File : BG016987.D
Acq On : 9 May 2015 12:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 05 16:13:58 2015

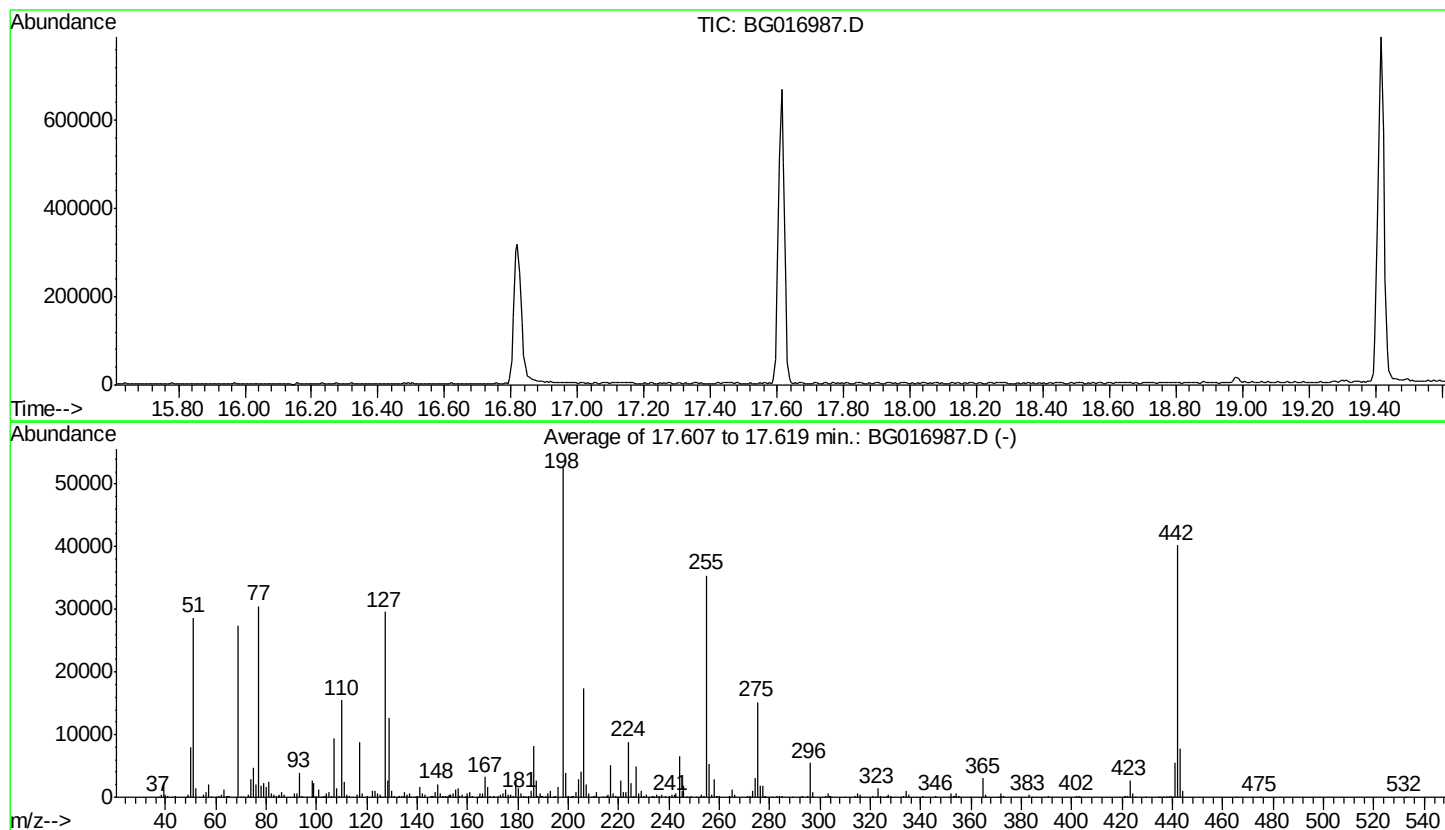

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	28709	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.9	27474	PASS
70	69	0.00	2	0.4	106	PASS
127	198	10	80	55.9	29605	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52930	PASS
199	198	5	9	7.4	3930	PASS
275	198	10	60	28.6	15133	PASS
365	198	1	100	5.6	2975	PASS
441	442	0.01	24	13.7	5499	PASS
442	198	50	100	75.9	40173	PASS
443	442	15	24	19.2	7706	PASS