

Data File : BG026931.D
Acq On : 10 May 2017 3:32
Operator : SJ/MA
Sample : I2884-01 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAB34

Quant Time: May 10 04:08:59 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 10 01:49:01 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	203097	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	977386	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.61	164	508315	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	909797	20.00	ng/ul	0.00
75) Chrysene-d12	21.59	240	829395	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	893105	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	2445	0.54	ng/uL	0.00
5) Phenol-d5	7.19	99	57321	3.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	35414	3.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	48218	3.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	48762	3.24	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	25913	3.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	23906	2.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	40163	2.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	12589	0.67	ng/ul	0.01
43) Dimethylphthalate-d6	14.02	166	129692	3.17	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	177950	3.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	61	0.01	ng/ul	-0.03
57) Fluorene-d10	15.60	176	113710	3.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.74	200	2751	0.50	ng/ul	0.00
70) Anthracene-d10	17.45	188	158398	3.59	ng/ul	0.00
76) Pyrene-d10	19.73	212	149297	3.41	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	142537	3.38	ng/ul	0.00

Target Compounds

						Qvalue
44) Dimethylphthalate	14.06	163	51831	1.29	ng/ul	99
69) Phenanthrene	17.39	178	334866	6.53	ng/ul	99
74) Fluoranthene	19.40	202	319978	6.72	ng/ul#	80
77) Pyrene	19.76	202	308812	5.55	ng/ul#	75
80) Benzo(a)anthracene	21.58	228	113652	2.34	ng/ul	98
82) Chrysene	21.64	228	140359	3.11	ng/ul	95
85) Benzo(b)fluoranthene	23.76	252	136916	2.68	ng/ul#	72
88) Benzo(a)pyrene	24.61	252	108838	2.17	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026931.D

Acq On : 10 May 2017 3:32

Operator : SJ/MA

Sample : I2884-01 5X

Misc :

ALS Vial : 26 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

YAB34


Quant Time: May 10 04:08:59 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 10 01:49:01 2017

Response via : Initial Calibration

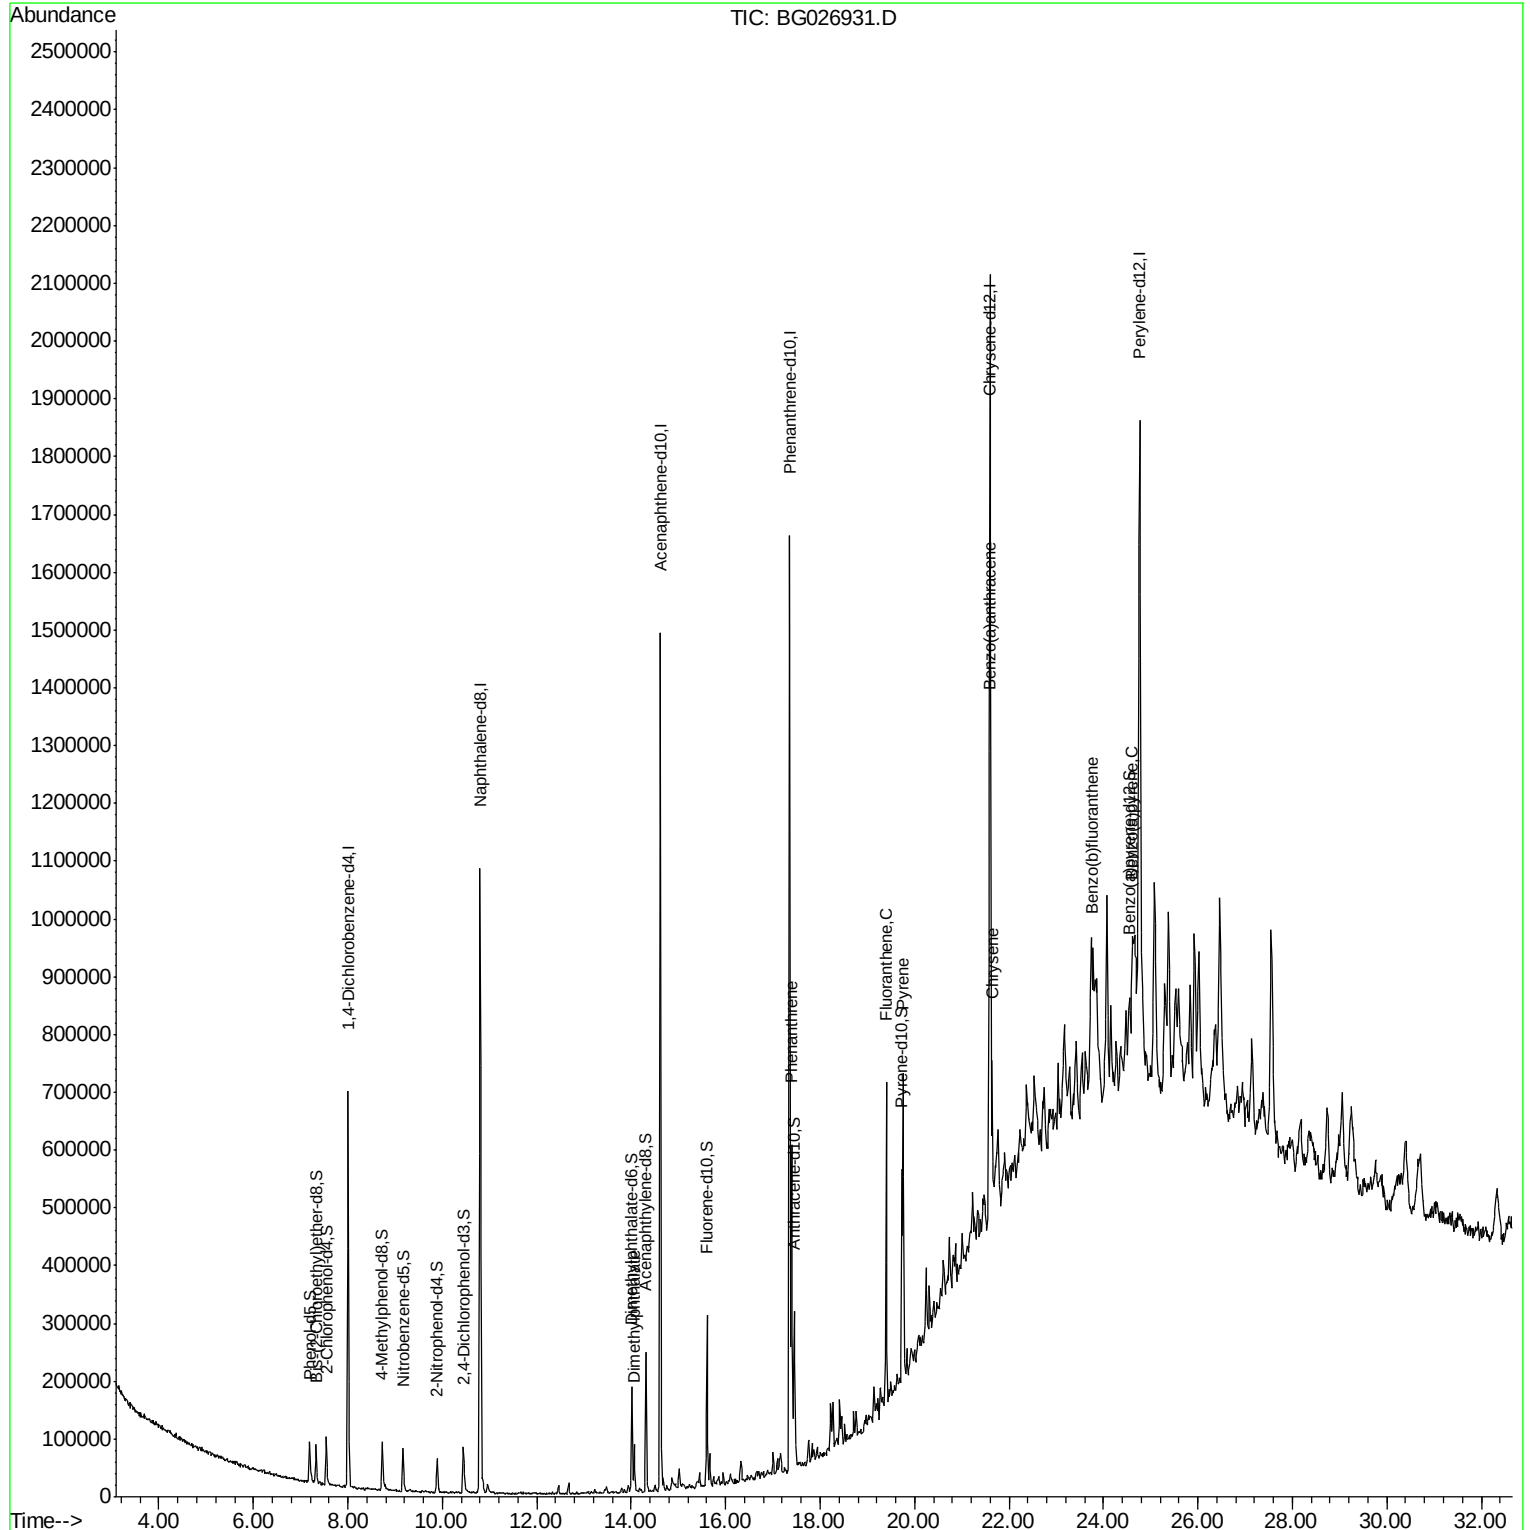


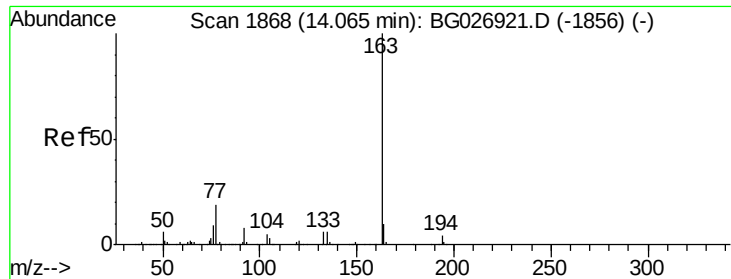




#44
Dimethylphthalate
Concen: 1.29 ng/ul
RT: 14.06 min Scan# 1868
Delta R.T. -0.00 min
Lab File: BG026931.D
Acq: 10 May 2017 3:32

Instrument :
BNA_G
ClientSampleId :
YAB34

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.4	5.0
164	11.1	9.0	13.4

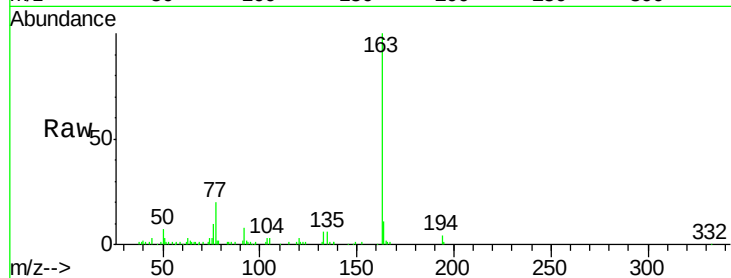


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

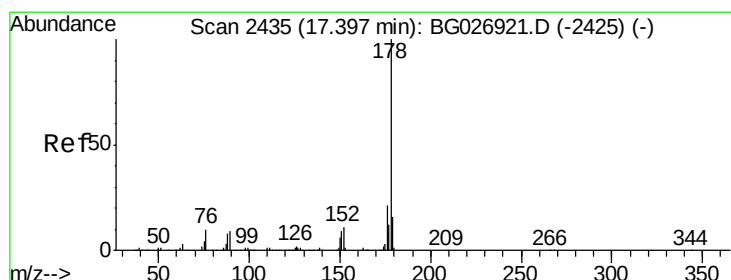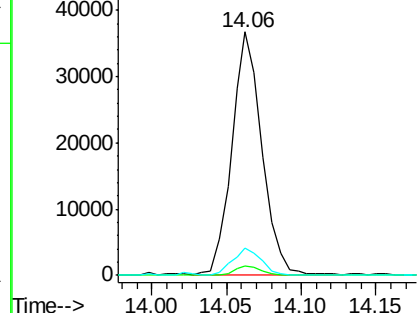
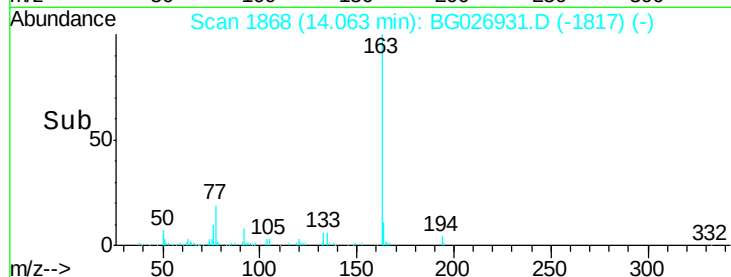



#69
Phenanthrene
Concen: 6.53 ng/ul
RT: 17.39 min Scan# 2435
Delta R.T. -0.00 min
Lab File: BG026931.D
Acq: 10 May 2017 3:32

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.4	18.6
176	19.7	16.5	24.7

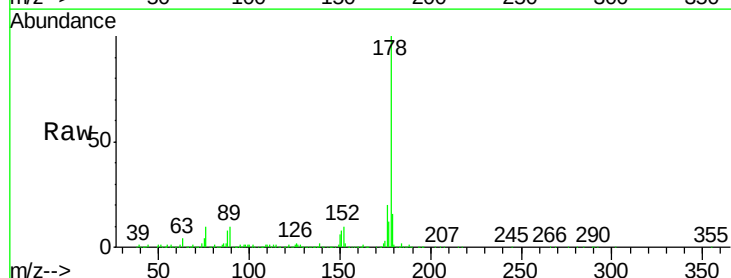

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

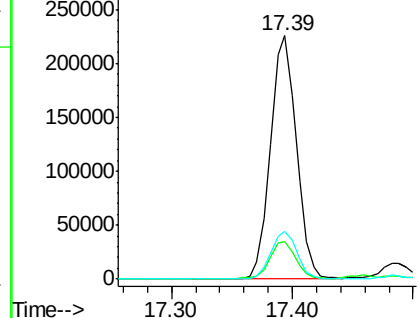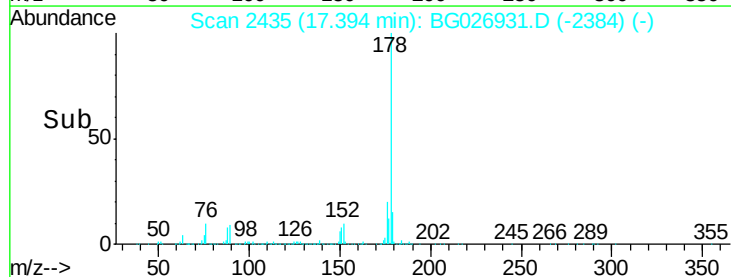

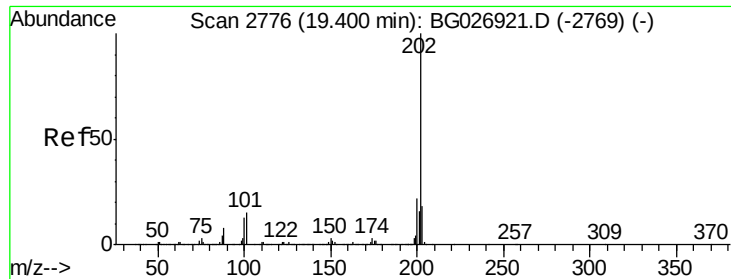

#74

Fluoranthene

Concen: 6.72 ng/ul

RT: 19.40 min Scan# 2776

Delta R.T. -0.00 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32

Instrument :

BNA_G

ClientSampleId :

YAB34


Tgt Ion:202 Resp: 319978

Ion Ratio Lower Upper

202 100

101 15.3 6.2 9.2#




100 12.4 5.2 7.8#

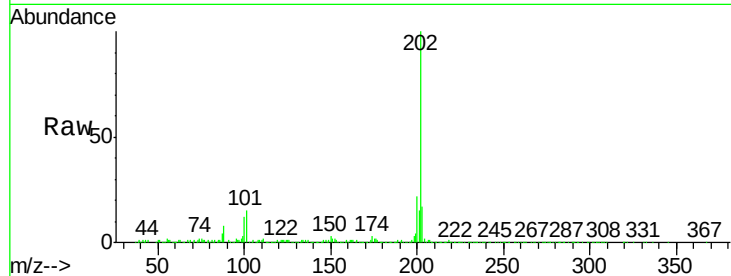

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

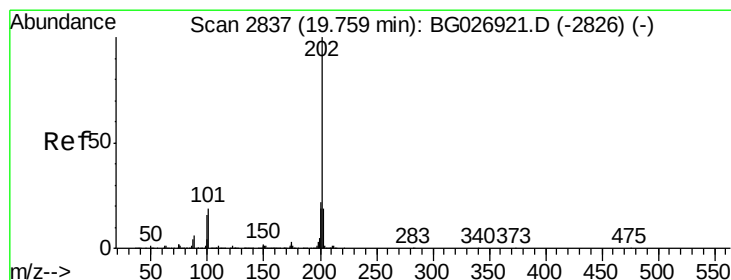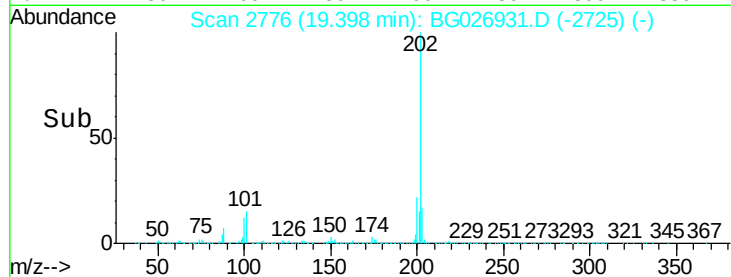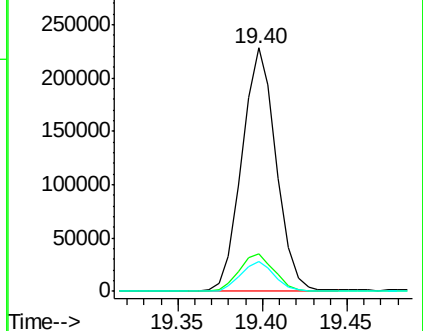

#77

Pyrene

Concen: 5.55 ng/ul

RT: 19.76 min Scan# 2837

Delta R.T. -0.00 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32


Tgt Ion:202 Resp: 308812

Ion Ratio Lower Upper

202 100

101 19.2 6.9 10.3#



100 15.4 6.6 10.0#

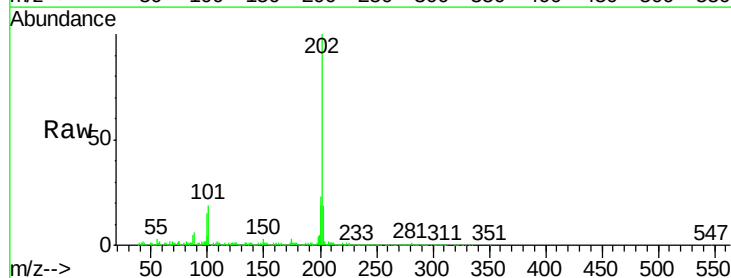


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

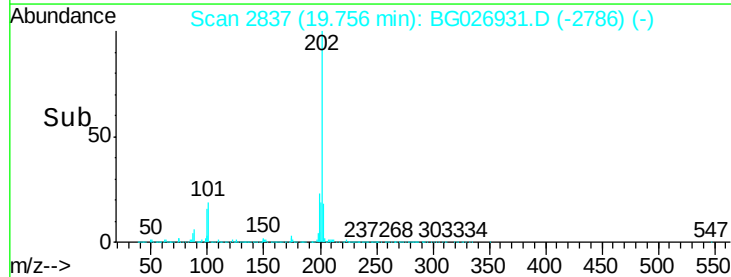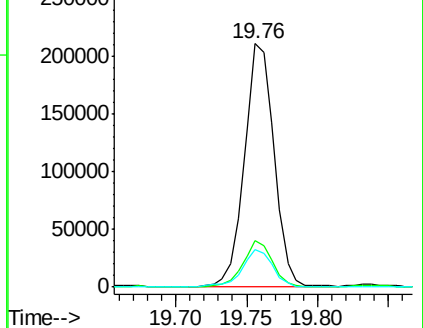

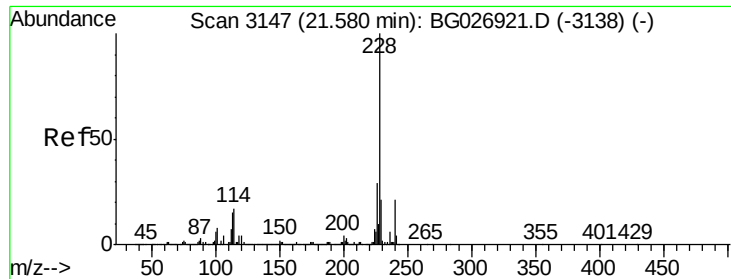

#80

Benzo(a)anthracene

Concen: 2.34 ng/ul

RT: 21.58 min Scan# 3147

Delta R.T. -0.00 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32

Instrument :

BNA_G

ClientSampled :

YAB34


Tgt Ion:228 Resp: 113652

Ion Ratio Lower Upper

228 100

229 21.1 16.3 24.5




226 28.6 21.9 32.9

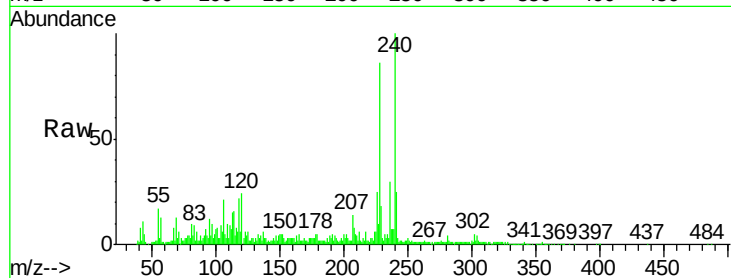

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

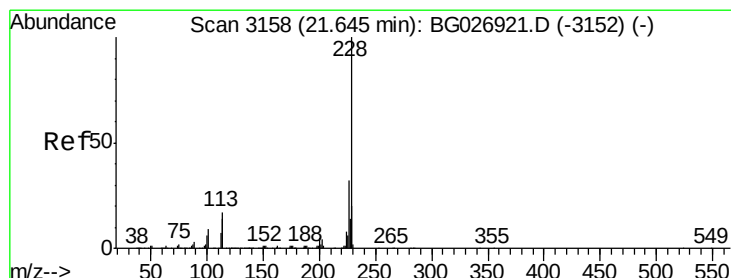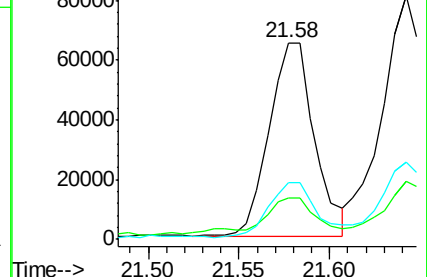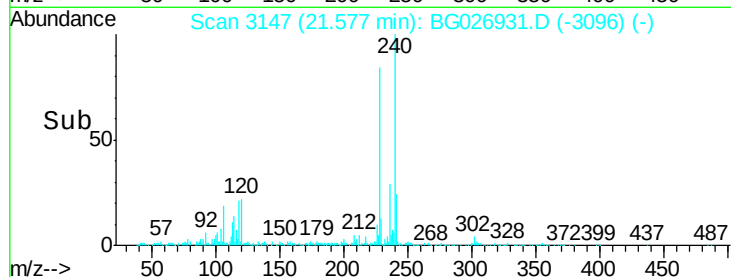

#82

Chrysene

Concen: 3.11 ng/ul

RT: 21.64 min Scan# 3158

Delta R.T. -0.00 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32


Tgt Ion:228 Resp: 140359

Ion Ratio Lower Upper

228 100

226 32.0 24.0 36.0



229 23.8 16.9 25.3

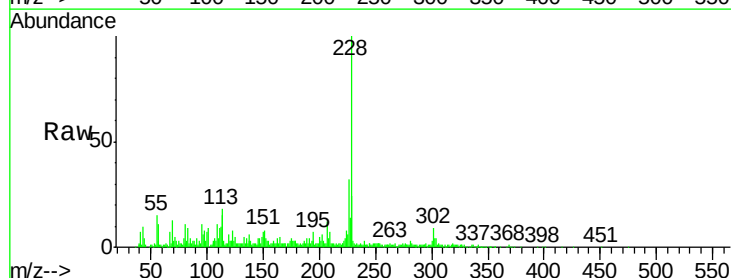


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

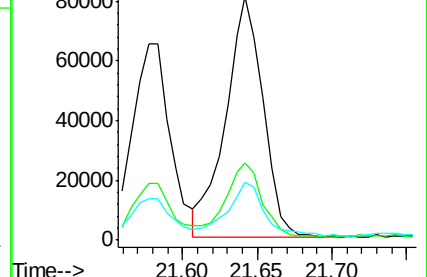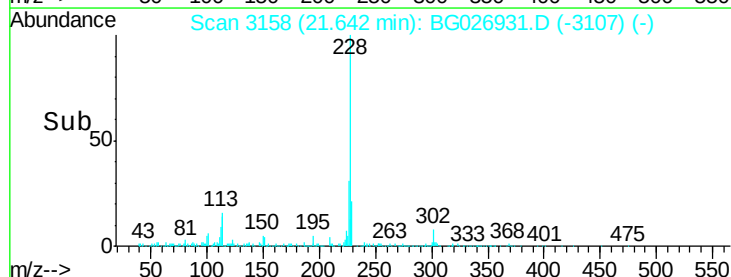

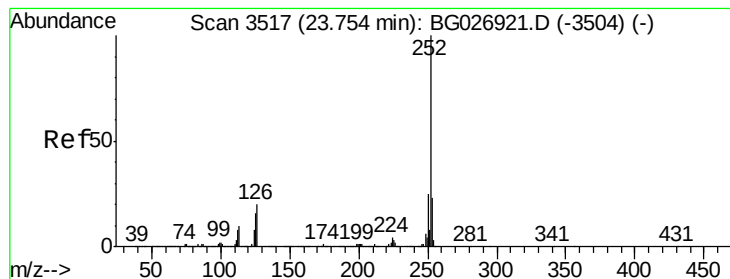

#85

Benzo(b)fluoranthene

Concen: 2.68 ng/ul

RT: 23.76 min Scan# 3519

Delta R.T. 0.01 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32

Instrument :

BNA_G

ClientSampleId :

YAB34


Tgt Ion:252 Resp: 136916

Ion Ratio Lower Upper

252 100

253 30.1 17.7 26.5#




125 30.5 4.0 6.0#

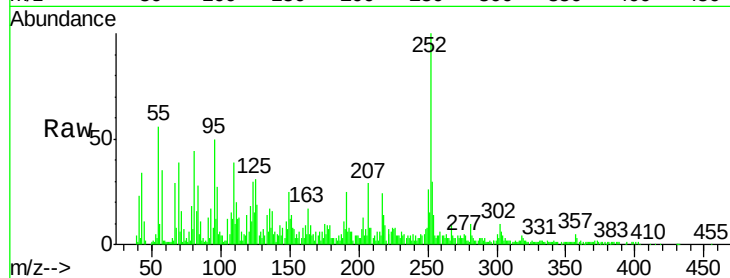

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

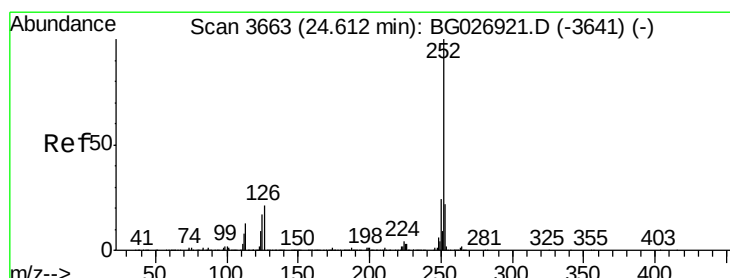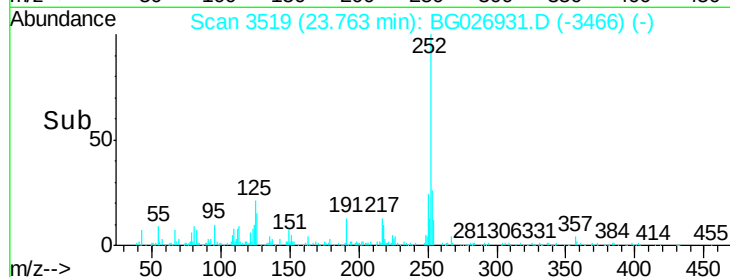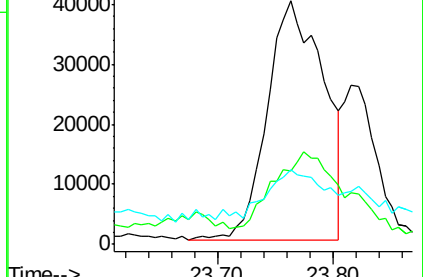

#88

Benzo(a)pyrene

Concen: 2.17 ng/ul

RT: 24.61 min Scan# 3663

Delta R.T. -0.00 min

Lab File: BG026931.D

Acq: 10 May 2017 3:32


Tgt Ion:252 Resp: 108838

Ion Ratio Lower Upper

252 100

253 25.1 17.8 26.6

125 27.1 5.4 8.0#

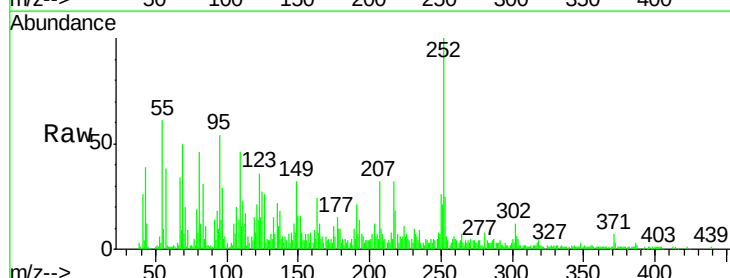

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

