

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
 Data File : BG053501.D
 Acq On : 9 May 2022 20:19
 Operator : CG/JU
 Sample : N2739-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 124035

Quant Time: May 10 03:03:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 05 02:13:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.090	152	28636	20.000	ng	0.00
21) Naphthalene-d8	10.898	136	110928	20.000	ng	#-0.02
39) Acenaphthene-d10	14.710	164	81283	20.000	ng	0.00
64) Phenanthrene-d10	17.454	188	189290	20.000	ng	-0.01
76) Chrysene-d12	21.736	240	203295	20.000	ng	0.00
86) Perylene-d12	25.014	264	208405	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.658	112	197905	117.290	ng	0.00
7) Phenol-d6	7.250	99	281476	109.919	ng	0.00
23) Nitrobenzene-d5	9.253	82	201698	77.401	ng	0.00
42) 2,4,6-Tribromophenol	16.202	330	125980	105.086	ng	0.00
45) 2-Fluorobiphenyl	13.336	172	398246	71.595	ng	0.00
79) Terphenyl-d14	20.056	244	702442	64.354	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propyla...	9.247	70	28530	15.528	ng	# 75
51) 2,6-Dinitrotoluene	14.710	165	10408	8.271	ng	# 19
57) 2,4-Dinitrotoluene	14.710	165	10408	5.706	ng	# 24
67) 4-Bromophenyl-phenylether	16.202	248	7785	3.522	ng	# 1
75) Fluoranthene	19.504	202	36247	2.908	ng	96
77) Benzidine	20.056	184	11766	2.685	ng	# 95
78) Pyrene	19.868	202	33318	2.532	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
Data File : BG053501.D
Acq On : 9 May 2022 20:19
Operator : CG/JU
Sample : N2739-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
124035

Quant Time: May 10 03:03:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration




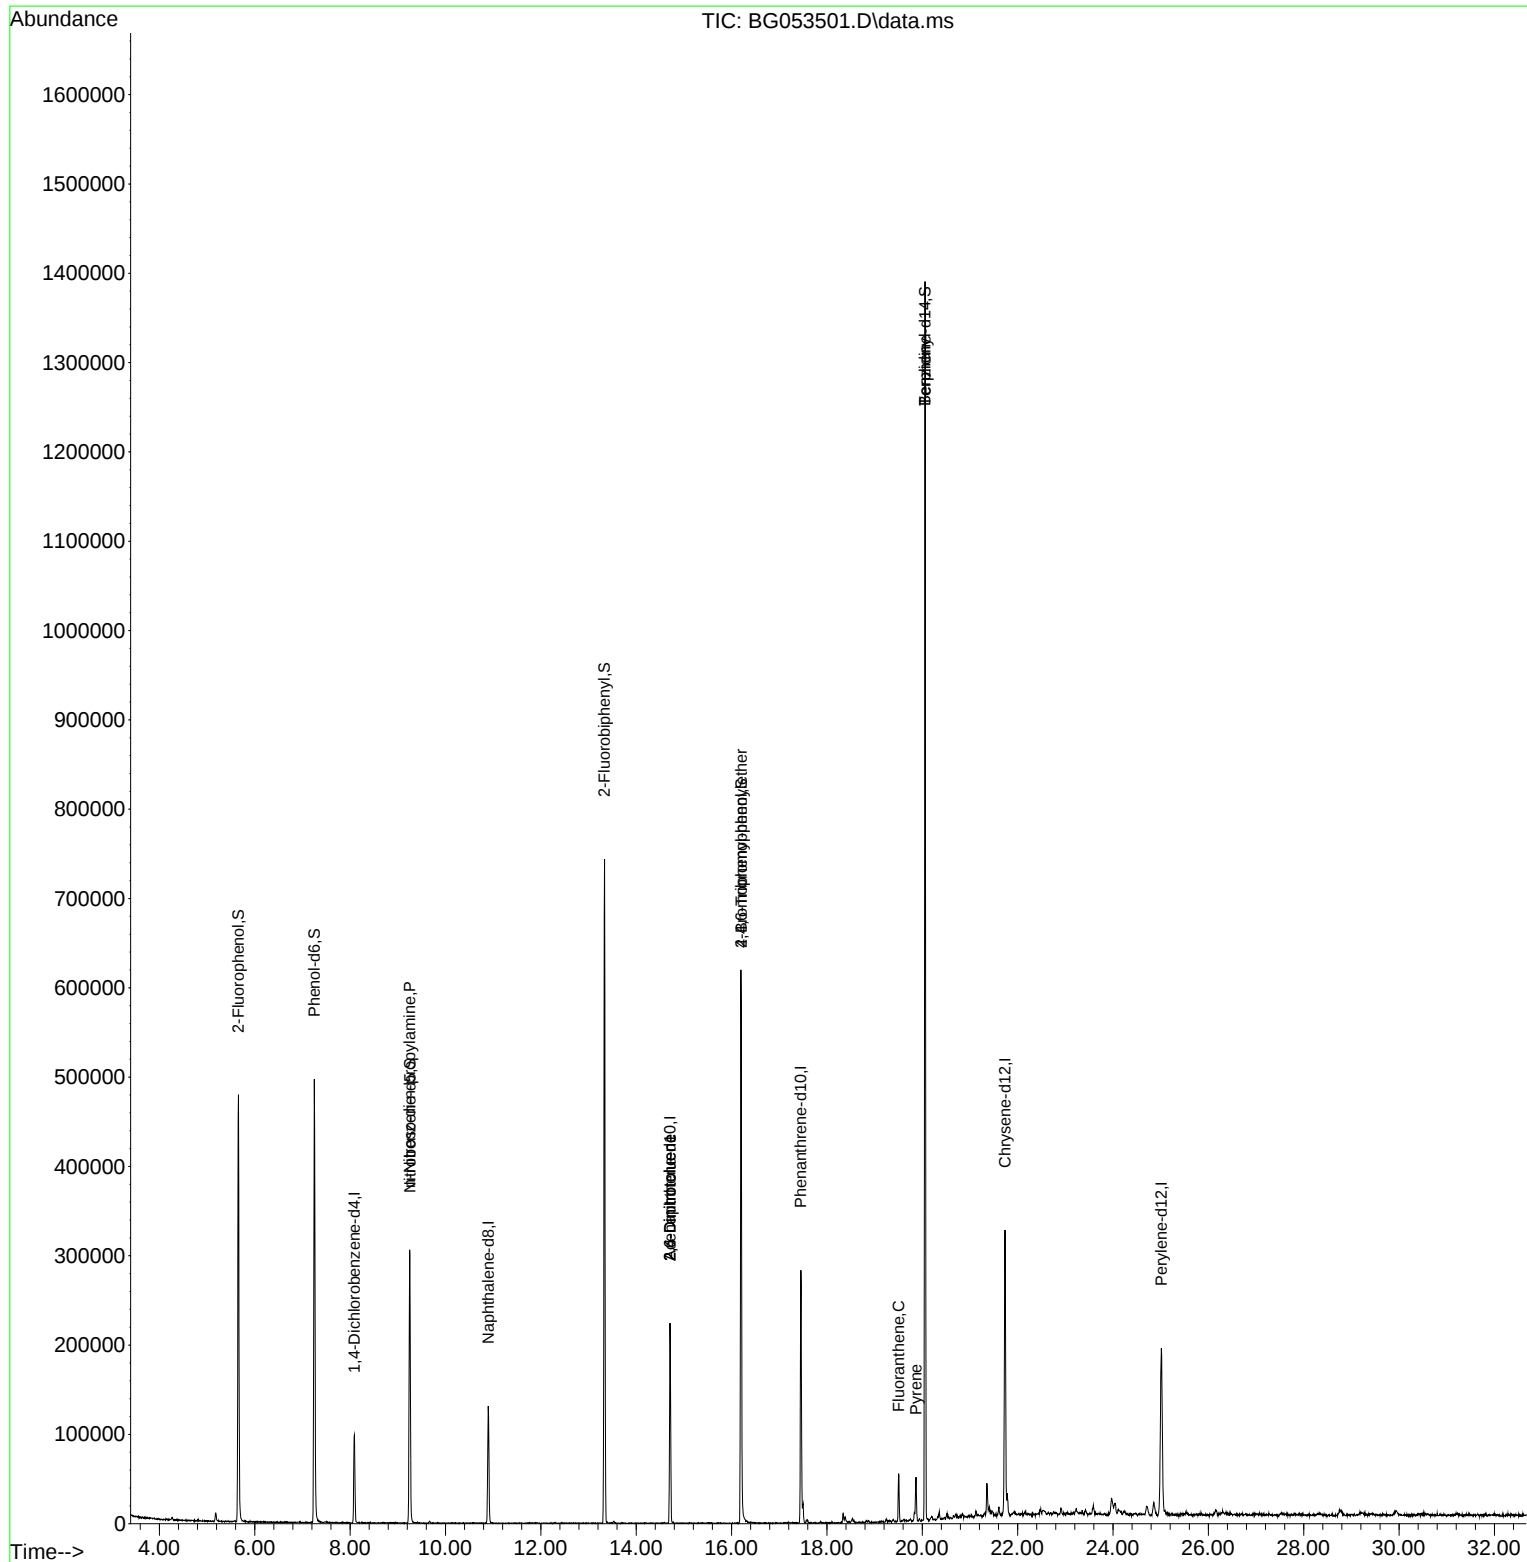




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.090 min Scan# 80
Delta R.T. -0.009 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19




Instrument :
BNA_G
ClientSampleId :
124035

Tgt Ion:152 Resp: 28636
Ion Ratio Lower Upper
152 100
150 150.2 131.6 197.4
115 58.4 50.9 76.3

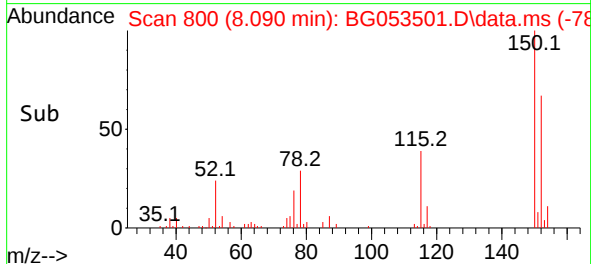

#5
2-Fluorophenol
Concen: 117.290 ng
RT: 5.658 min Scan# 386
Delta R.T. -0.009 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Tgt Ion:112 Resp: 197905
Ion Ratio Lower Upper
112 100
64 70.1 55.1 82.7
63 39.1 30.4 45.6

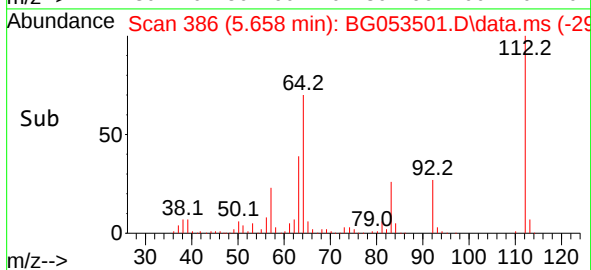

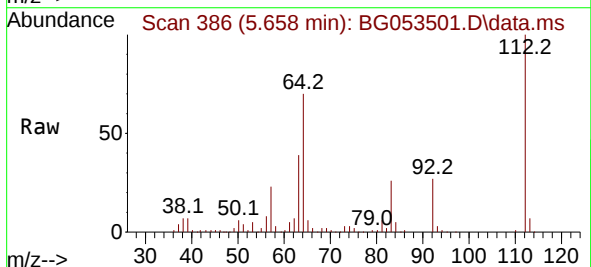




#7
Phenol-d6
Concen: 109.919 ng
RT: 7.250 min Scan# 61
Delta R.T. -0.009 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19




Instrument :
BNA_G
ClientSampleId :
124035


Tgt Ion: 99 Resp: 281476
Ion Ratio Lower Upper
99 100
42 20.2 17.0 25.6
71 42.5 33.8 50.8

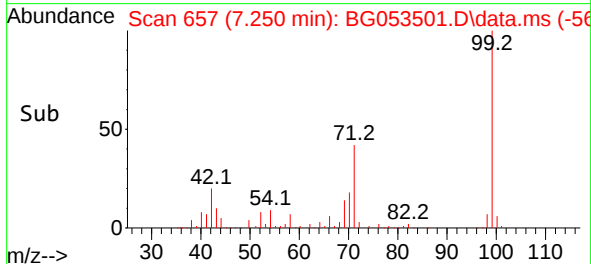

#19
n-Nitroso-di-n-propylamine
Concen: 15.528 ng
RT: 9.247 min Scan# 997
Delta R.T. 0.350 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Tgt Ion: 70 Resp: 28530
Ion Ratio Lower Upper
70 100
42 42.9 47.3 70.9#
101 0.0 7.0 10.4#
130 1.6 14.6 22.0#


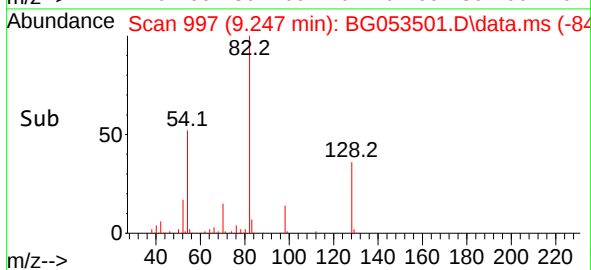

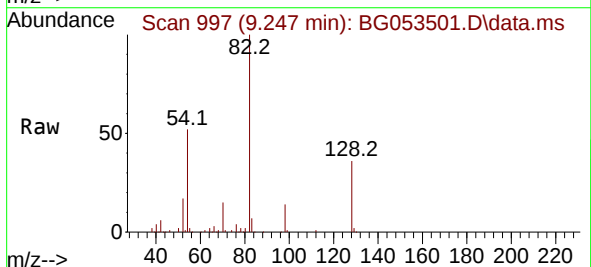




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.898 min Scan# 110928
Delta R.T. -0.015 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19




Instrument :
BNA_G
ClientSampleId :
124035


Tgt Ion:	136	Resp:	110928
Ion	Ratio	Lower	Upper
136	100		
137	12.9	8.5	12.7#
54	10.0	7.4	11.2
68	6.3	4.9	7.3

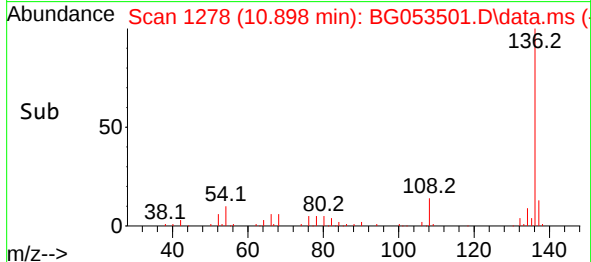

#23
Nitrobenzene-d5
Concen: 77.401 ng
RT: 9.253 min Scan# 998
Delta R.T. -0.009 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Tgt Ion:	82	Resp:	201698
Ion	Ratio	Lower	Upper
82	100		
128	34.2	27.9	41.9
54	48.6	41.2	61.8

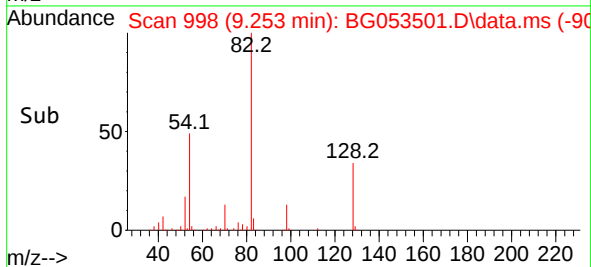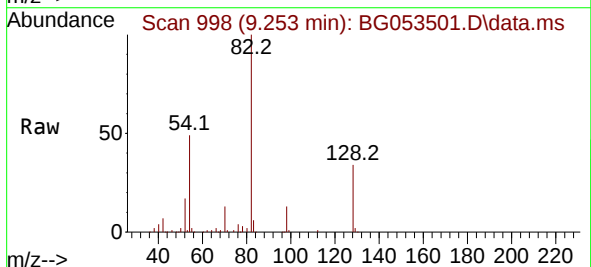



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.710 min Scan# 1929

Delta R.T. -0.009 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19

Instrument :

BNA_G

ClientSampleId :

124035





Tgt Ion:164 Resp: 81283

Ion Ratio Lower Upper

164 100

162 100.5 82.3 123.5

160 43.2 34.2 51.2

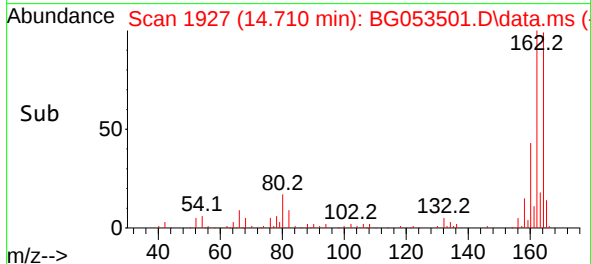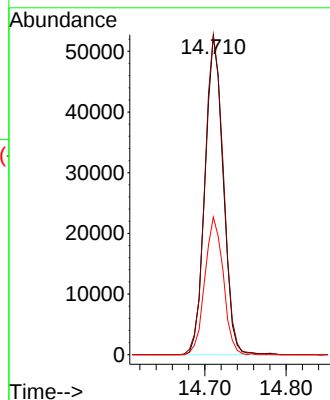

#42

2,4,6-Tribromophenol

Concen: 105.086 ng

RT: 16.202 min Scan# 2181

Delta R.T. -0.009 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19




Tgt Ion:330 Resp: 125980


Ion Ratio Lower Upper

330 100

332 97.2 76.0 114.0

141 34.7 27.1 40.7

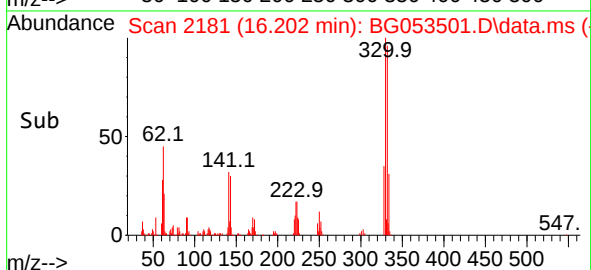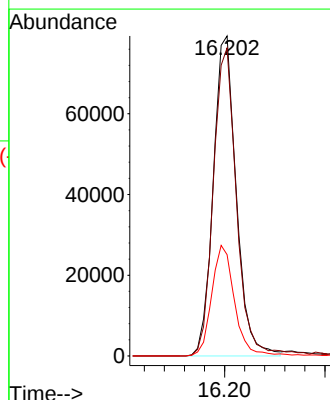



#45

2-Fluorobiphenyl

Concen: 71.595 ng

RT: 13.336 min Scan# 1

Delta R.T. -0.009 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19

Instrument :

BNA_G

ClientSampleId :

124035





Tgt Ion:172 Resp: 398246

Ion Ratio Lower Upper

172 100

171 33.0 28.5 42.7

170 23.3 18.9 28.3

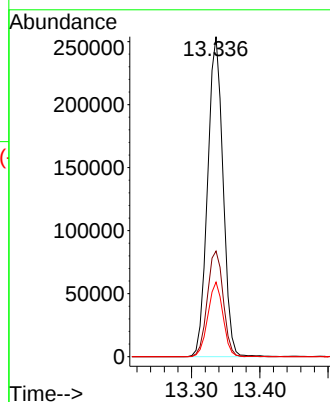

#51

2,6-Dinitrotoluene

Concen: 8.271 ng

RT: 14.710 min Scan# 1927

Delta R.T. 0.420 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19




Tgt Ion:165 Resp: 10408

Ion Ratio Lower Upper

165 100

63 2.9 54.1 81.1#

89 2.5 54.8 82.2#

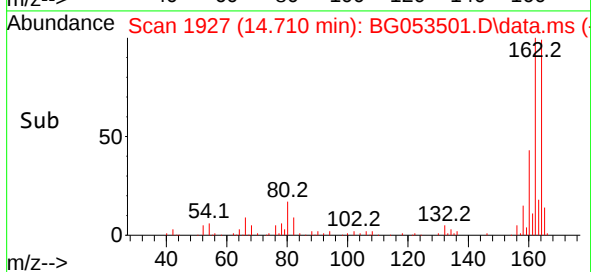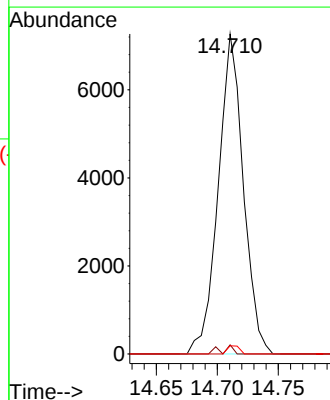



#57

2,4-Dinitrotoluene

Concen: 5.706 ng

RT: 14.710 min Scan# 1991

Delta R.T. -0.373 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19

Instrument :

BNA_G

ClientSampleId :

124035

Tgt Ion:165 Resp: 10408





Ion Ratio Lower Upper

165 100

63 2.9 34.6 52.0#

89 2.5 60.3 90.5#

182 0.0 2.2 3.4#

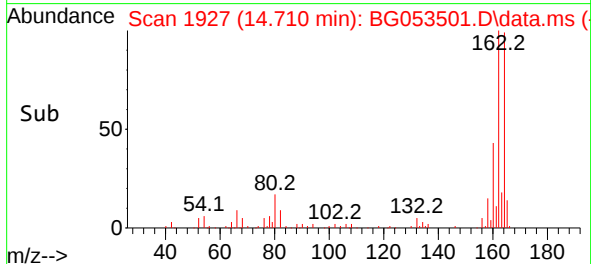

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.454 min Scan# 2394

Delta R.T. -0.015 min

Lab File: BG053501.D

Acq: 9 May 2022 20:19




Tgt Ion:188 Resp: 189290


Ion Ratio Lower Upper

188 100

94 7.3 5.4 8.0

80 8.2 6.8 10.2



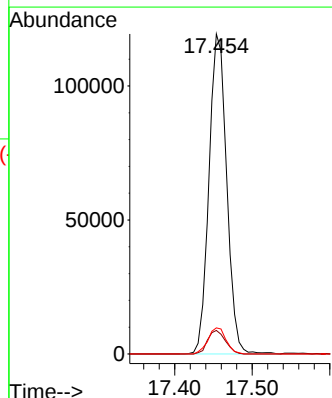
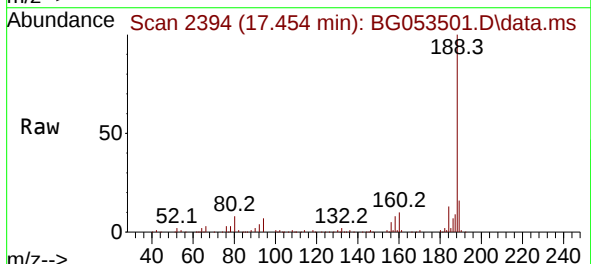




#67
4-Bromophenyl-phenylether
Concen: 3.522 ng
RT: 16.202 min Scan# 2181
Delta R.T. -0.449 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19




Instrument :
BNA_G
ClientSampleId :
124035


Tgt Ion:248 Resp: 7785
Ion Ratio Lower Upper
248 100
250 203.8 75.2 112.8#
141 521.0 50.0 75.0#

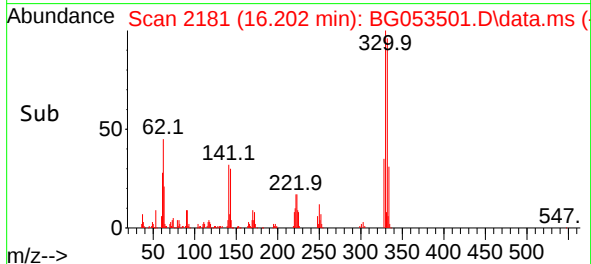

#75
Fluoranthene
Concen: 2.908 ng
RT: 19.504 min Scan# 2743
Delta R.T. -0.015 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Tgt Ion:202 Resp: 36247
Ion Ratio Lower Upper
202 100
101 7.9 0.0 26.9
203 15.1 0.0 37.2


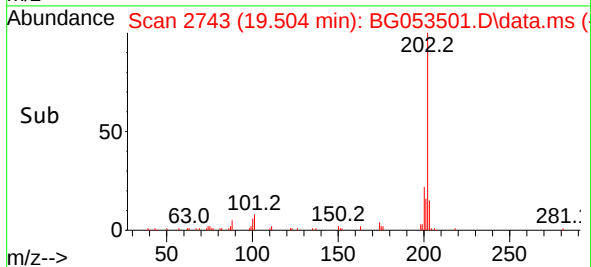

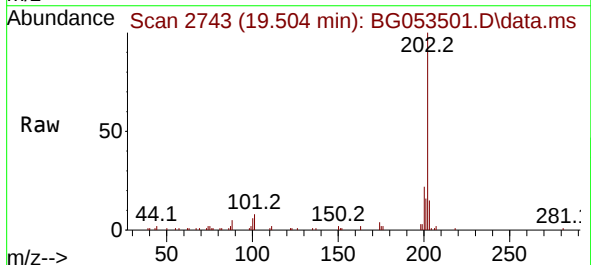




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.736 min Scan# 31
Delta R.T. -0.009 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19




Instrument :
BNA_G
ClientSampleId :
124035


Tgt Ion:240 Resp: 203295
Ion Ratio Lower Upper
240 100
120 6.0 4.6 7.0
236 26.4 20.2 30.4

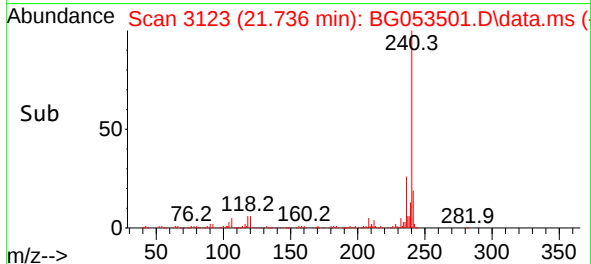

#77
Benzidine
Concen: 2.685 ng
RT: 20.056 min Scan# 2837
Delta R.T. 0.367 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Tgt Ion:184 Resp: 11766
Ion Ratio Lower Upper
184 100
185 15.1 11.8 17.6
183 7.5 8.9 13.3#


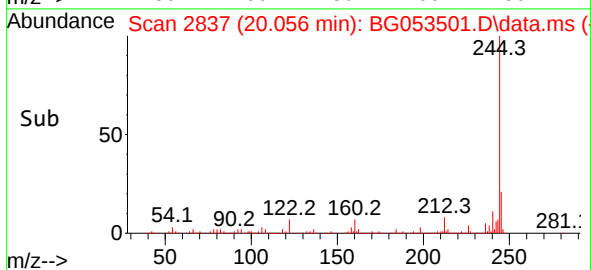

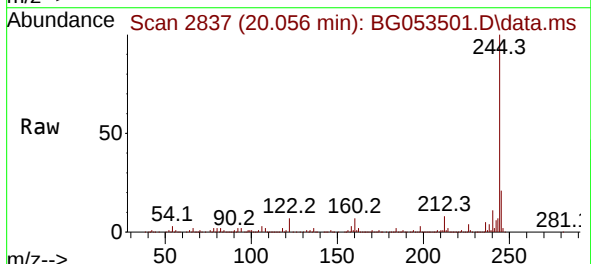




#78
 Pyrene
 Concen: 2.532 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BG053501.D
 Acq: 9 May 2022 20:19




Instrument :
 BNA_G
 ClientSampleId :
 124035


Tgt Ion:202 Resp: 33318
 Ion Ratio Lower Upper
 202 100
 200 18.6 16.6 24.8
 203 16.8 14.6 21.8

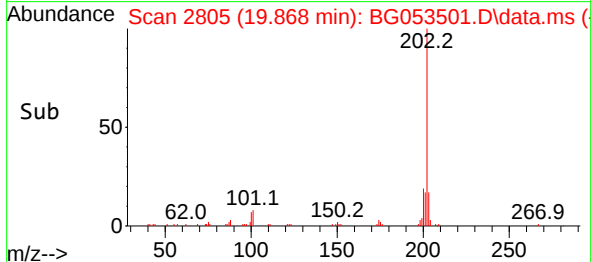

#79
 Terphenyl-d14
 Concen: 64.354 ng
 RT: 20.056 min Scan# 2837
 Delta R.T. -0.015 min
 Lab File: BG053501.D
 Acq: 9 May 2022 20:19

Tgt Ion:244 Resp: 702442
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.5 9.7
 122 6.8 5.0 7.4

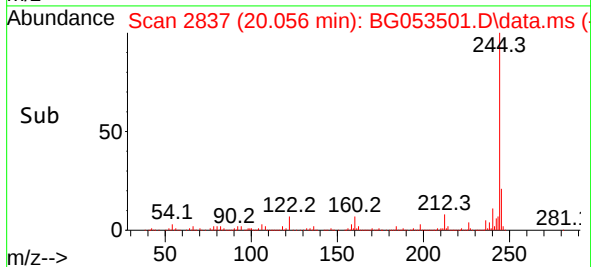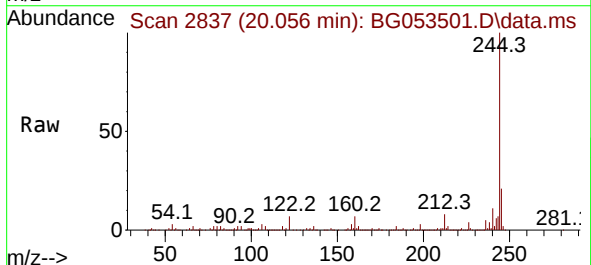



#86
Perylene-d12
Concen: 20.000 ng
RT: 25.014 min Scan# 30
Delta R.T. -0.021 min
Lab File: BG053501.D
Acq: 9 May 2022 20:19

Instrument :
BNA_G
ClientSampleId :
124035

Tgt Ion:264 Resp: 208405

Ion	Ratio	Lower	Upper
264	100		
260	22.2	19.0	28.6
265	20.2	17.4	26.2

