
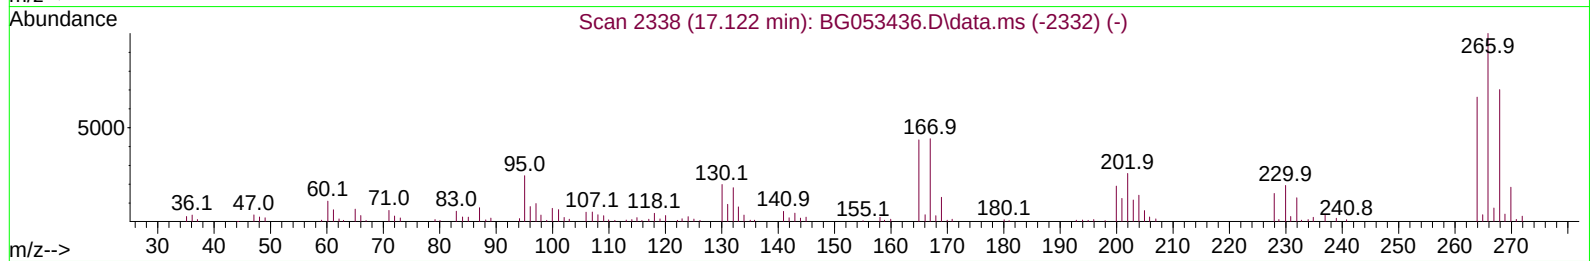
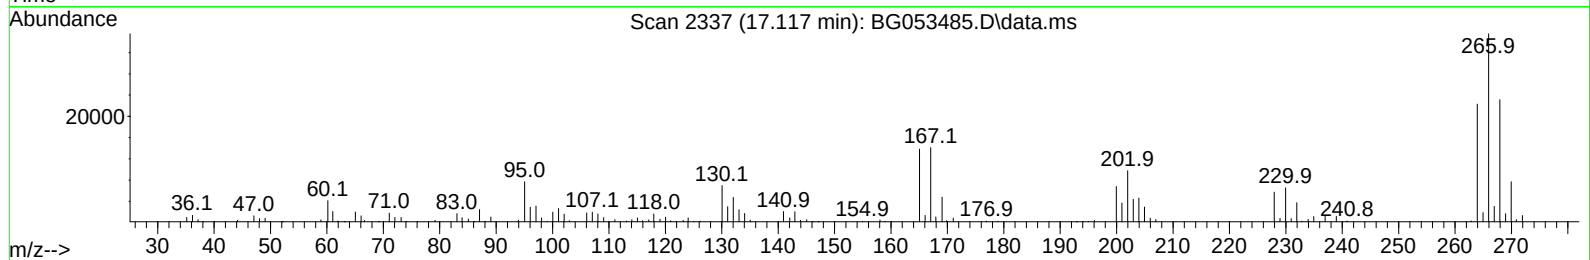


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
Data File : BG053485.D
Acq On : 9 May 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 16:59:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

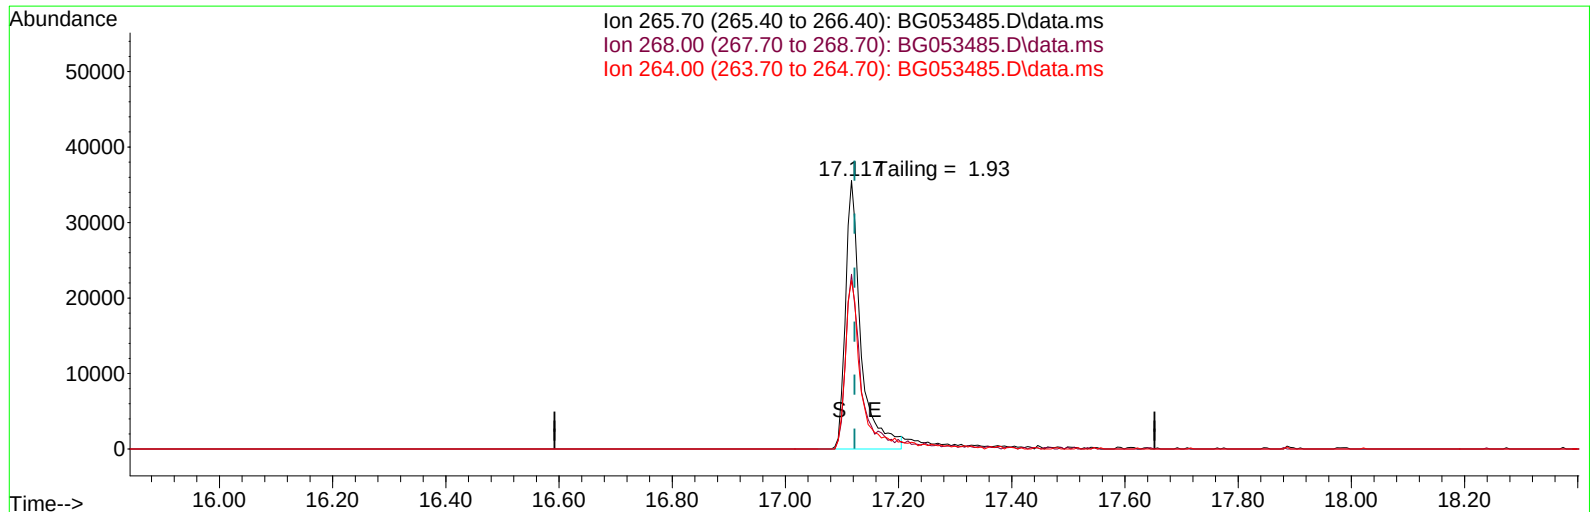

TIC: BG053485.D\data.ms

(70) Pentachlorophenol (C)




17.117min (-0.005) 31858.10 ng

response 71050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.12
264.00	66.20	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
Data File : BG053485.D
Acq On : 9 May 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 16:59:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

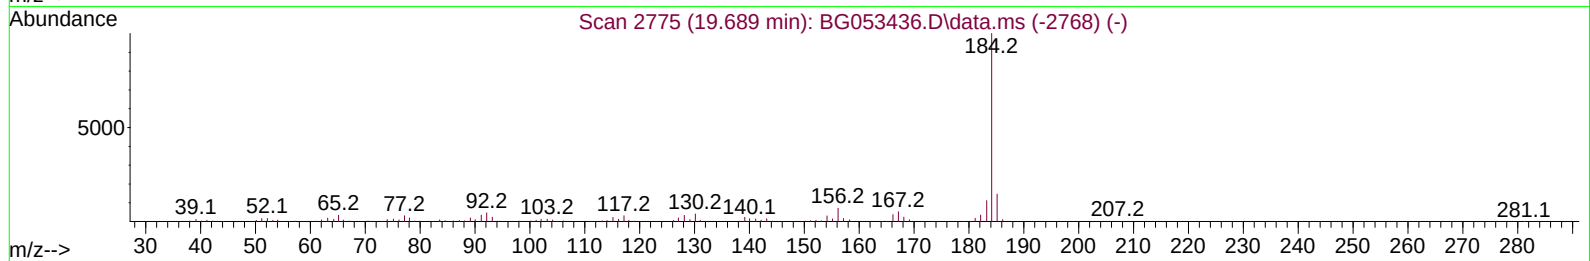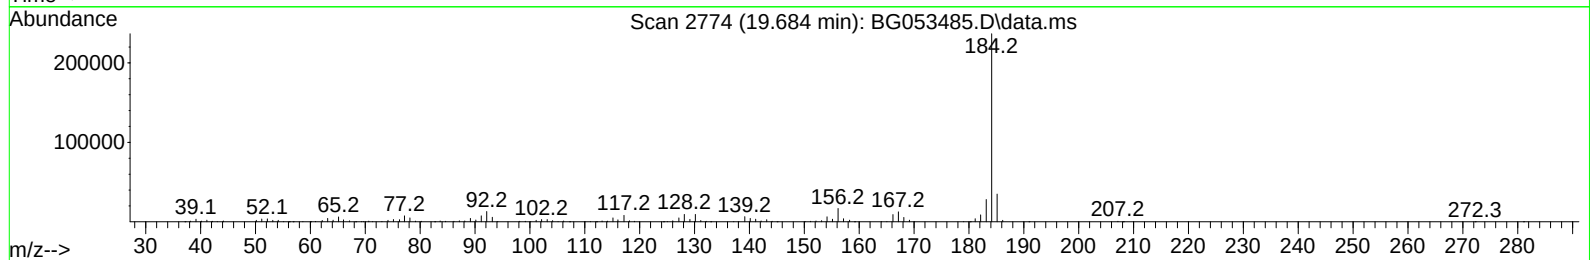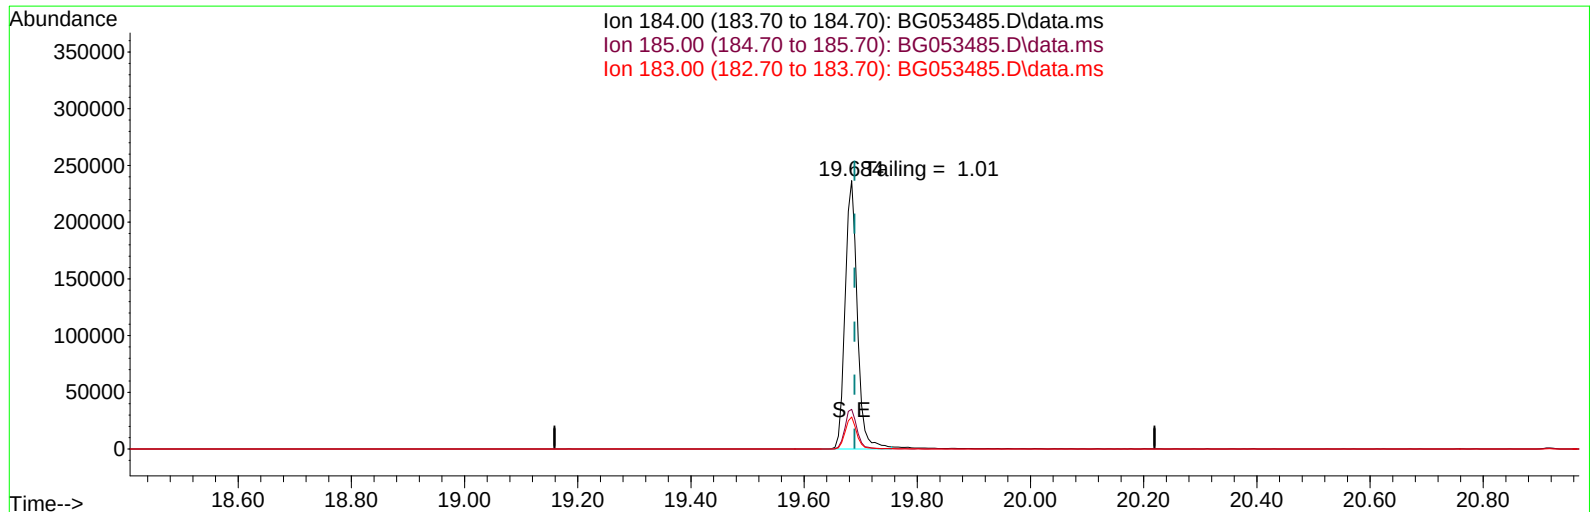

TIC: BG053485.D\data.ms

(77) Benzidine

19.684min (-0.005) 0.00 ng

response 359148

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.80
183.00	11.10	11.92
0.00	0.00	0.00