
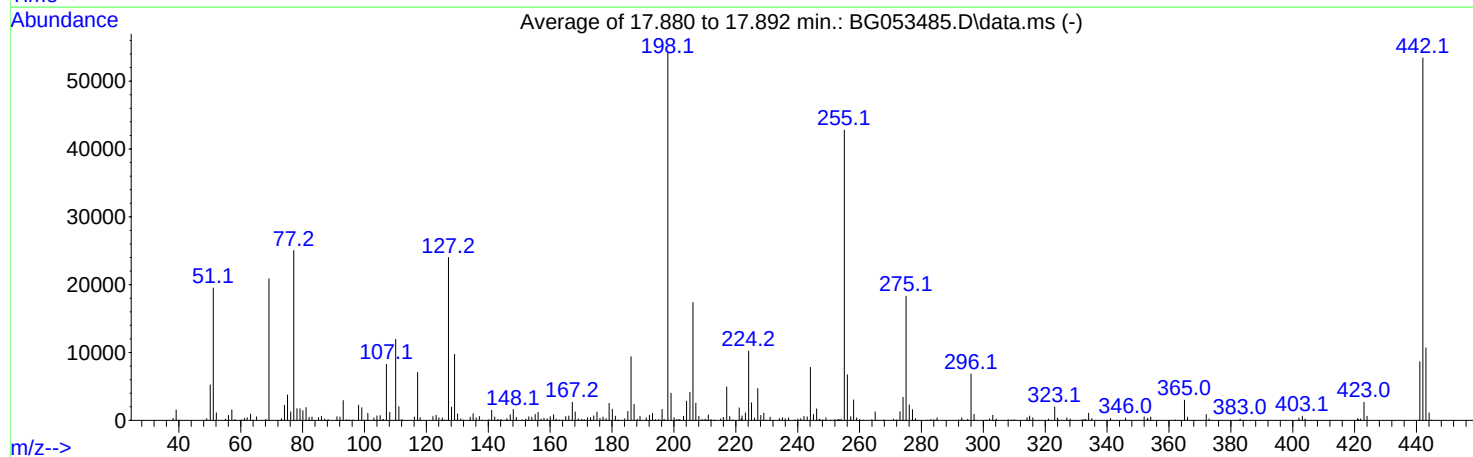


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
 Data File : BG053485.D
 Acq On : 9 May 2022 9:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 02:13:53 2022

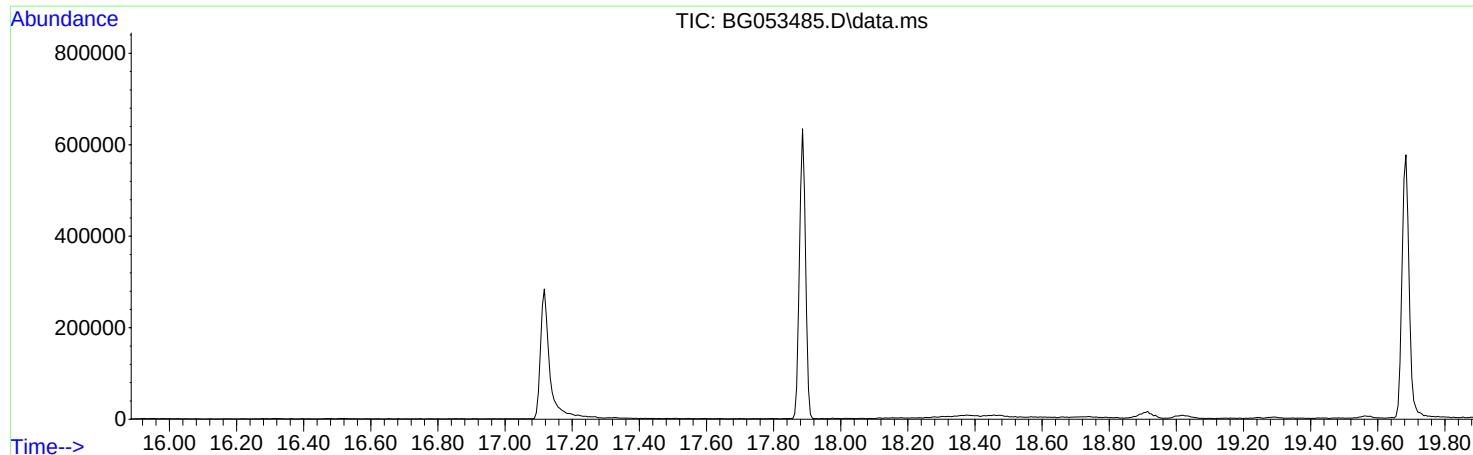




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	19495	PASS
68	69	0.00	2	0.8	164	PASS
69	198	0.00	100	38.5	20877	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	24021	PASS
197	198	0.00	2	0.3	171	PASS
198	198	100	100	100.0	54224	PASS
199	198	5	9	7.4	4018	PASS
275	198	10	60	33.7	18295	PASS
365	198	1	100	5.5	2972	PASS
441	198	0.01	100	15.9	8644	PASS
442	442	50	100	100.0	53421	PASS
443	442	15	24	20.0	10684	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
Data File : BG053485.D
Acq On : 9 May 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 09 16:59:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

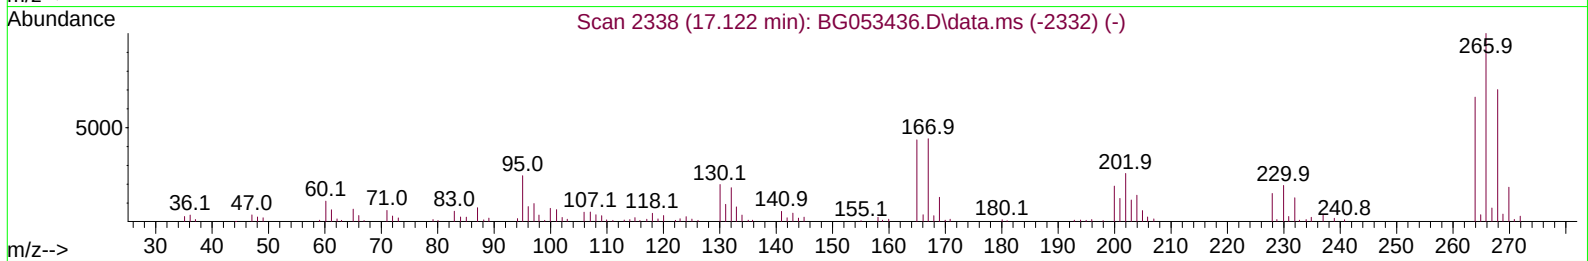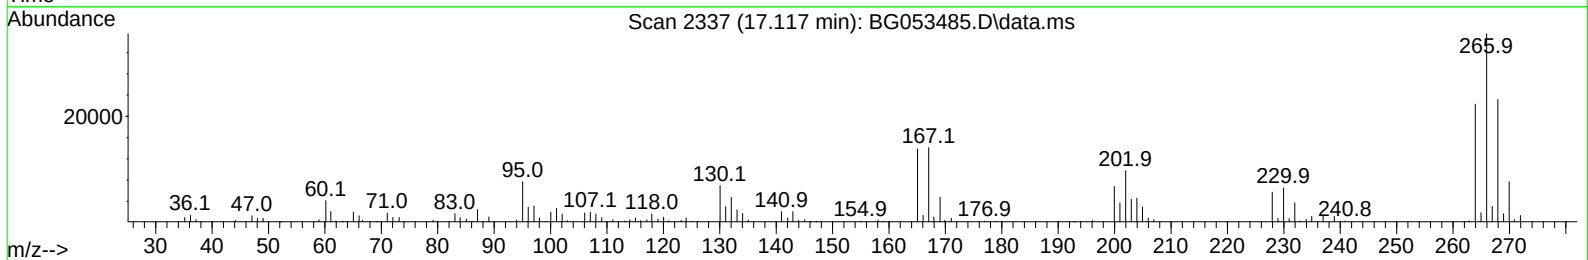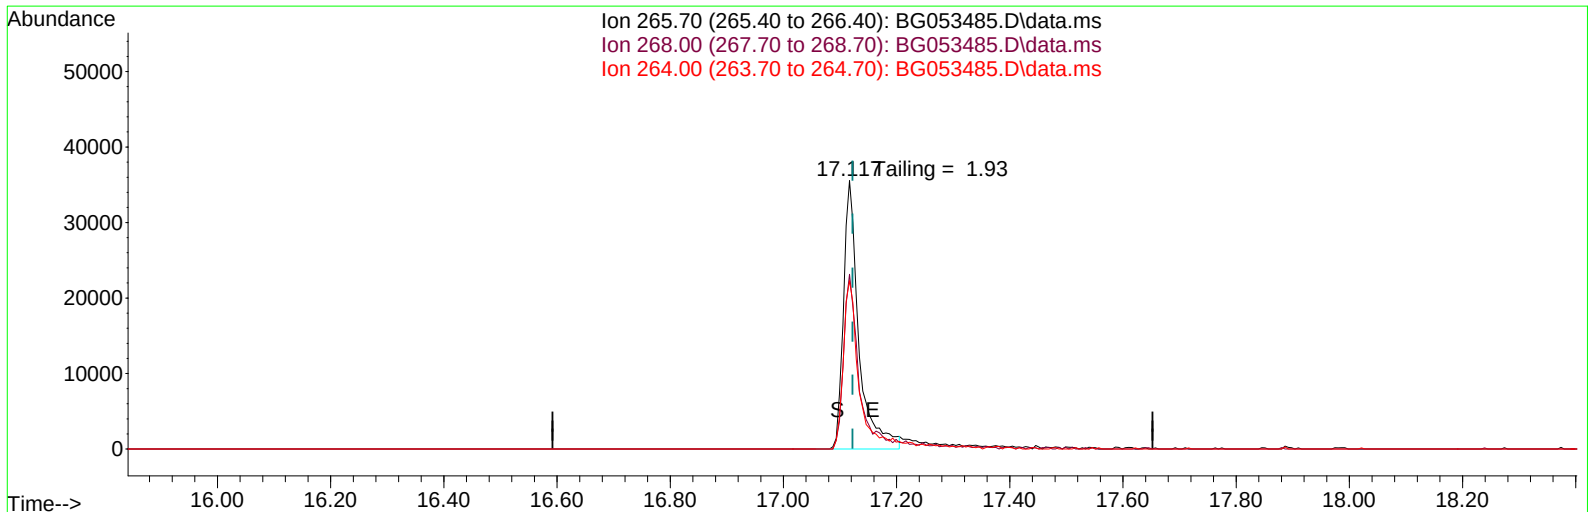

TIC: BG053485.D\data.ms

(70) Pentachlorophenol (C)

17.117min (-0.005) 31858.10 ng




response 71050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.12
264.00	66.20	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050922\
Data File : BG053485.D
Acq On : 9 May 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 09 16:59:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

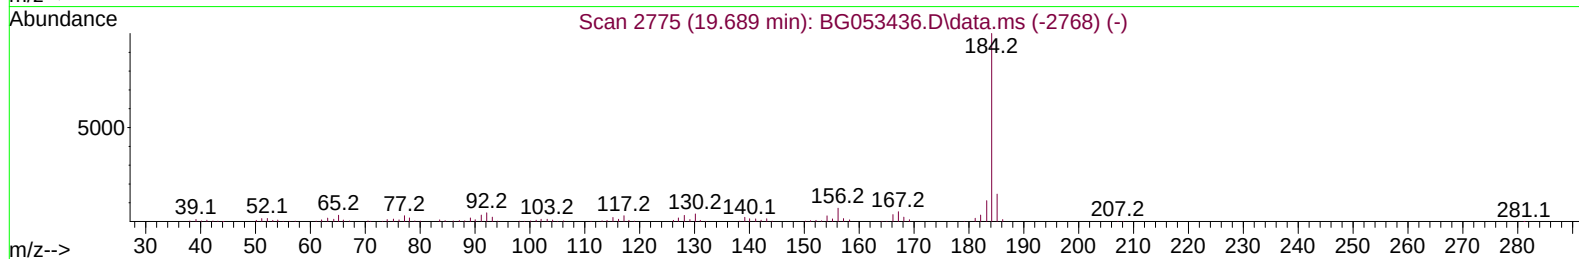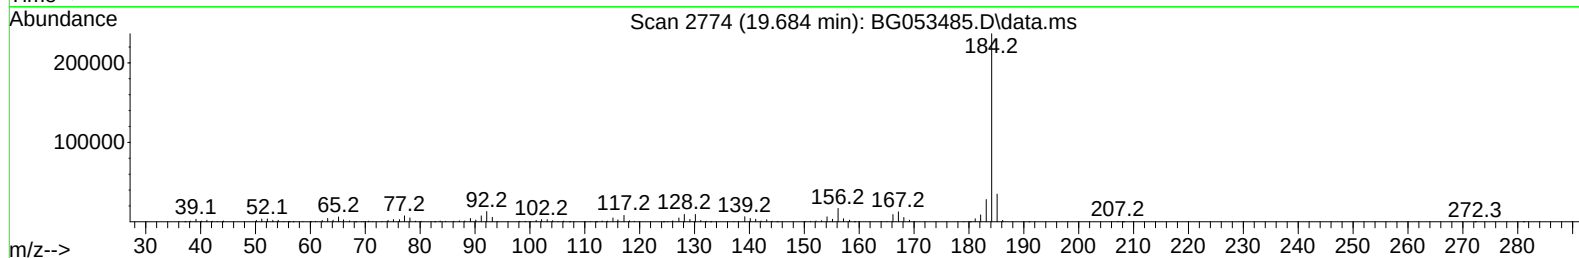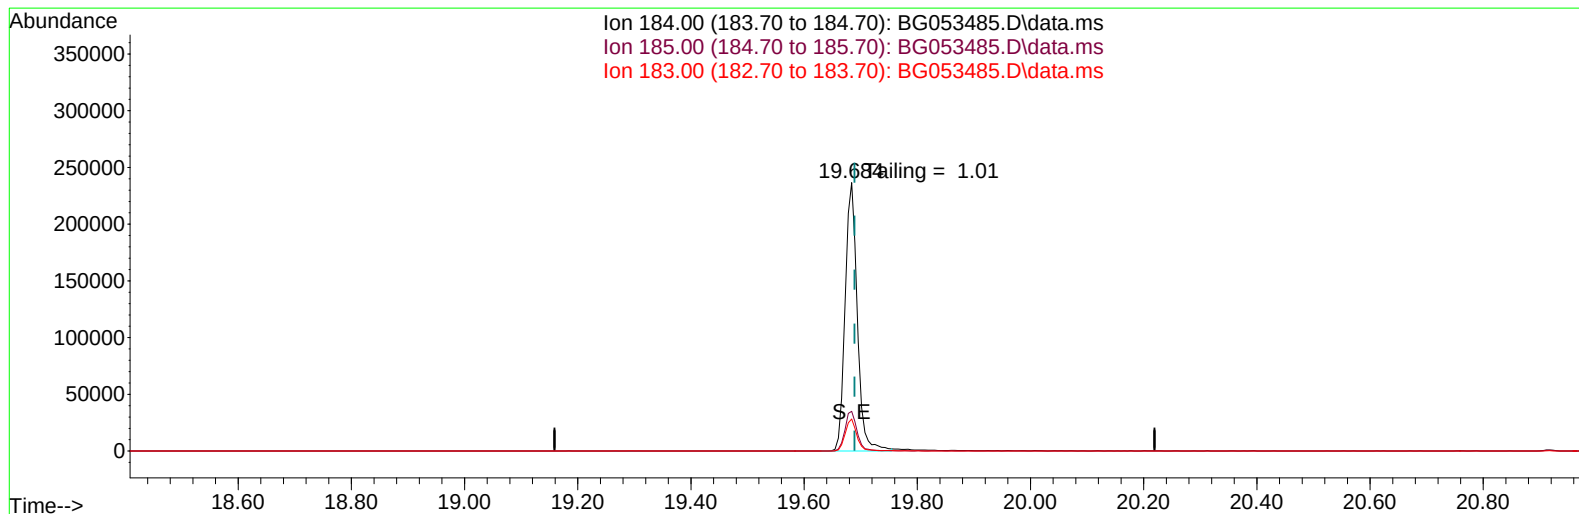

TIC: BG053485.D\data.ms

(77) Benzidine

19.684min (-0.005) 0.00 ng

response 359148

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.80
183.00	11.10	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/9/2022	BNA_G	<u>BG053485.D</u>
Compound Name	Response	Retention Time
DDT	207406	20.91
DDD	1776	20.47
DDE	419	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2195	209601	1.05

Instrument :
BNA_G
ClientSampleId :
DFTPP