

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
 Data File : BG057353.D
 Acq On : 9 May 2023 15:18
 Operator : CG/JU
 Sample : 02656-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.682	22	24	28	rVB3	689	756	0.17%	0.039%
2	3.718	28	30	31	rBV	742	527	0.12%	0.027%
3	3.788	41	42	46	rVB2	765	725	0.16%	0.037%
4	3.829	46	49	52	rBV2	386	497	0.11%	0.025%
5	4.088	92	93	96	rBV2	625	637	0.14%	0.033%
6	4.240	118	119	124	rVB2	475	538	0.12%	0.027%
7	4.446	151	154	158	rVB3	878	1179	0.26%	0.060%
8	4.540	169	170	173	rVB2	505	455	0.10%	0.023%
9	5.157	271	275	276	rVB	401	503	0.11%	0.026%
10	5.550	340	342	345	rVB	379	460	0.10%	0.023%
11	5.586	345	348	349	rBV	613	550	0.12%	0.028%
12	5.597	349	350	353	rVV	788	666	0.15%	0.034%
13	5.656	357	360	362	rVV	415	572	0.13%	0.029%
14	5.691	364	366	369	rVB	591	594	0.13%	0.030%
15	5.838	389	391	394	rBV2	574	577	0.13%	0.029%
16	8.370	815	822	829	rBB	64250	108887	24.27%	5.558%
17	9.939	1083	1089	1092	rBB	226	472	0.11%	0.024%
18	11.119	1287	1290	1294	rBV	259	529	0.12%	0.027%
19	11.207	1297	1305	1313	rVV	92237	166949	37.21%	8.522%
20	11.266	1313	1315	1318	rVB	446	475	0.11%	0.024%
21	11.689	1384	1387	1389	rBV	330	472	0.11%	0.024%
22	13.205	1643	1645	1649	rBB	338	453	0.10%	0.023%
23	14.979	1941	1947	1956	rVB2	187946	289795	64.59%	14.793%
24	16.553	2211	2215	2216	rVV	426	499	0.11%	0.025%
25	17.364	2352	2353	2357	rBV	389	462	0.10%	0.024%
26	17.422	2360	2363	2366	rVB2	360	508	0.11%	0.026%
27	17.722	2407	2414	2422	rVV	263304	404355	90.13%	20.642%
28	17.822	2428	2431	2435	rVB2	490	642	0.14%	0.033%
29	18.456	2537	2539	2542	rVB2	429	529	0.12%	0.027%
30	18.644	2568	2571	2572	rBV2	536	549	0.12%	0.028%
31	18.768	2591	2592	2594	rBV	499	450	0.10%	0.023%
32	19.061	2639	2642	2644	rBV	673	738	0.16%	0.038%
33	19.208	2664	2667	2668	rBV2	637	738	0.16%	0.038%
34	19.238	2670	2672	2673	rVB2	1066	635	0.14%	0.032%
35	19.255	2673	2675	2677	rBV	1075	1105	0.25%	0.056%
36	19.408	2700	2701	2704	rVB	842	552	0.12%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
 Data File : BG057353.D
 Acq On : 9 May 2023 15:18
 Operator : CG/JU
 Sample : 02656-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	19.443	2704	2707	2708	rVB2	801	559	0.12%	0.029%
38	19.455	2708	2709	2712	rBV	795	714	0.16%	0.036%
39	19.484	2712	2714	2715	rBV2	957	555	0.12%	0.028%
40	19.526	2718	2721	2722	rBV	994	864	0.19%	0.044%
41	19.608	2733	2735	2737	rVB2	688	576	0.13%	0.029%
42	19.643	2737	2741	2744	rBV2	952	1066	0.24%	0.054%
43	19.696	2748	2750	2755	rVB2	815	1084	0.24%	0.055%
44	19.731	2755	2756	2758	rBV2	605	480	0.11%	0.025%
45	19.855	2775	2777	2779	rVB3	738	645	0.14%	0.033%
46	19.884	2779	2782	2788	rBV4	902	1741	0.39%	0.089%
47	19.925	2788	2789	2791	rBV2	962	647	0.14%	0.033%
48	19.954	2791	2794	2796	rBV3	1878	1563	0.35%	0.080%
49	19.984	2798	2799	2802	rBV2	616	540	0.12%	0.028%
50	20.095	2816	2818	2820	rVV2	931	533	0.12%	0.027%
51	20.201	2835	2836	2837	rBV	1101	459	0.10%	0.023%
52	20.219	2837	2839	2842	rVB3	1076	823	0.18%	0.042%
53	20.301	2851	2853	2856	rBV4	1324	1227	0.27%	0.063%
54	20.324	2856	2857	2860	rVV2	865	750	0.17%	0.038%
55	20.413	2870	2872	2874	rBV3	1120	943	0.21%	0.048%
56	20.507	2885	2888	2893	rVB4	899	1396	0.31%	0.071%
57	20.689	2915	2919	2921	rBV4	1032	1151	0.26%	0.059%
58	20.730	2923	2926	2930	rBV4	1411	2255	0.50%	0.115%
59	20.883	2950	2952	2954	rVB3	1172	763	0.17%	0.039%
60	21.270	3016	3018	3019	rBV2	1459	1212	0.27%	0.062%
61	21.629	3076	3079	3085	rVB4	6437	9318	2.08%	0.476%
62	21.699	3087	3091	3097	rVB	19006	27801	6.20%	1.419%
63	22.034	3140	3148	3157	rBV2	259703	448641	100.00%	22.902%
64	22.539	3232	3234	3236	rBV4	1762	2116	0.47%	0.108%
65	22.639	3249	3251	3254	rBV4	1842	2228	0.50%	0.114%
66	22.874	3289	3291	3292	rBV2	1693	892	0.20%	0.046%
67	23.632	3418	3420	3422	rBV3	1655	1717	0.38%	0.088%
68	23.890	3462	3464	3467	rBV4	1565	1250	0.28%	0.064%
69	23.920	3467	3469	3472	rBV3	1765	1306	0.29%	0.067%
70	24.431	3551	3556	3562	rBV6	4921	8991	2.00%	0.459%
71	25.441	3726	3728	3729	rBV2	3306	2718	0.61%	0.139%
72	25.459	3729	3731	3734	rVV3	5600	8523	1.90%	0.435%
73	25.541	3735	3745	3755	rVB2	136648	406670	90.64%	20.760%
74	26.487	3904	3906	3908	rBV3	1579	1643	0.37%	0.084%
75	26.628	3928	3930	3931	rBV2	1569	1378	0.31%	0.070%
76	27.051	4000	4002	4003	rBV	2006	1314	0.29%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
 Data File : BG057353.D
 Acq On : 9 May 2023 15:18
 Operator : CG/JU
 Sample : 02656-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

77	27.826	4132	4134	4138	rBV5	1903	2684	0.60%	0.137%
78	28.948	4323	4325	4326	rBV	2305	1818	0.41%	0.093%
79	29.512	4419	4421	4424	rBV3	1681	1288	0.29%	0.066%
80	30.146	4528	4529	4531	rBV	1854	944	0.21%	0.048%
81	30.434	4576	4578	4581	rBV4	1973	2042	0.46%	0.104%
82	30.487	4585	4587	4589	rVB3	1892	1017	0.23%	0.052%
83	31.098	4689	4691	4693	rBV3	1653	1778	0.40%	0.091%
84	31.174	4702	4704	4707	rVB4	1931	1282	0.29%	0.065%
85	31.368	4735	4737	4738	rBV	1857	1246	0.28%	0.064%
86	31.592	4773	4775	4776	rBV2	1665	1148	0.26%	0.059%
87	31.785	4806	4808	4810	rBV2	1825	1150	0.26%	0.059%
88	31.985	4841	4842	4845	rVB3	2410	1451	0.32%	0.074%
89	32.050	4851	4853	4854	rBV2	1715	1166	0.26%	0.060%
90	32.296	4893	4895	4896	rBV2	2003	1845	0.41%	0.094%




Sum of corrected areas: 1958941

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
Data File : BG057353.D
Acq On : 9 May 2023 15:18
Operator : CG/JU
Sample : 02656-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

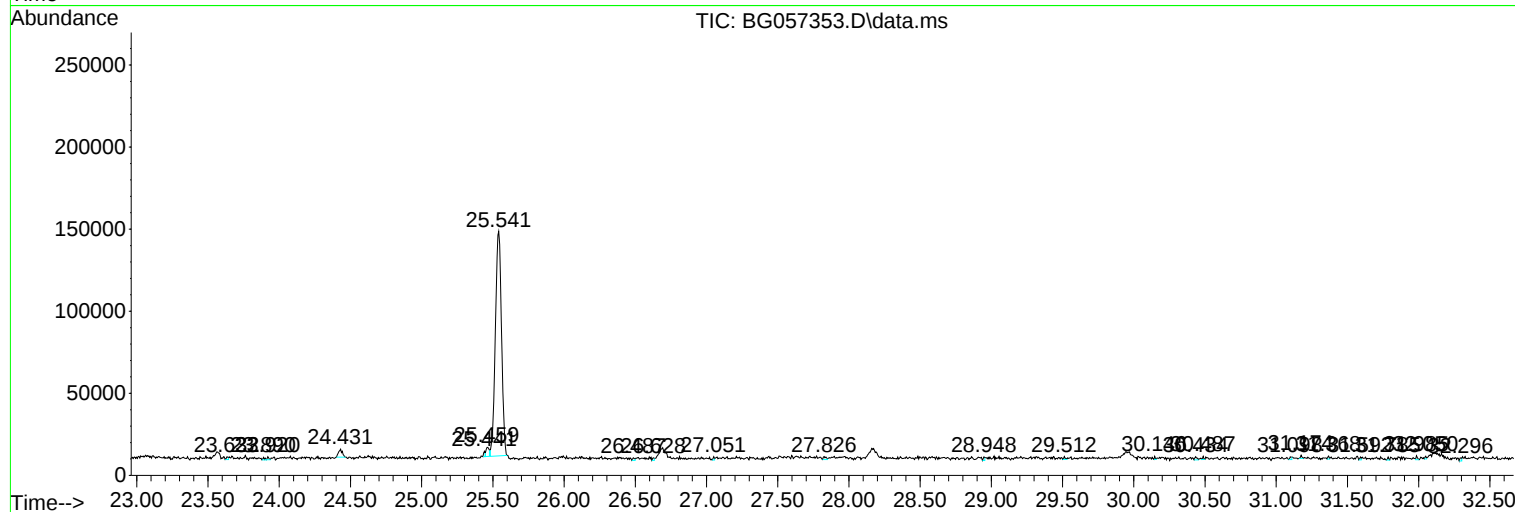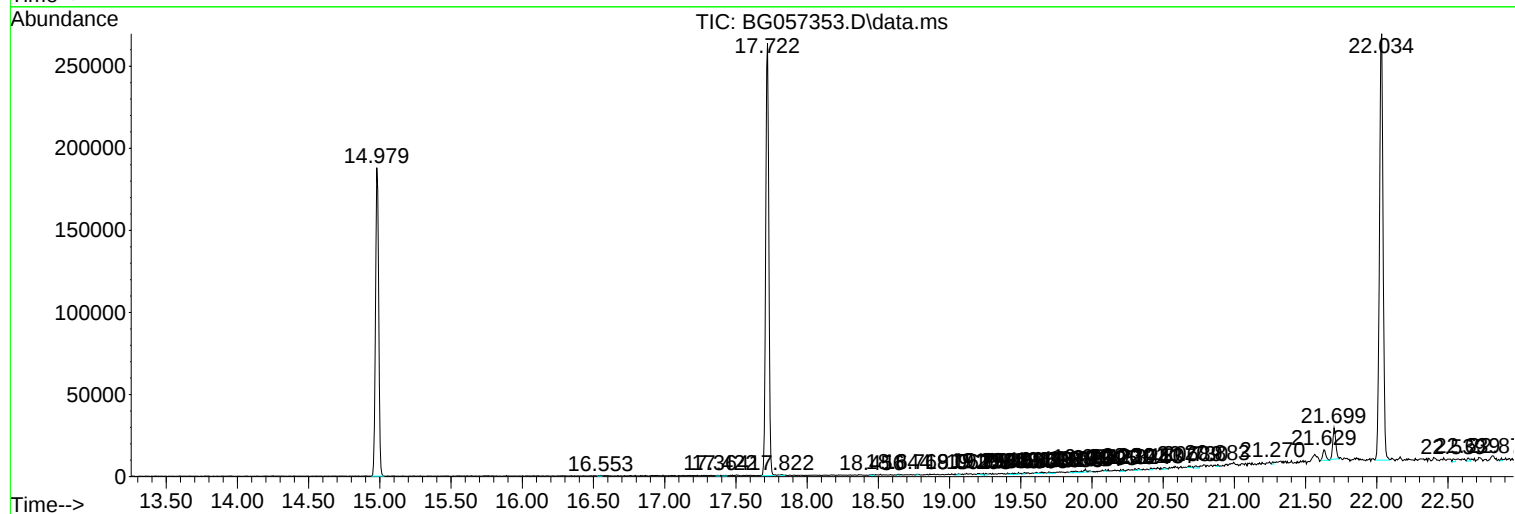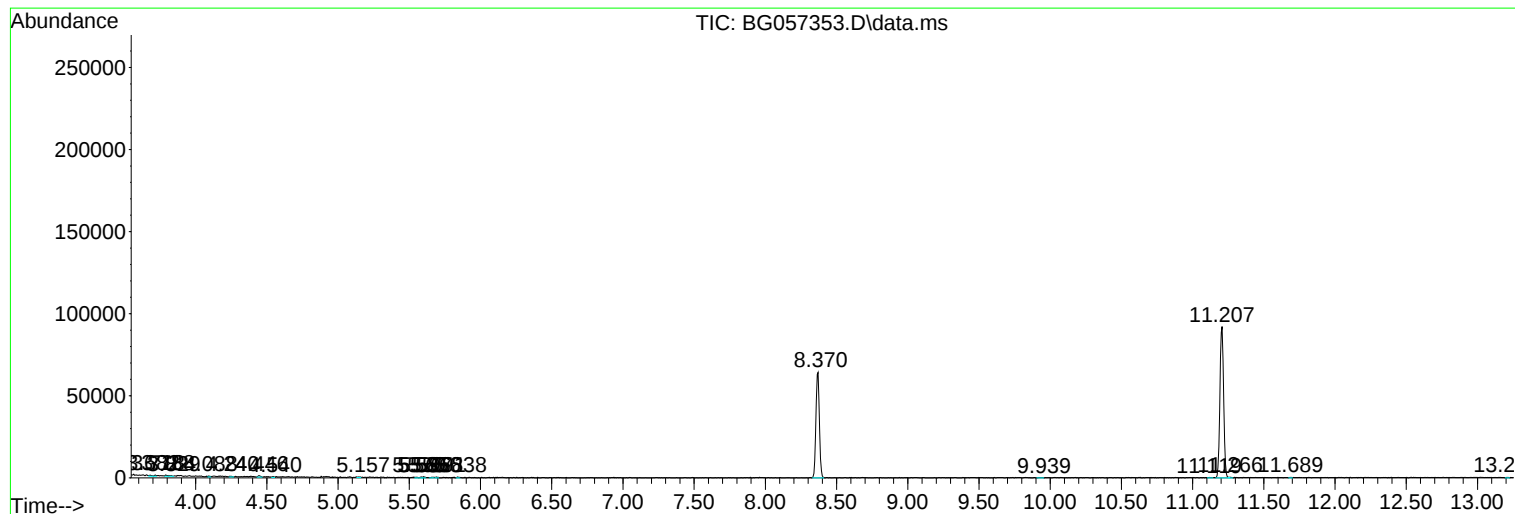

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
Data File : BG057353.D
Acq On : 9 May 2023 15:18
Operator : CG/JU
Sample : 02656-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050923\
Data File : BG057353.D
Acq On : 9 May 2023 15:18
Operator : CG/JU
Sample : 02656-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------