


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051015\
 Data File : BG017029.D
 Acq On : 10 May 2015 18:22
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 05 16:13:58 2015

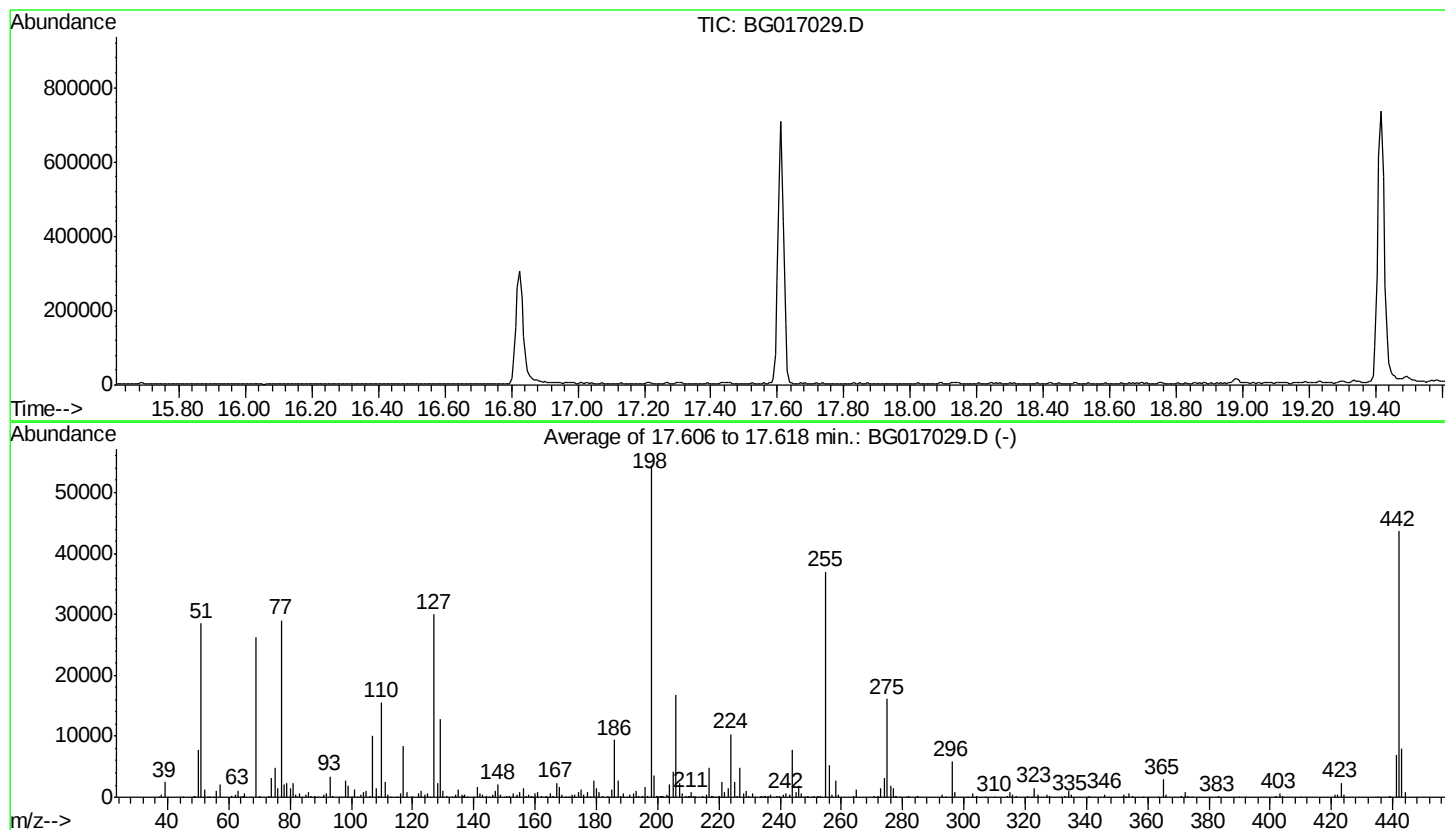

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	28546	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.4	26317	PASS
70	69	0.00	2	0.5	119	PASS
127	198	10	80	55.0	29941	PASS
197	198	0.00	2	0.2	136	PASS
198	198	100	100	100.0	54405	PASS
199	198	5	9	6.6	3601	PASS
275	198	10	60	29.6	16131	PASS
365	198	1	100	5.3	2869	PASS
441	442	0.01	24	15.7	6862	PASS
442	198	50	100	80.3	43666	PASS
443	442	15	24	18.5	8081	PASS