


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051015\
 Data File : BG017047.D
 Acq On : 11 May 2015 5:24
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC040

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 05 16:13:58 2015

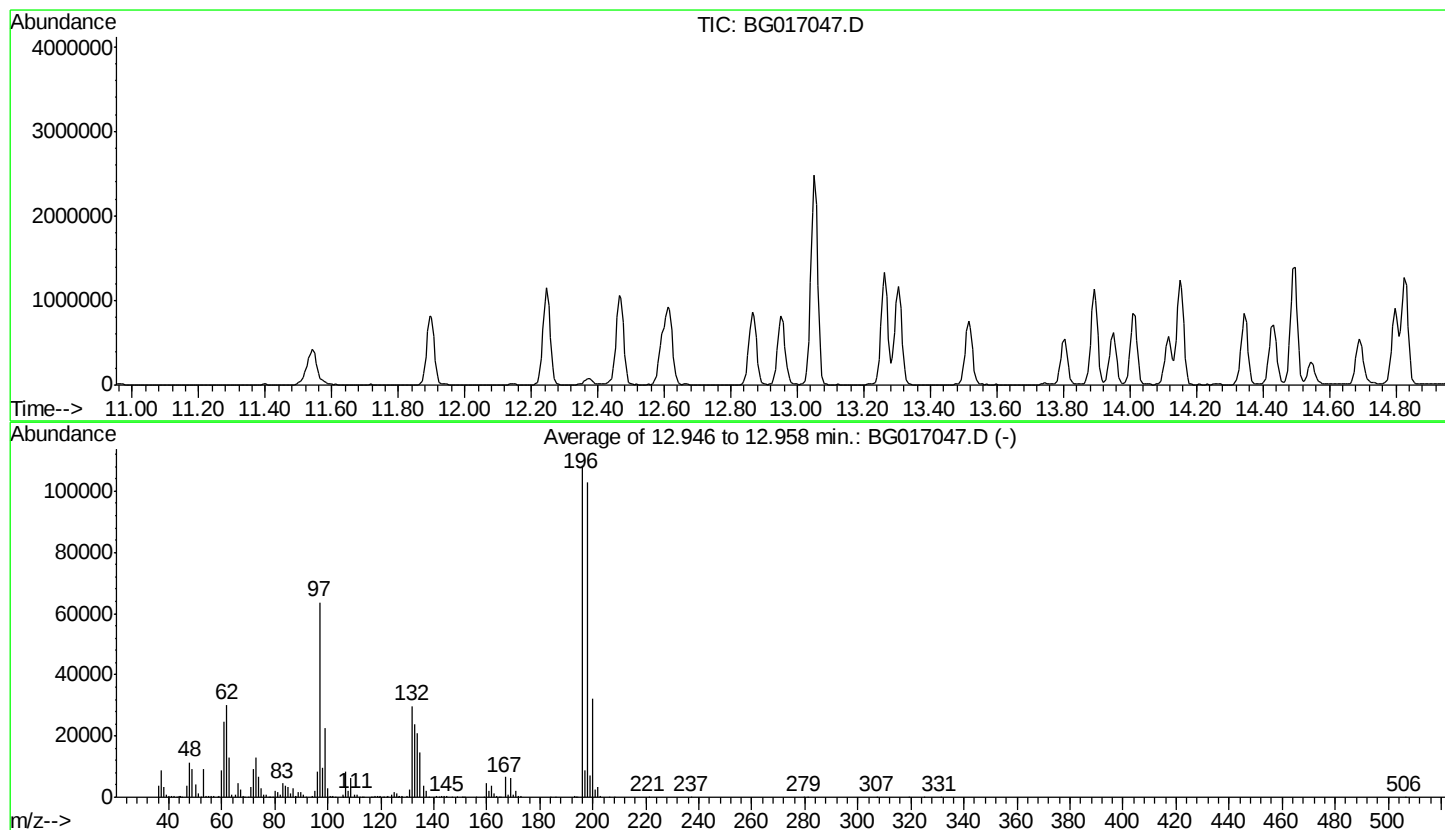

AutoFind: Scans 1746, 1747, 1748; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	1.2	1203	FAIL*
68	69	COMPARISON MASS IS NOT PRESENT!!!				
69	198	0.00	100	0.0	0	PASS
70	69	COMPARISON MASS IS NOT PRESENT!!!				
127	198	10	80	0.4	415	FAIL*
197	198	0.00	2	8.5	8719	FAIL*
198	198	100	100	100.0	102717	PASS
199	198	5	9	6.9	7106	PASS
275	198	10	60	0.0	0	FAIL*
365	198	1	100	0.0	0	FAIL*
441	442	COMPARISON MASS IS NOT PRESENT!!!				
442	198	50	100	0.0	0	FAIL*
443	442	COMPARISON MASS IS NOT PRESENT!!!				