

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
 Data File : BG026944.D
 Acq On : 10 May 2017 19:01
 Operator : SJ/MA
 Sample : I2960-05DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.092	678	681	685	rVB2	10689	13137	0.27%	0.039%
2	7.192	691	698	714	rVB	266267	562847	11.40%	1.681%
3	7.333	716	722	730	rVB	238286	395758	8.01%	1.182%
4	7.550	751	759	770	rBV	297892	525578	10.64%	1.570%
5	7.656	775	777	787	rVB2	13524	25027	0.51%	0.075%
6	8.008	829	837	852	rVB	590692	1034843	20.96%	3.091%
7	8.555	926	930	942	rVB6	6239	18762	0.38%	0.056%
8	8.649	942	946	950	rBV3	5494	8267	0.17%	0.025%
9	8.725	953	959	981	rVB	339268	675495	13.68%	2.018%
10	9.166	1027	1034	1049	rVB	275441	514180	10.41%	1.536%
11	9.336	1057	1063	1065	rBV5	6327	10773	0.22%	0.032%
12	9.577	1101	1104	1110	rVB5	7594	11507	0.23%	0.034%
13	9.700	1121	1125	1131	rVB5	4257	6419	0.13%	0.019%
14	9.888	1149	1157	1174	rBV	215997	423359	8.57%	1.264%
15	10.212	1206	1212	1218	rVB7	3922	9657	0.20%	0.029%
16	10.447	1243	1252	1271	rBV	327542	664484	13.46%	1.985%
17	10.811	1303	1314	1330	rVB	922673	1739447	35.23%	5.195%
18	10.946	1330	1337	1362	rBV	258174	537696	10.89%	1.606%
19	11.187	1375	1378	1383	rBV5	3413	5610	0.11%	0.017%
20	11.281	1387	1394	1396	rVB6	3494	5804	0.12%	0.017%
21	12.209	1545	1552	1559	rBV7	5268	10145	0.21%	0.030%
22	12.397	1578	1584	1589	rVB5	5816	11133	0.23%	0.033%
23	12.462	1589	1595	1599	rVB3	5196	9426	0.19%	0.028%
24	12.679	1626	1632	1639	rVB4	5539	9619	0.19%	0.029%
25	12.991	1681	1685	1688	rBV5	2937	5031	0.10%	0.015%
26	13.161	1708	1714	1720	rVB7	4006	6234	0.13%	0.019%
27	13.226	1720	1725	1731	rBV7	6776	10293	0.21%	0.031%
28	13.443	1754	1762	1769	rBV5	12164	24348	0.49%	0.073%
29	13.590	1781	1787	1793	rBV6	4064	7557	0.15%	0.023%
30	13.954	1842	1849	1853	rBV8	6886	18069	0.37%	0.054%
31	14.019	1853	1860	1865	rVV	668462	964208	19.53%	2.880%
32	14.066	1865	1868	1877	rVB	269030	375066	7.60%	1.120%
33	14.219	1891	1894	1899	rVB7	4895	7938	0.16%	0.024%
34	14.319	1902	1911	1924	rBV	815948	1311651	26.56%	3.918%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
 Data File : BG026944.D
 Acq On : 10 May 2017 19:01
 Operator : SJ/MA
 Sample : I2960-05DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION

35	14.507	1937	1943	1949	rBV2	26812	41066	0.83%	0.123%
36	14.624	1949	1963	1970	rVV2	1306248	2167667	43.90%	6.474%
37	14.683	1970	1973	1981	rVB3	14011	26501	0.54%	0.079%
38	14.859	1993	2003	2025	rBV2	110405	359557	7.28%	1.074%
39	15.018	2025	2030	2035	rVB6	9484	20418	0.41%	0.061%
40	15.123	2045	2048	2053	rVB6	8249	12959	0.26%	0.039%
41	15.188	2056	2059	2065	rVB6	5407	6343	0.13%	0.019%
42	15.341	2084	2085	2091	rBV5	3648	5717	0.12%	0.017%
43	15.411	2091	2097	2098	rBV5	8327	11794	0.24%	0.035%
44	15.453	2100	2104	2109	rVB	36491	50082	1.01%	0.150%
45	15.517	2113	2115	2119	rVB5	5206	5807	0.12%	0.017%
46	15.611	2119	2131	2137	rBV	959038	1483343	30.04%	4.430%
47	15.658	2137	2139	2145	rVB3	17353	27042	0.55%	0.081%
48	15.740	2146	2153	2161	rBV2	90282	141568	2.87%	0.423%
49	15.846	2165	2171	2178	rVB6	22710	42426	0.86%	0.127%
50	15.952	2184	2189	2194	rVB9	10098	16827	0.34%	0.050%
51	15.999	2194	2197	2202	rBV6	6330	7305	0.15%	0.022%
52	16.069	2207	2209	2212	rBV4	5466	6568	0.13%	0.020%
53	16.111	2212	2216	2221	rVB6	7339	12247	0.25%	0.037%
54	16.181	2226	2228	2234	rBV7	5301	7718	0.16%	0.023%
55	16.310	2245	2250	2261	rVV3	40266	87219	1.77%	0.261%
56	16.487	2277	2280	2283	rVB5	5458	5381	0.11%	0.016%
57	16.557	2287	2292	2298	rBV8	8220	20478	0.41%	0.061%
58	16.669	2300	2311	2316	rBV8	11864	46082	0.93%	0.138%
59	16.716	2316	2319	2321	rVB3	7741	6838	0.14%	0.020%
60	16.769	2324	2328	2331	rVB6	8815	10497	0.21%	0.031%
61	16.821	2332	2337	2338	rBV5	7353	8515	0.17%	0.025%
62	17.015	2366	2370	2374	rBV7	7991	12516	0.25%	0.037%
63	17.098	2379	2384	2389	rVB5	22694	25553	0.52%	0.076%
64	17.156	2389	2394	2395	rBV5	9916	15647	0.32%	0.047%
65	17.250	2405	2410	2414	rVB7	9386	16994	0.34%	0.051%
66	17.356	2420	2428	2433	rBV2	1452470	2152212	43.59%	6.428%
67	17.397	2433	2435	2439	rVV	234833	291942	5.91%	0.872%
68	17.456	2439	2445	2456	rVB2	939945	1491436	30.20%	4.455%
69	17.679	2478	2483	2485	rBV6	7672	13210	0.27%	0.039%
70	17.756	2489	2496	2501	rBV4	25037	53416	1.08%	0.160%
71	17.832	2506	2509	2512	rBV5	7222	9734	0.20%	0.029%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
Data File : BG026944.D
Acq On : 10 May 2017 19:01
Operator : SJ/MA
Sample : I2960-05DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC40DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.1
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Title : SVOA CALIBRATION

72	18.179	2564	2568	2572	rBV6	18258	28640	0.58%	0.086%
73	18.237	2572	2578	2582	rVV3	87441	144774	2.93%	0.432%
74	18.279	2582	2585	2594	rVB3	40127	69806	1.41%	0.208%
75	18.425	2605	2610	2614	rBV2	47140	82441	1.67%	0.246%
76	18.725	2657	2661	2665	rBV3	21388	39640	0.80%	0.118%
77	18.772	2666	2669	2673	rVB6	27560	41282	0.84%	0.123%
78	19.401	2771	2776	2783	rVB	567406	806726	16.34%	2.410%
79	19.507	2790	2794	2796	rBV5	33113	52225	1.06%	0.156%
80	19.736	2827	2833	2846	rBV3	1127258	2299321	46.56%	6.868%
81	21.481	3124	3130	3136	rBV	3791690	4937946	100.00%	14.749%
82	21.604	3143	3151	3156	rBV2	1391372	2529430	51.22%	7.555%
83	23.766	3515	3519	3525	rBV2	134371	331892	6.72%	0.991%
84	24.559	3647	3654	3661	rBV2	438693	1151625	23.32%	3.440%
85	24.777	3681	3691	3700	rBV2	718893	2285207	46.28%	6.825%


Sum of corrected areas: 33480948

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
Data File : BG026944.D
Acq On : 10 May 2017 19:01
Operator : SJ/MA
Sample : I2960-05DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC40DL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

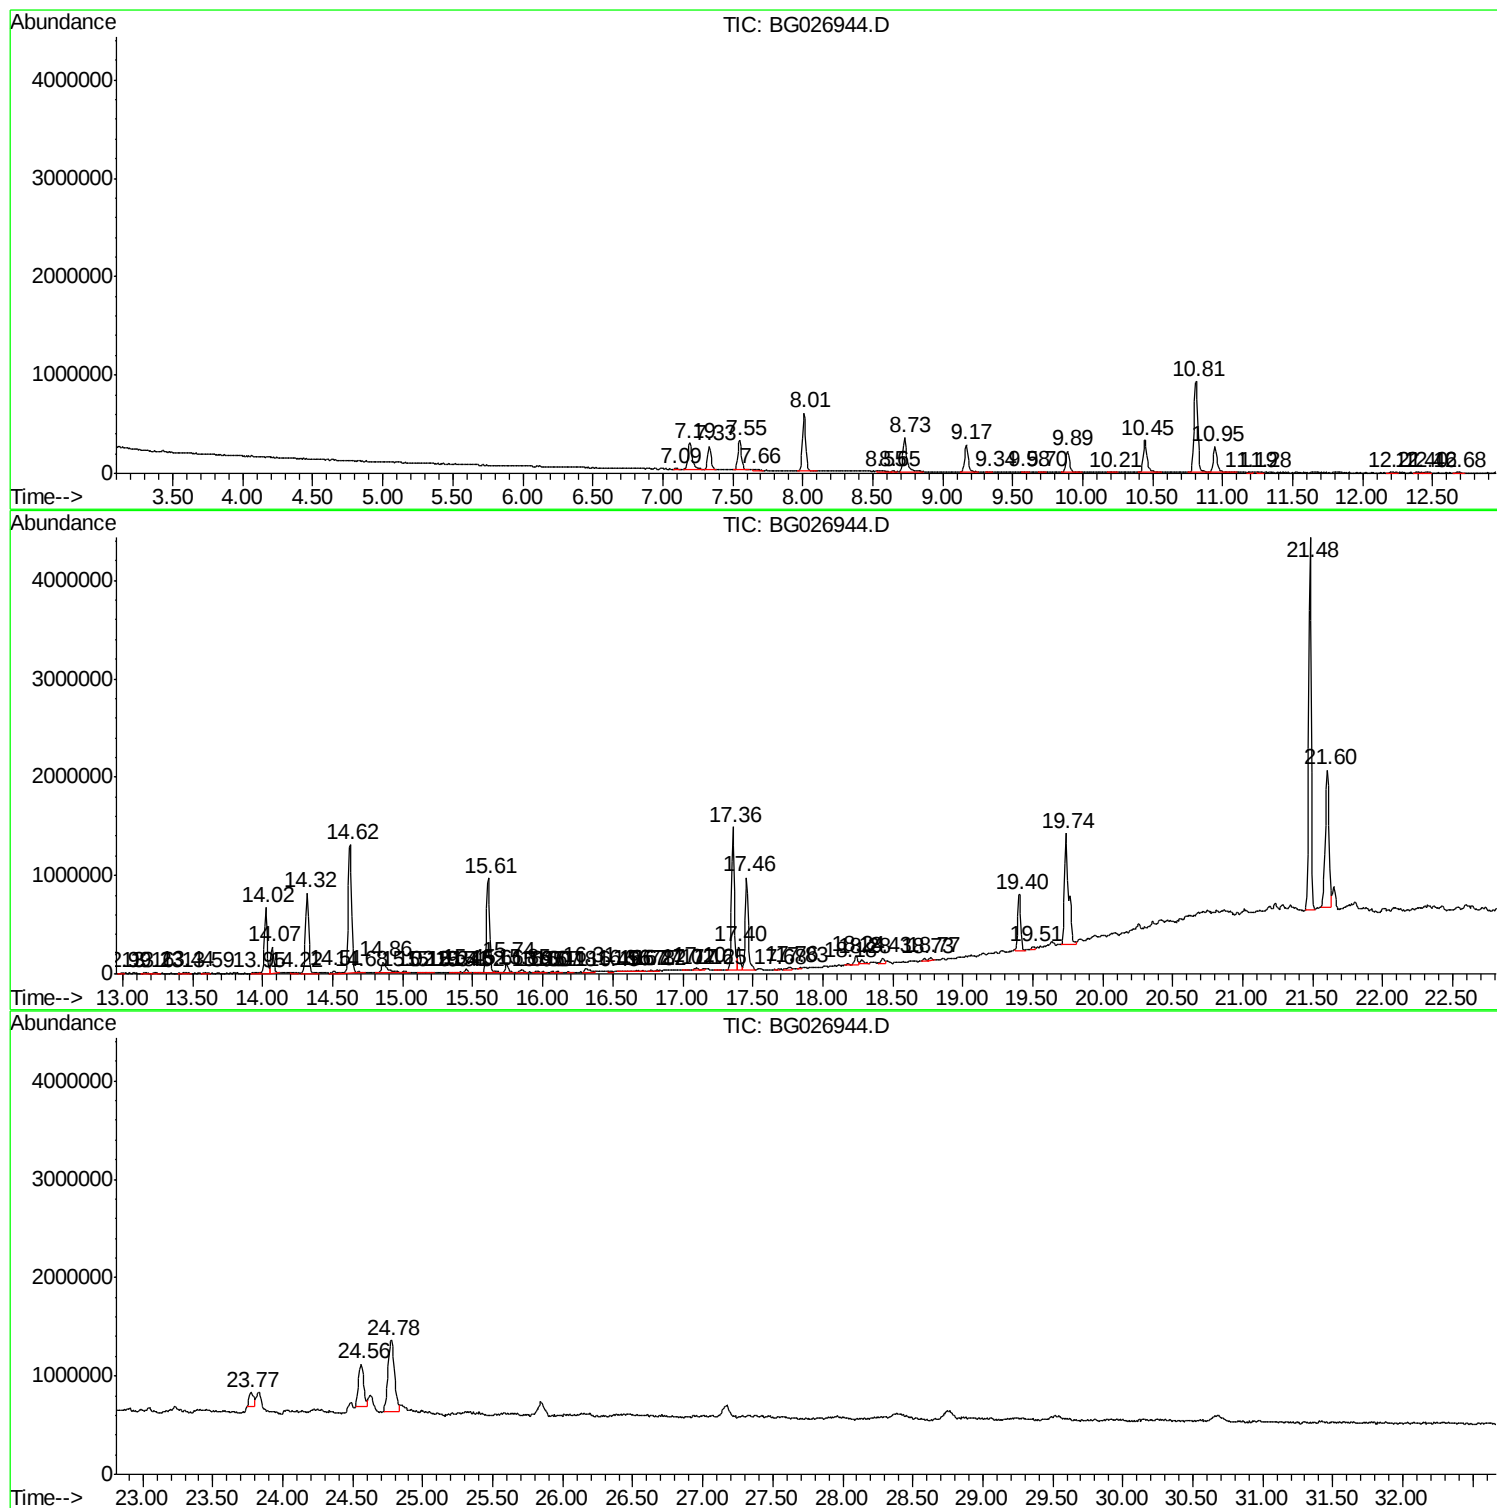

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
Data File : BG026944.D
Acq On : 10 May 2017 19:01
Operator : SJ/MA
Sample : I2960-05DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC40DL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051017\
Data File : BG026944.D
Acq On : 10 May 2017 19:01
Operator : SJ/MA
Sample : I2960-05DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC40DL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc