
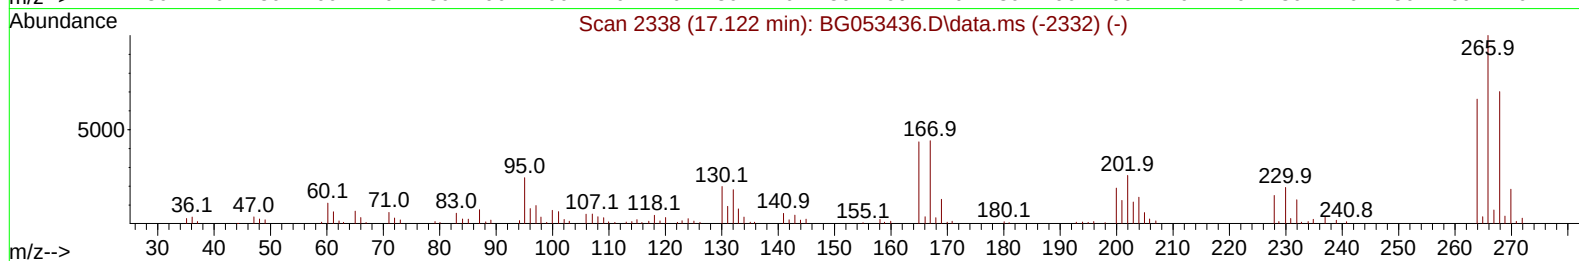
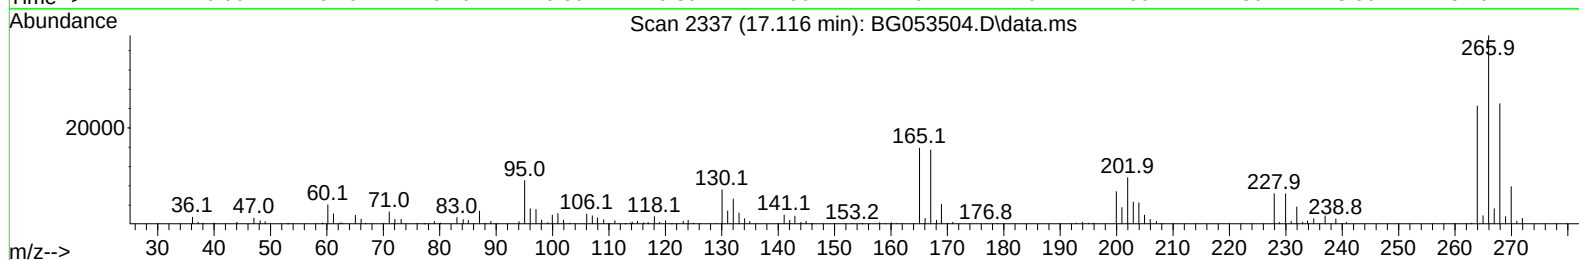


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053504.D
Acq On : 10 May 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 13:53:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

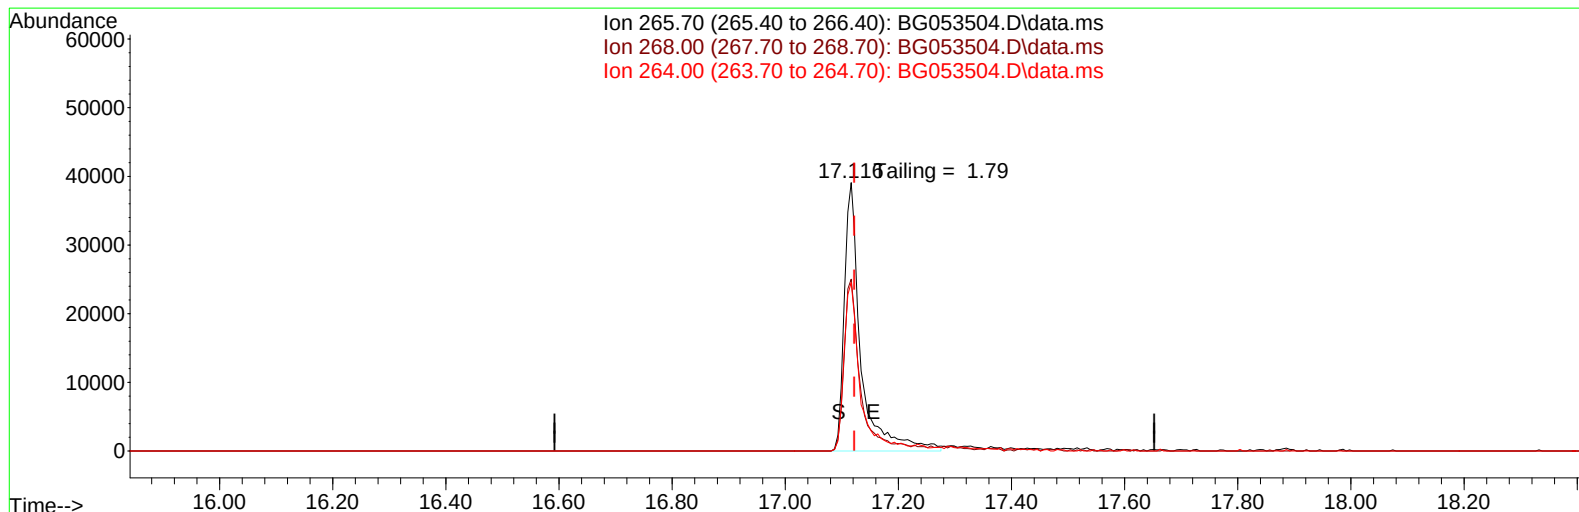

TIC: BG053504.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.006) 24102.21 ng

response 78775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.02
264.00	66.20	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053504.D
Acq On : 10 May 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 13:53:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

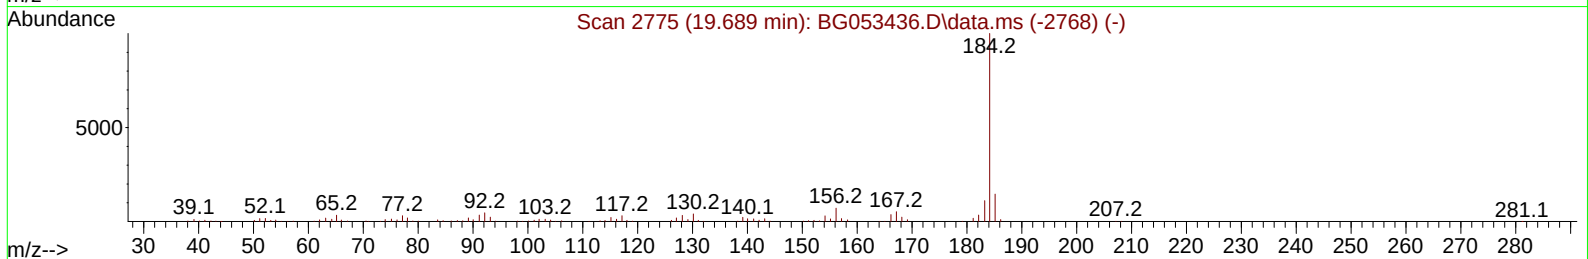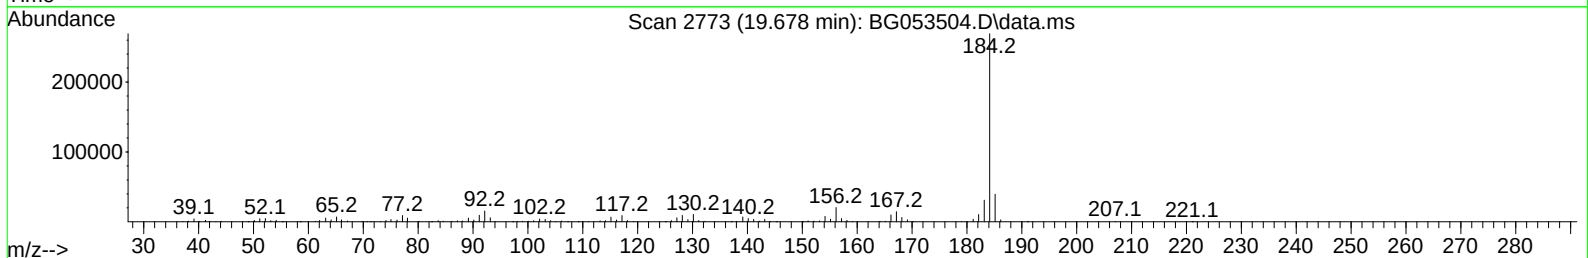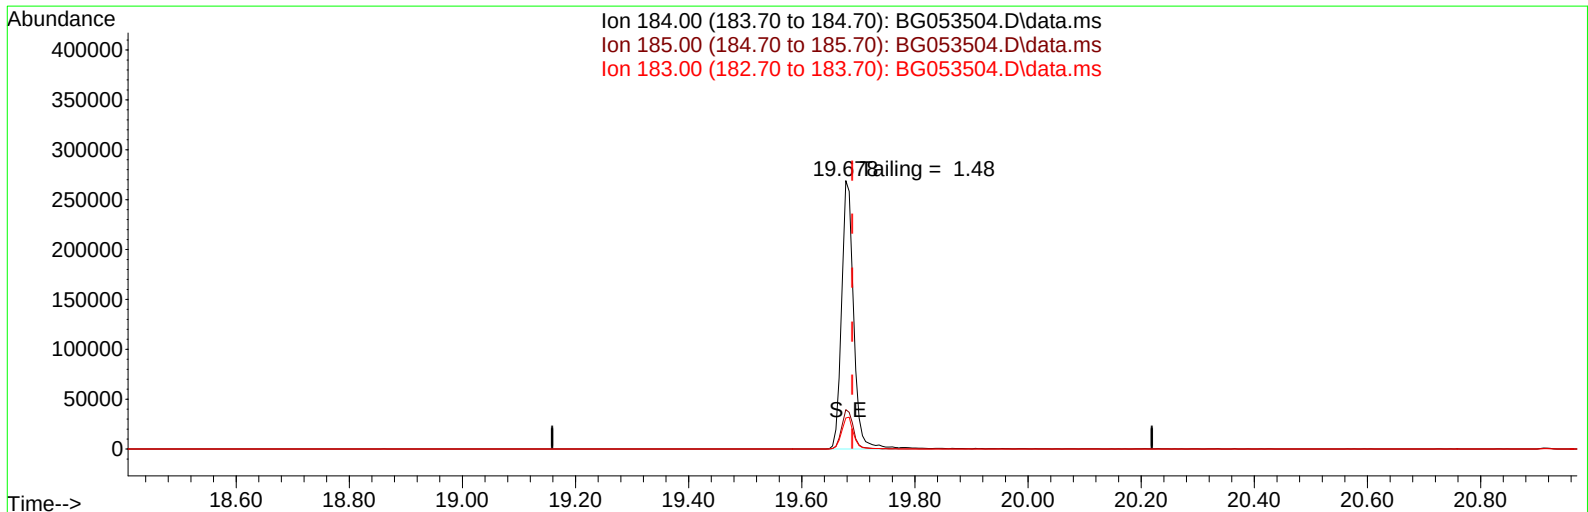

TIC: BG053504.D\data.ms

(77) Benzidine

19.678min (-0.011) 0.00 ng

response 396316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	11.10	11.57
0.00	0.00	0.00