

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
 Data File : BG053511.D
 Acq On : 10 May 2022 17:00
 Operator : CG/JU
 Sample : N2763-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-4-20220509

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.650	380	385	399	rBV	176264	304996	13.64%	3.976%
2	7.248	649	657	672	rBV	104792	202586	9.06%	2.641%
3	8.088	794	800	808	rVB	78395	135065	6.04%	1.761%
4	9.245	990	997	1008	rVB	294419	550994	24.63%	7.184%
5	10.896	1267	1278	1290	rBV	98906	186465	8.34%	2.431%
6	13.334	1686	1693	1700	rBV	832706	1288546	57.61%	16.800%
7	14.709	1921	1927	1935	rBV	166206	270130	12.08%	3.522%
8	16.195	2174	2180	2204	rBV	629126	1054346	47.14%	13.746%
9	17.458	2388	2395	2402	rBV	247345	383434	17.14%	4.999%
10	19.608	2757	2761	2769	rBV3	11806	22827	1.02%	0.298%
11	20.060	2832	2838	2850	rVB	1701683	2236673	100.00%	29.161%
12	21.734	3117	3123	3131	rVB	323449	527421	23.58%	6.876%
13	25.012	3671	3681	3694	rVB2	179253	506598	22.65%	6.605%




Sum of corrected areas: 7670081

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053511.D
Acq On : 10 May 2022 17:00
Operator : CG/JU
Sample : N2763-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-4-20220509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

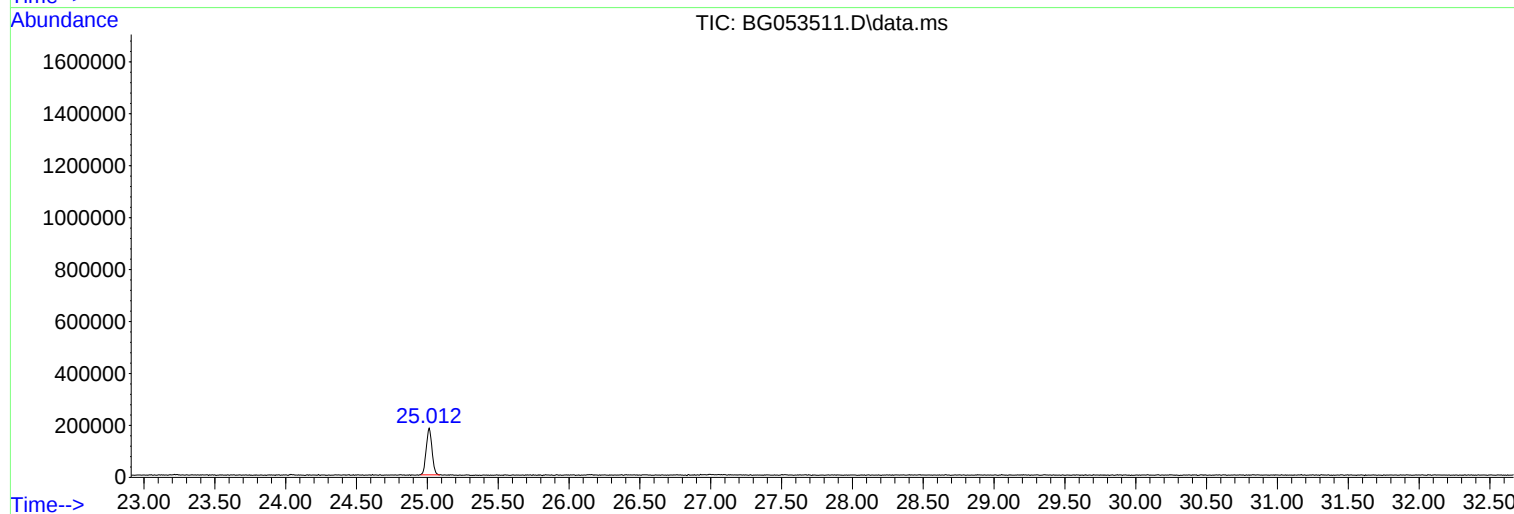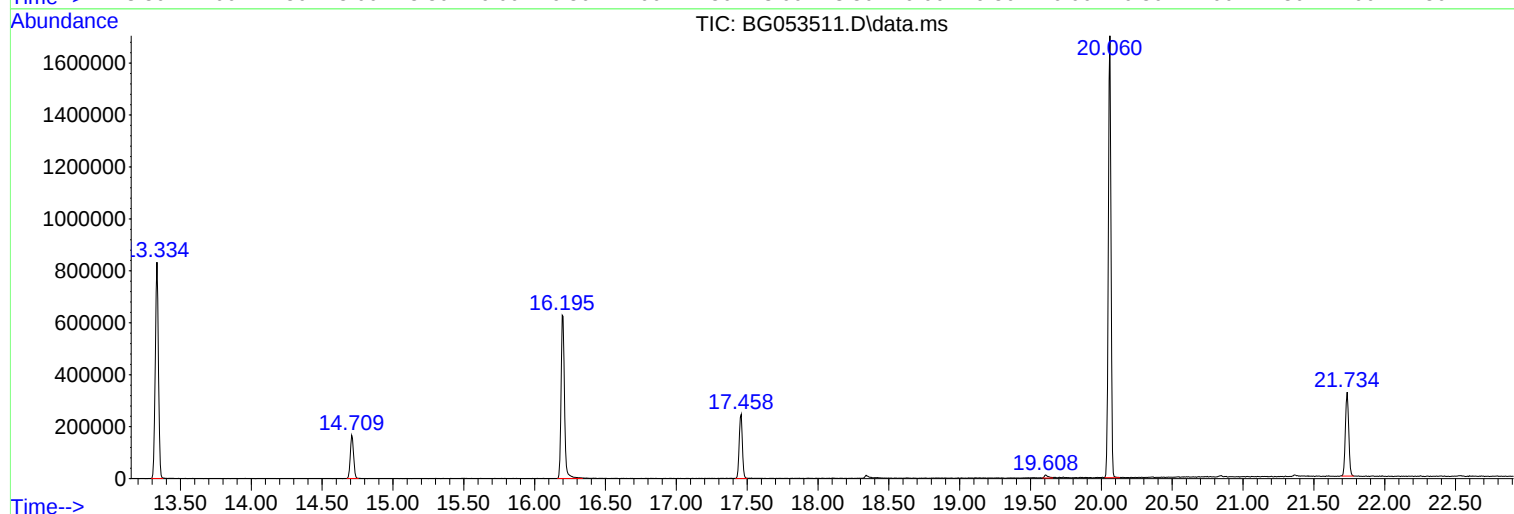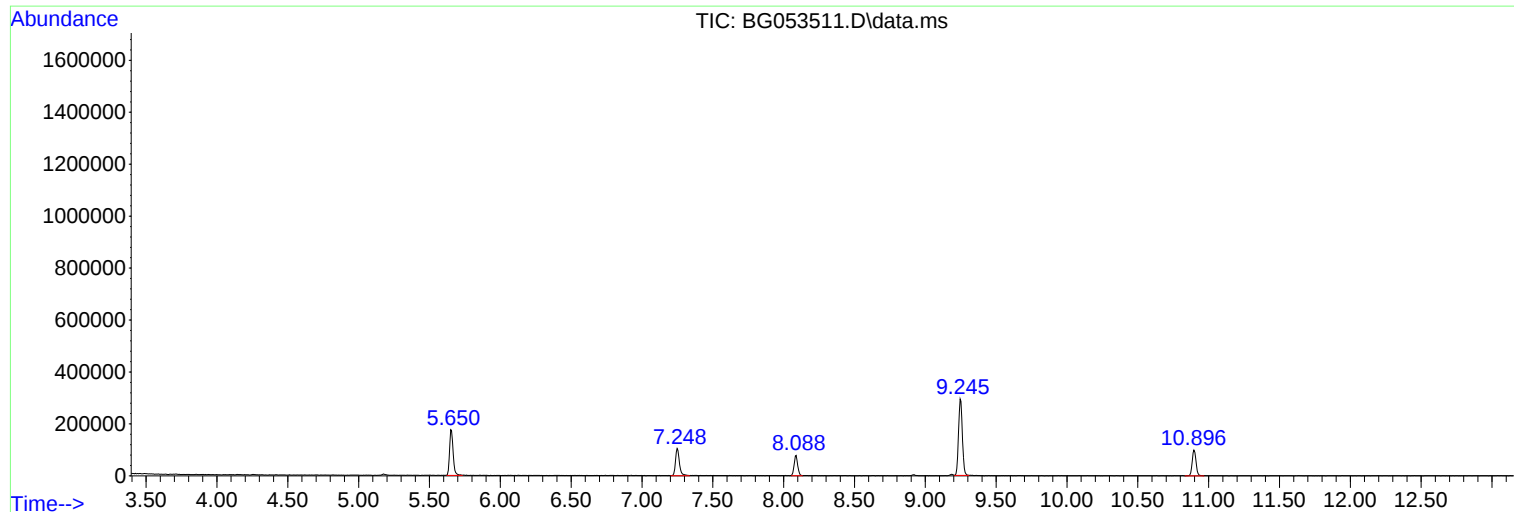

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053511.D
Acq On : 10 May 2022 17:00
Operator : CG/JU
Sample : N2763-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-4-20220509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053511.D
Acq On : 10 May 2022 17:00
Operator : CG/JU
Sample : N2763-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-4-20220509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------