

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
 Data File : BG053514.D
 Acq On : 10 May 2022 18:56
 Operator : CG/JU
 Sample : N2731-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-303-20220505

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.652	379	385	397	rBV	209849	357066	12.59%	4.107%
2	7.250	651	657	670	rBV	128367	239368	8.44%	2.753%
3	8.090	792	800	808	rBV	78782	139457	4.92%	1.604%
4	9.247	989	997	1013	rBV	309686	585197	20.64%	6.731%
5	10.898	1268	1278	1288	rBV	105865	192528	6.79%	2.214%
6	13.336	1686	1693	1704	rBV	859447	1368337	48.27%	15.738%
7	14.710	1921	1927	1938	rVB	176971	284863	10.05%	3.276%
8	16.196	2173	2180	2198	rBV	693619	1119163	39.48%	12.872%
9	17.454	2387	2394	2404	rBV	256828	398863	14.07%	4.588%
10	20.062	2831	2838	2843	rBV	2066683	2834988	100.00%	32.607%
11	21.354	3053	3058	3071	rBV2	36572	78824	2.78%	0.907%
12	21.736	3116	3123	3132	rBV	323994	557285	19.66%	6.410%
13	25.008	3669	3680	3691	rBV2	184671	538512	19.00%	6.194%




Sum of corrected areas: 8694451

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053514.D
Acq On : 10 May 2022 18:56
Operator : CG/JU
Sample : N2731-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-303-20220505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

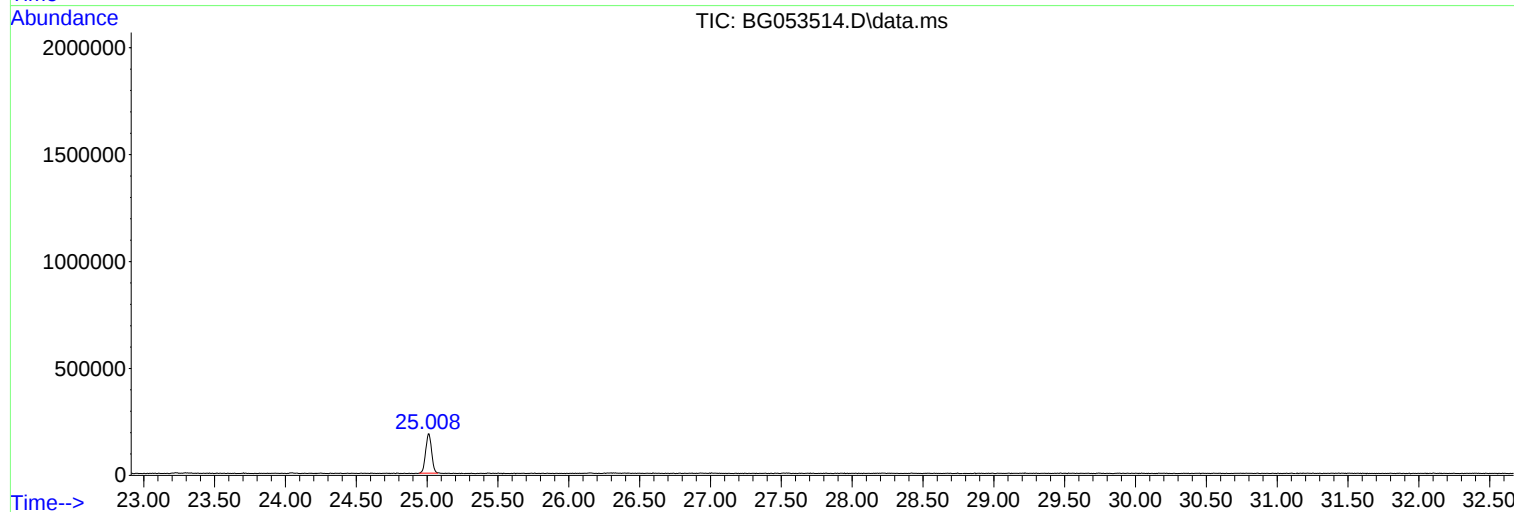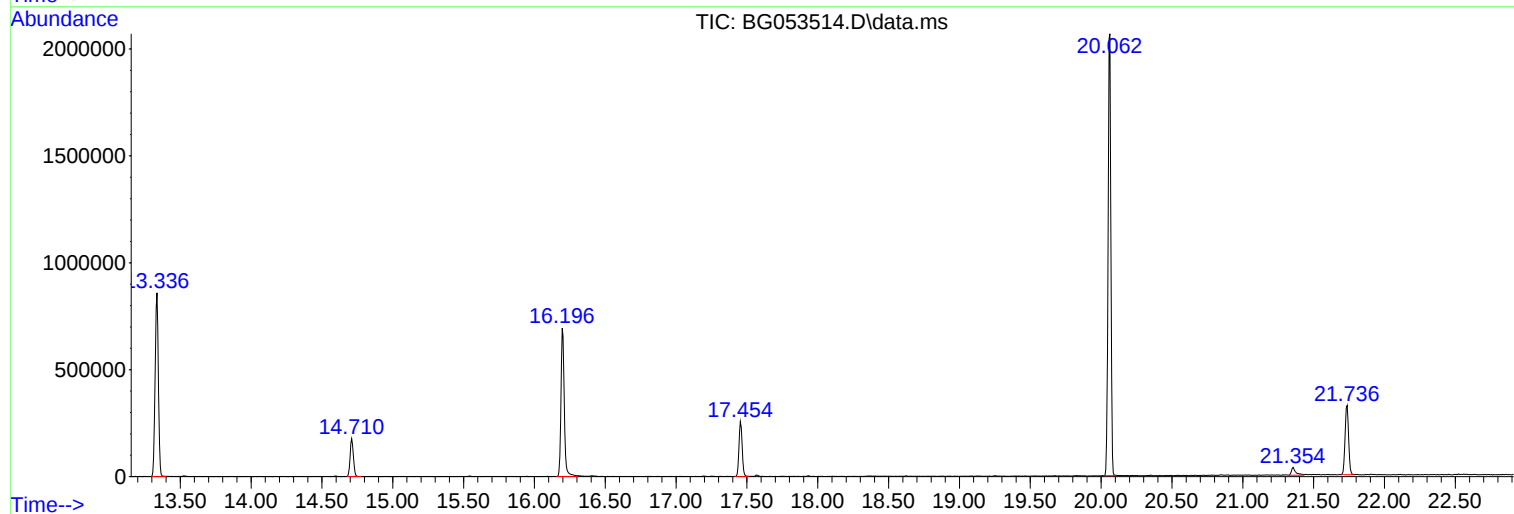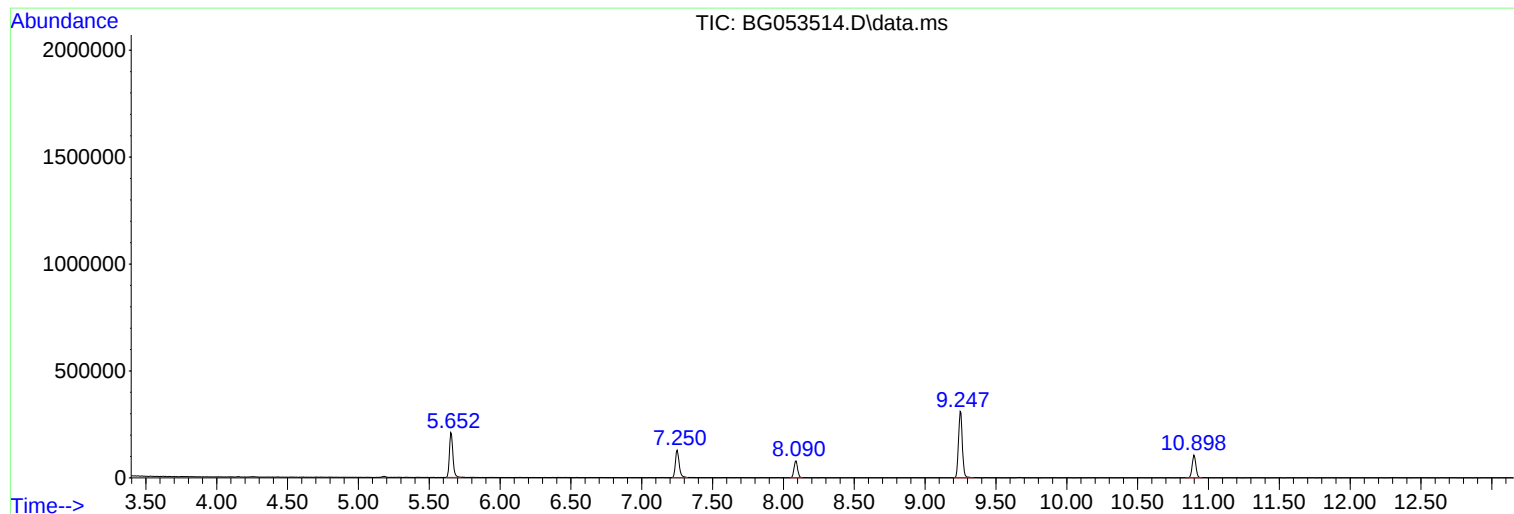

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053514.D
Acq On : 10 May 2022 18:56
Operator : CG/JU
Sample : N2731-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-303-20220505










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Bromoacetic acid, octadecyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.354	2.83 ng	78824	Chrysene-d12	21.736

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	94
2			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	91
3			Behenic alcohol	326	C22H46O	000661-19-8	91
4			2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	91
5			1-Tetracosene	336	C24H48	010192-32-2	91

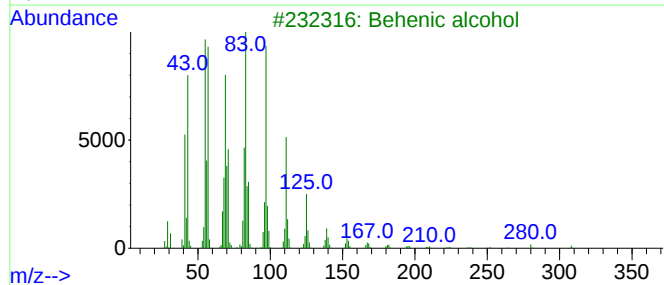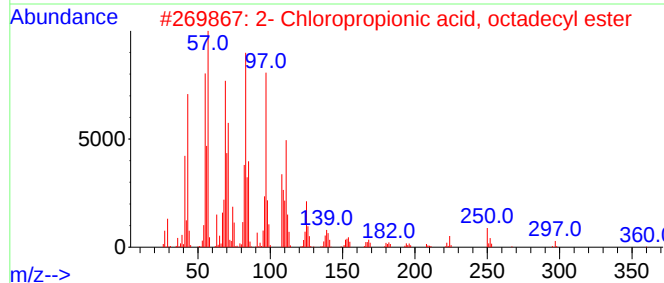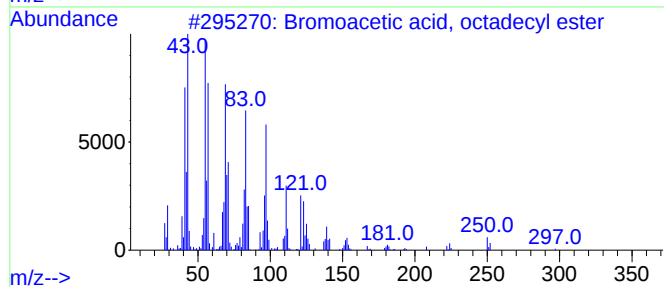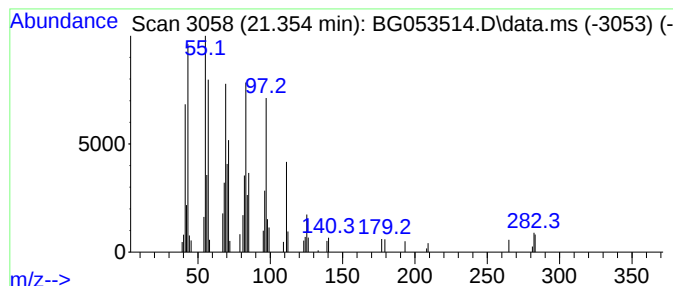

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053514.D
Acq On : 10 May 2022 18:56
Operator : CG/JU
Sample : N2731-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-303-20220505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bromoacetic aci...	21.354	2.8	ng	78824	5	21.736	557285	20.0