
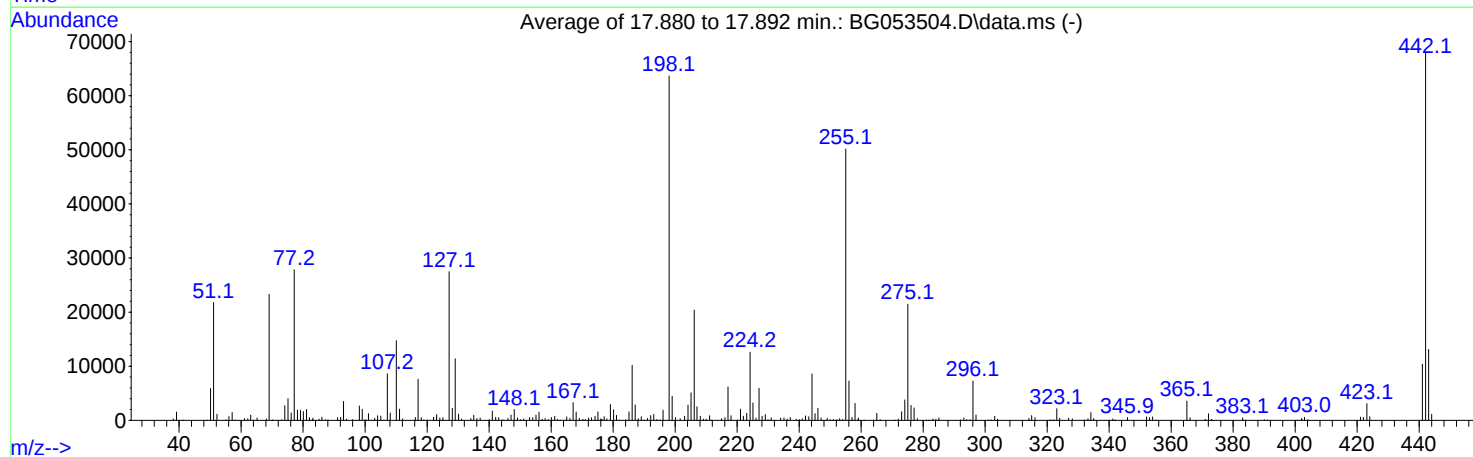


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
 Data File : BG053504.D
 Acq On : 10 May 2022 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

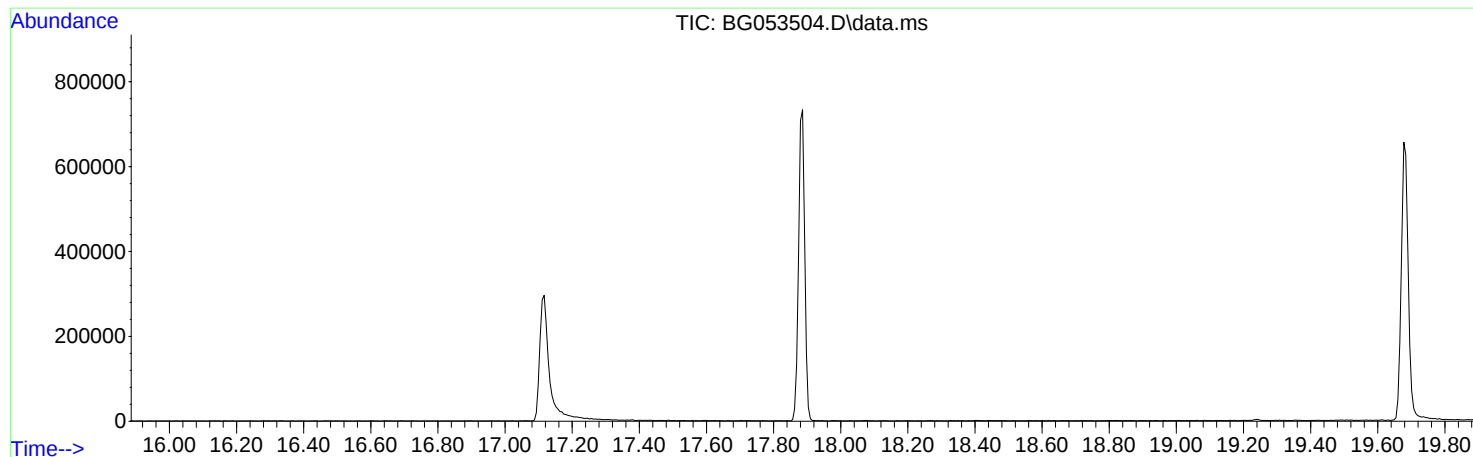




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	21752	PASS
68	69	0.00	2	1.2	278	PASS
69	198	0.00	100	36.6	23298	PASS
70	69	0.00	2	0.3	65	PASS
127	198	10	80	43.2	27475	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63632	PASS
199	198	5	9	7.0	4443	PASS
275	198	10	60	33.7	21475	PASS
365	198	1	100	5.6	3564	PASS
441	198	0.01	100	16.3	10368	PASS
442	442	50	100	100.0	67981	PASS
443	442	15	24	19.3	13093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053504.D
Acq On : 10 May 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 10 13:53:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

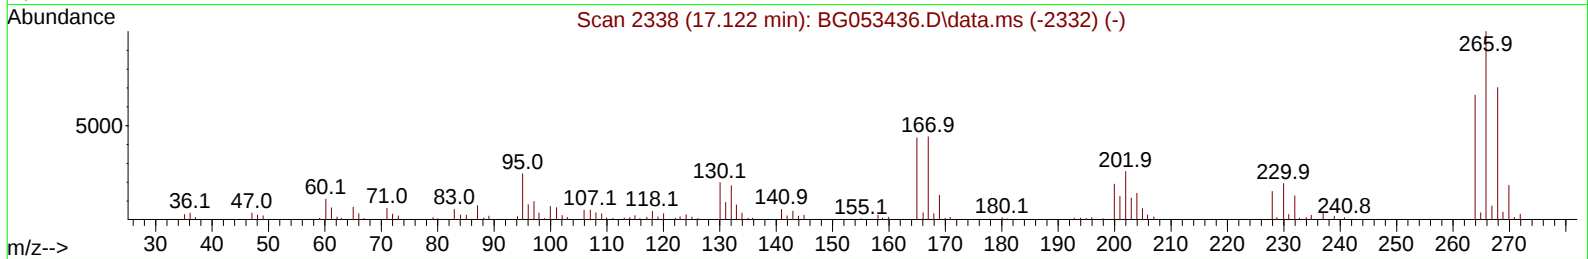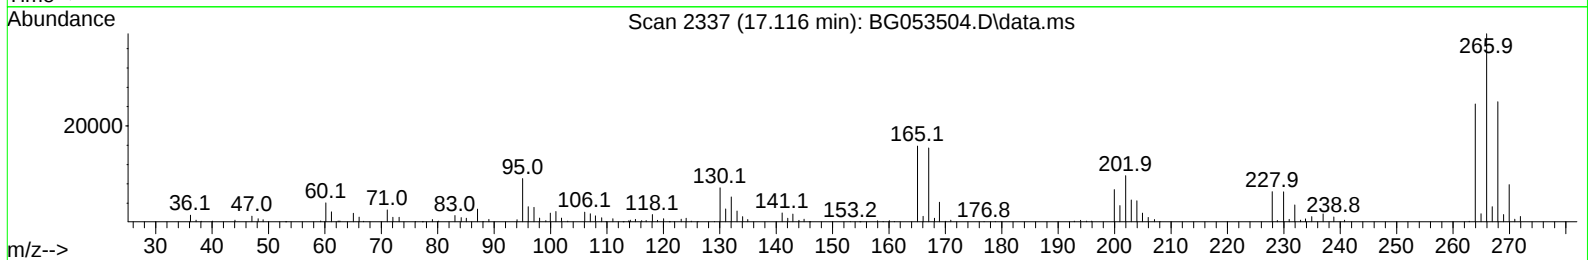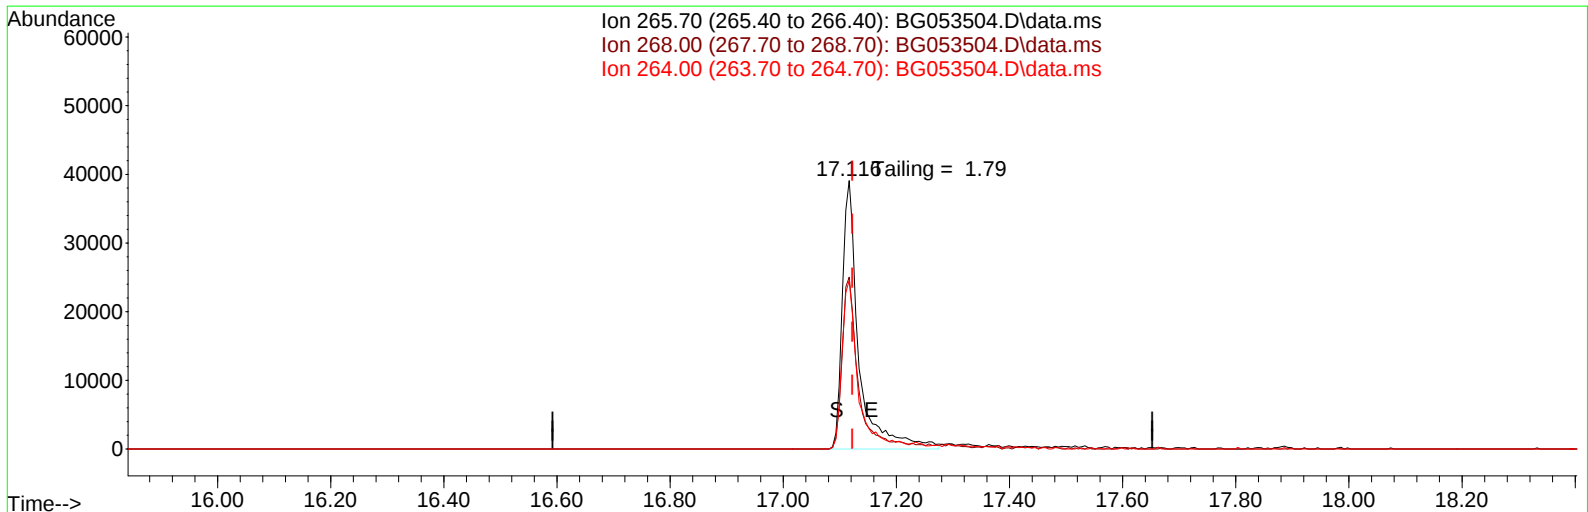

TIC: BG053504.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.006) 24102.21 ng




response 78775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.02
264.00	66.20	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051022\
Data File : BG053504.D
Acq On : 10 May 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 10 13:53:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

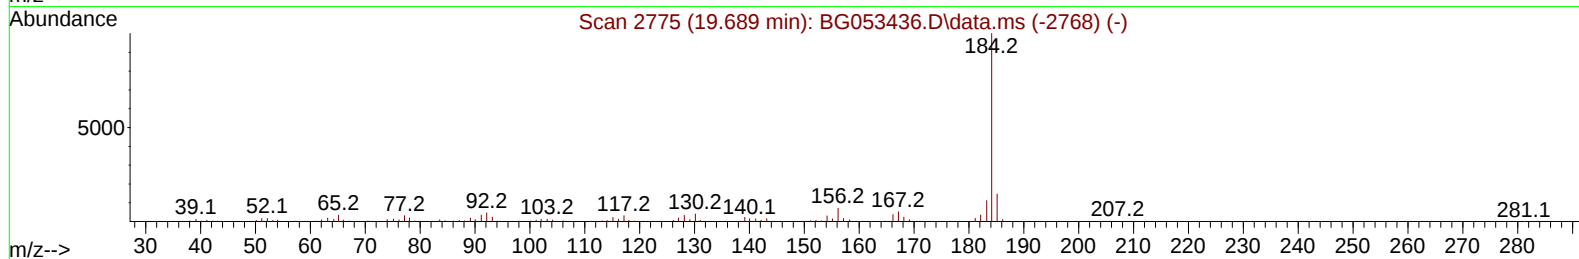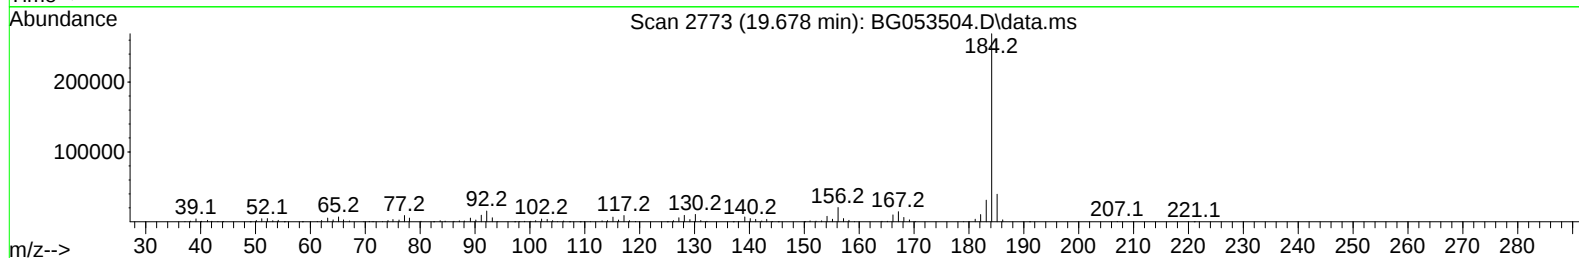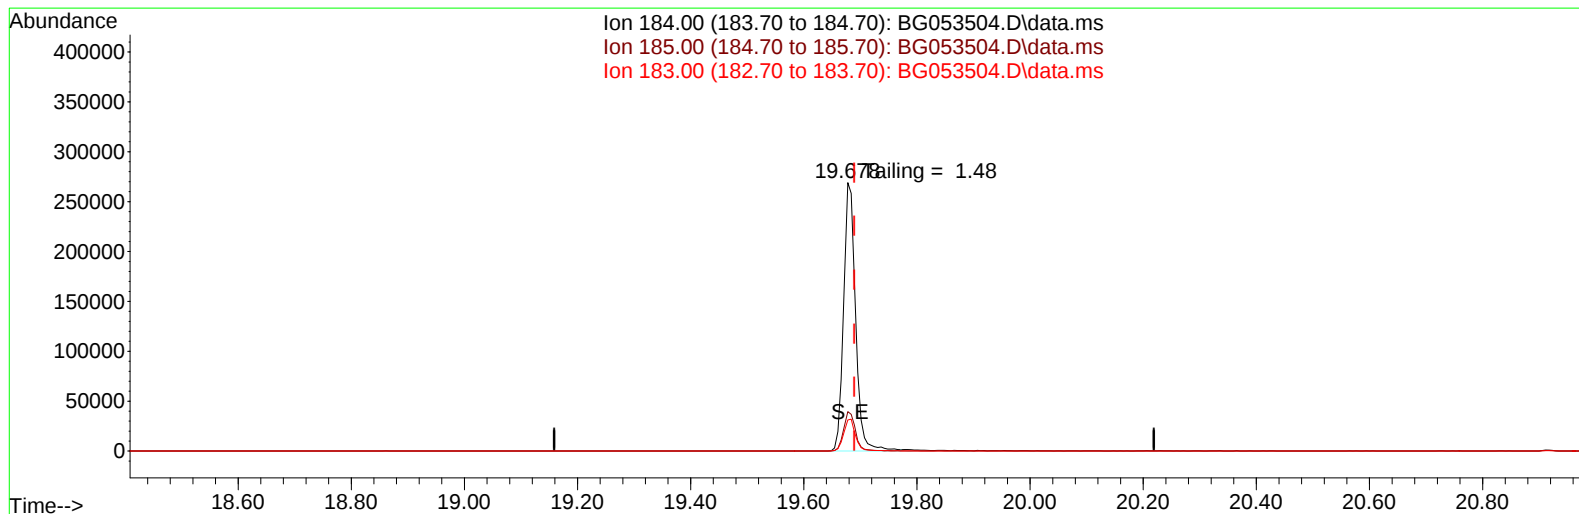

TIC: BG053504.D\data.ms

(77) Benzidine

19.678min (-0.011) 0.00 ng

response 396316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	11.10	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2022	BNA_G	BG053504.D
Compound Name	Response	Retention Time
DDT	240186	20.917
DDD	5395	20.477
DDE	505	19.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5900	246086	2.40

Instrument :
BNA_G
ClientSampleId :
DFTPP