

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
 Data File : BG057379.D
 Acq On : 10 May 2023 21:42
 Operator : CG/JU
 Sample : 02591-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JREB7

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/11/2023
 Supervised By : Jagrut Upadhyay 05/11/2023

Quant Time: May 11 00:29:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 10 11:18:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.369	152	14963	20.000	ng/u1	0.00
20) Naphthalene-d8	11.201	136	65047	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.978	164	50175	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.716	188	123376	20.000	ng/u1	0.00
79) Chrysene-d12	22.027	240	108563	20.000	ng/u1	# 0.00
88) Perylene-d12	25.534	264	118484	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.646	96	832	2.447	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.506	99	20423	14.433	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.664	67	11553	13.881	ng/u1	0.00
11) 2-Chlorophenol-d4	7.888	132	14475	15.523	ng/u1	0.00
15) 4-Methylphenol-d8	9.068	113	13947	12.968	ng/u1	0.00
21) Nitrobenzene-d5	9.538	128	7910	15.270	ng/u1	0.00
24) 2-Nitrophenol-d4	10.273	143	9099	15.051	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.819	165	18222	15.623	ng/u1	0.00
31) 4-Chloroaniline-d4	11.330	131	17186	11.118	ng/u1	0.00
46) Dimethylphthalate-d6	14.361	166	63116	15.875	ng/u1	0.00
49) Acenaphthylene-d8	14.679	160	70907	15.868	ng/u1	0.00
54) 4-Nitrophenol-d4	15.178	143	5452	9.421	ng/u1	0.00
60) Fluorene-d10	15.959	176	56834	15.345	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.083	200	7338m	10.039	ng/u1	0.00
73) Anthracene-d10	17.815	188	91660	16.276	ng/u1	0.00
81) Pyrene-d10	20.083	212	113678	17.641	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.288	264	103588	17.160	ng/u1	0.00

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.881	149	3994762	1106.799	ng/u1# 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057379.D
Acq On : 10 May 2023 21:42
Operator : CG/JU
Sample : 02591-10
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JREB7

Quant Time: May 11 00:29:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 10 11:18:43 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 05/11/2023
Supervised By : Jagrut Upadhyay 05/11/2023

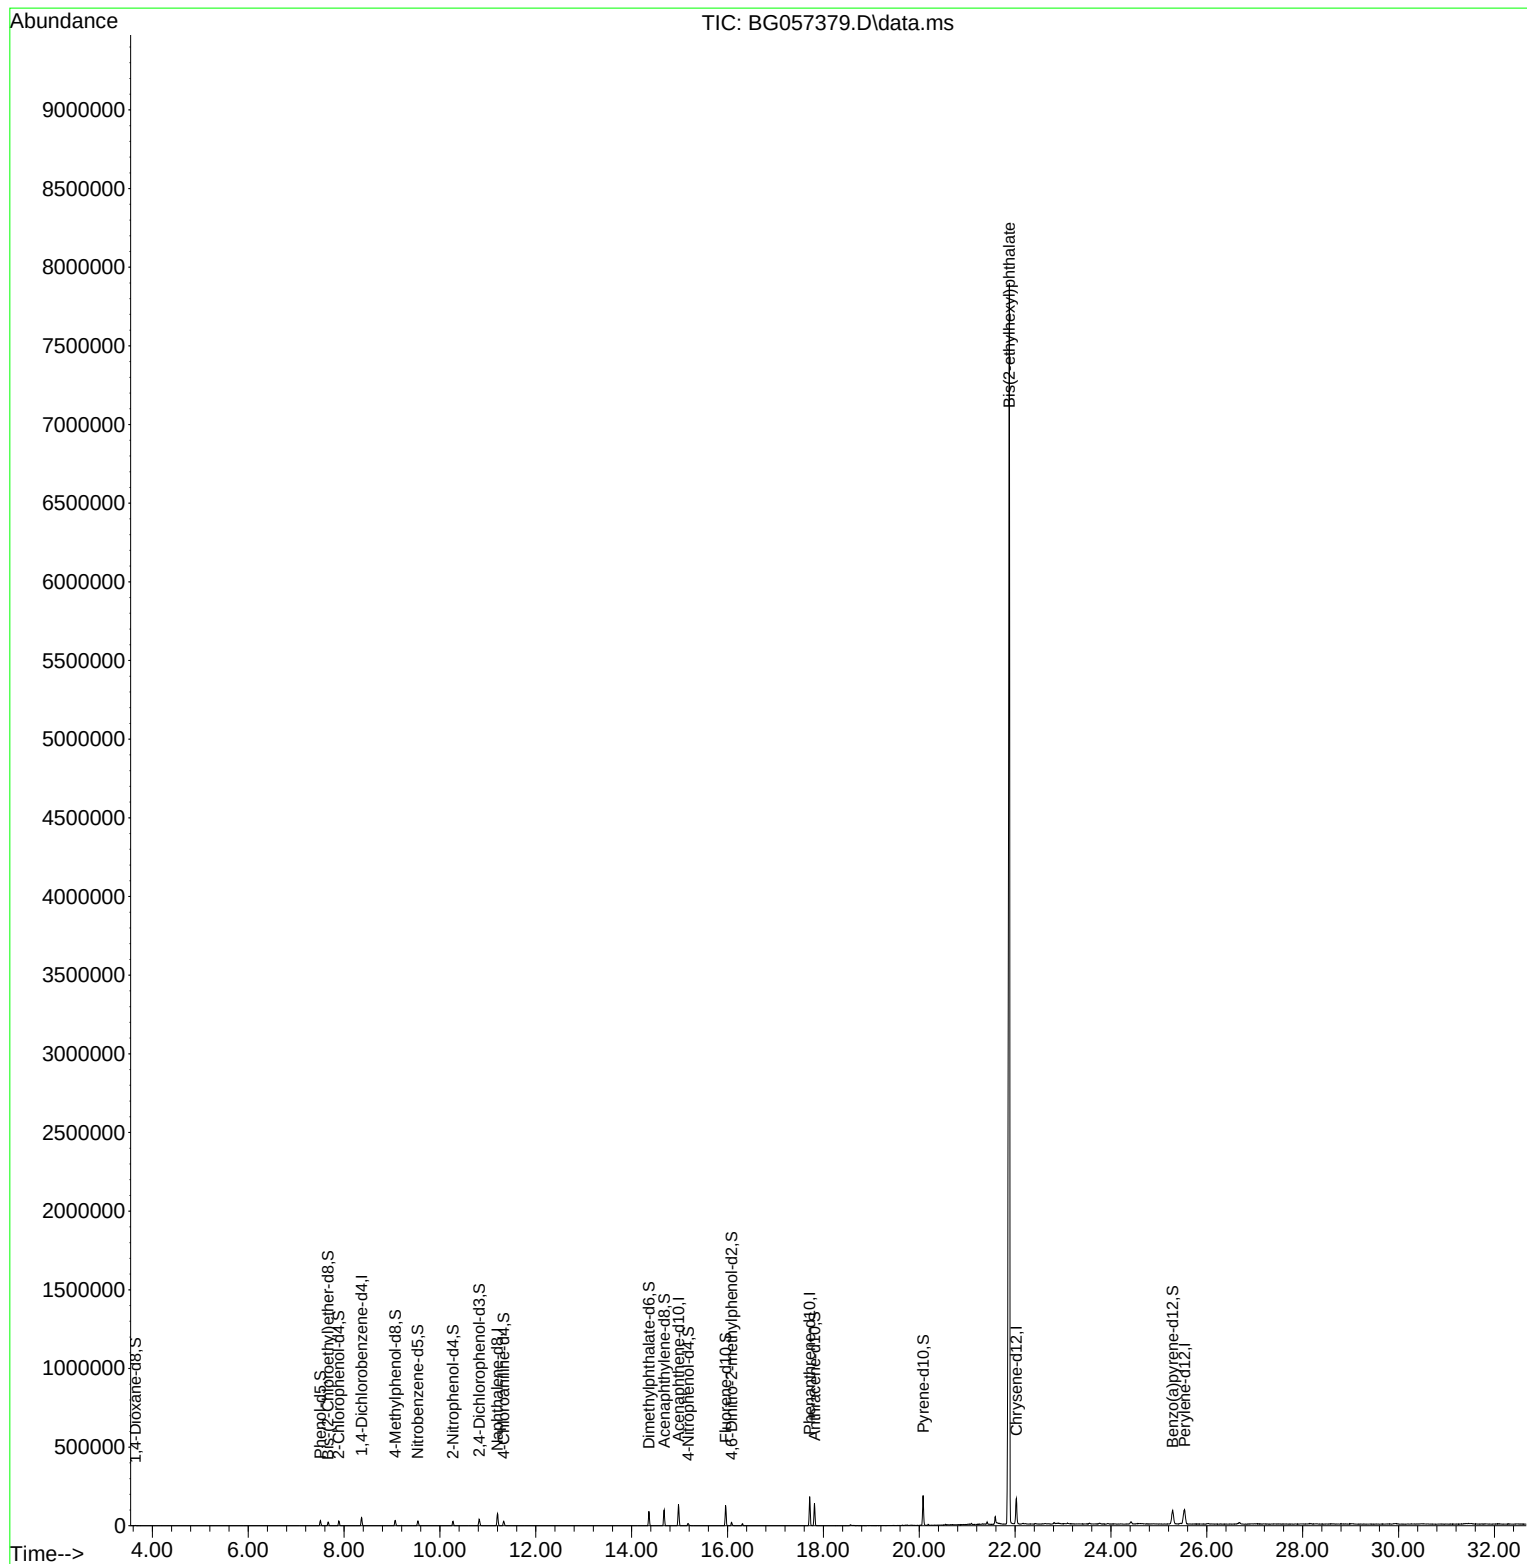

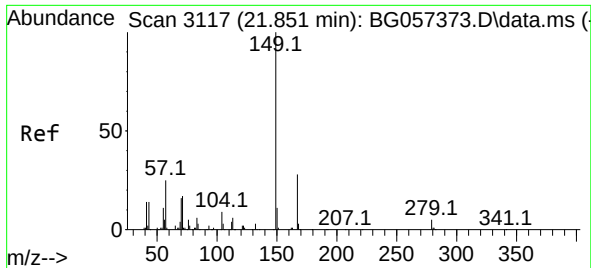

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1106.799 ng/ul
 RT: 21.881 min Scan# 3117
 Delta R.T. 0.032 min
 Lab File: BG057379.D
 Acq: 10 May 2023 21:42

Instrument :
 BNA_G
 ClientSampleId :
 JREB7

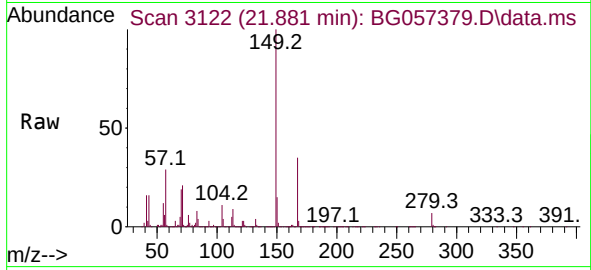

Tgt Ion:149 Resp: 3994762
 Ion Ratio Lower Upper
 149 100
 167 35.4 23.0 34.6
 279 7.2 3.6 5.4

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 05/11/2023
 Supervised By :Jagrut Upadhyay 05/11/2023

