

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
 Data File : BG057365.D
 Acq On : 10 May 2023 11:12
 Operator : CG/JU
 Sample : PB152684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK684

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.644	13	18	23	rVB	3991	5743	0.87%	0.097%
2	3.756	34	37	42	rVB2	717	1273	0.19%	0.021%
3	3.808	42	46	48	rBV2	648	976	0.15%	0.016%
4	4.085	91	93	108	rBV	52202	91084	13.82%	1.536%
5	4.184	108	110	113	rVV	1196	1602	0.24%	0.027%
6	4.443	151	154	160	rVB2	917	1527	0.23%	0.026%
7	7.503	669	675	685	rBV	73716	129553	19.66%	2.185%
8	7.674	697	704	713	rBB	58779	98305	14.92%	1.658%
9	7.891	735	741	750	rBB	72382	126262	19.16%	2.129%
10	8.367	816	822	829	rBB	56029	91030	13.82%	1.535%
11	9.066	935	941	953	rBV	94545	166768	25.31%	2.812%
12	9.542	1015	1022	1032	rBV	75908	135954	20.63%	2.293%
13	10.270	1140	1146	1156	rBB	66562	119685	18.17%	2.018%
14	10.817	1233	1239	1252	rBV	91658	173883	26.39%	2.932%
15	11.204	1298	1305	1313	rBV	77877	137237	20.83%	2.314%
16	11.328	1319	1326	1338	rBV	92838	176750	26.83%	2.981%
17	12.761	1565	1570	1576	rBV3	1448	2631	0.40%	0.044%
18	14.365	1836	1843	1853	rBV	228694	321930	48.86%	5.429%
19	14.676	1889	1896	1905	rBV	240842	367962	55.85%	6.205%
20	14.976	1940	1947	1955	rVB	143831	225297	34.19%	3.799%
21	15.164	1973	1979	1995	rBV	58247	113004	17.15%	1.906%
22	15.963	2108	2115	2125	rBV	328179	478974	72.70%	8.077%
23	16.080	2131	2135	2148	rBV	70451	118822	18.03%	2.004%
24	16.198	2153	2155	2158	rVB	852	1001	0.15%	0.017%
25	17.719	2408	2414	2424	rVV	200353	301006	45.69%	5.076%
26	17.819	2424	2431	2440	rBV	354311	539237	81.84%	9.093%
27	19.282	2677	2680	2683	rVB2	774	834	0.13%	0.014%
28	19.487	2713	2715	2718	rVB2	645	695	0.11%	0.012%
29	19.646	2738	2742	2748	rVB4	4279	6897	1.05%	0.116%
30	19.722	2750	2755	2758	rBV	4536	5997	0.91%	0.101%
31	19.893	2782	2784	2785	rBV	1297	999	0.15%	0.017%
32	20.086	2810	2817	2823	rBV	448124	658867	100.00%	11.111%
33	20.263	2844	2847	2848	rBV2	763	760	0.12%	0.013%
34	20.380	2864	2867	2868	rBV2	777	887	0.13%	0.015%
35	20.462	2877	2881	2886	rBV4	1092	1916	0.29%	0.032%
36	20.515	2889	2890	2894	rBV3	1344	1910	0.29%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
 Data File : BG057365.D
 Acq On : 10 May 2023 11:12
 Operator : CG/JU
 Sample : PB152684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK684

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	20.586	2901	2902	2904	rBV2	984	790	0.12%	0.013%
38	20.603	2904	2905	2908	rVB2	1253	665	0.10%	0.011%
39	20.868	2946	2950	2953	rBV4	1136	1376	0.21%	0.023%
40	20.985	2968	2970	2973	rVB3	1358	813	0.12%	0.014%
41	21.062	2981	2983	2985	rBV2	1196	1329	0.20%	0.022%
42	21.555	3066	3067	3069	rBV	1384	727	0.11%	0.012%
43	21.702	3088	3092	3096	rBV4	1974	2813	0.43%	0.047%
44	22.025	3141	3147	3155	rBV2	190721	330294	50.13%	5.570%
45	22.360	3203	3204	3206	rVB	1714	843	0.13%	0.014%
46	22.377	3206	3207	3208	rBV	1746	761	0.12%	0.013%
47	22.530	3232	3233	3234	rBV	1812	798	0.12%	0.013%
48	22.812	3280	3281	3284	rVB3	1639	789	0.12%	0.013%
49	22.871	3288	3291	3293	rBV4	1633	2174	0.33%	0.037%
50	23.212	3347	3349	3350	rBV	1235	898	0.14%	0.015%
51	23.905	3465	3467	3468	rBV2	1877	1211	0.18%	0.020%
52	24.539	3573	3575	3577	rBV2	1407	1533	0.23%	0.026%
53	25.297	3693	3704	3718	rVB2	213398	615100	93.36%	10.373%
54	25.438	3725	3728	3729	rBV2	3454	3523	0.53%	0.059%
55	25.538	3735	3745	3756	rVB	105867	321902	48.86%	5.428%
56	25.655	3763	3765	3768	rVB3	1510	1238	0.19%	0.021%
57	26.390	3888	3890	3891	rBV2	2091	1305	0.20%	0.022%
58	26.448	3899	3900	3903	rBV3	1628	1679	0.25%	0.028%
59	26.648	3930	3934	3935	rBV3	2738	2759	0.42%	0.047%
60	26.895	3974	3976	3977	rBV	1609	1000	0.15%	0.017%
61	27.042	3999	4001	4003	rBV2	2365	1925	0.29%	0.032%
62	27.470	4072	4074	4075	rBV2	1634	1104	0.17%	0.019%
63	27.700	4111	4113	4114	rVB	1628	951	0.14%	0.016%
64	27.993	4161	4163	4164	rBV2	1427	1168	0.18%	0.020%
65	28.070	4174	4176	4177	rBV2	1456	1151	0.17%	0.019%
66	28.634	4269	4272	4275	rBV4	2375	3622	0.55%	0.061%
67	28.992	4329	4333	4335	rBV4	1693	2748	0.42%	0.046%
68	29.098	4348	4351	4355	rBV5	1623	3170	0.48%	0.053%
69	29.715	4454	4456	4459	rBV3	1334	1393	0.21%	0.023%
70	29.861	4479	4481	4486	rBV5	1463	1900	0.29%	0.032%
71	30.061	4513	4515	4518	rBV3	1503	1143	0.17%	0.019%
72	30.954	4665	4667	4668	rBV2	1600	1095	0.17%	0.018%
73	30.989	4671	4673	4674	rBV2	1673	865	0.13%	0.015%
74	31.118	4693	4695	4698	rBV3	1494	1625	0.25%	0.027%
75	31.412	4743	4745	4746	rBV	1254	683	0.10%	0.012%
76	31.541	4765	4767	4768	rBV2	1594	999	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057365.D
Acq On : 10 May 2023 11:12
Operator : CG/JU
Sample : PB152684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK684

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Title : SVOA CALIBRATION

77	31.941	4833	4835	4836	rVB2	1754	808	0.12%	0.014%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 5929928

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057365.D
Acq On : 10 May 2023 11:12
Operator : CG/JU
Sample : PB152684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

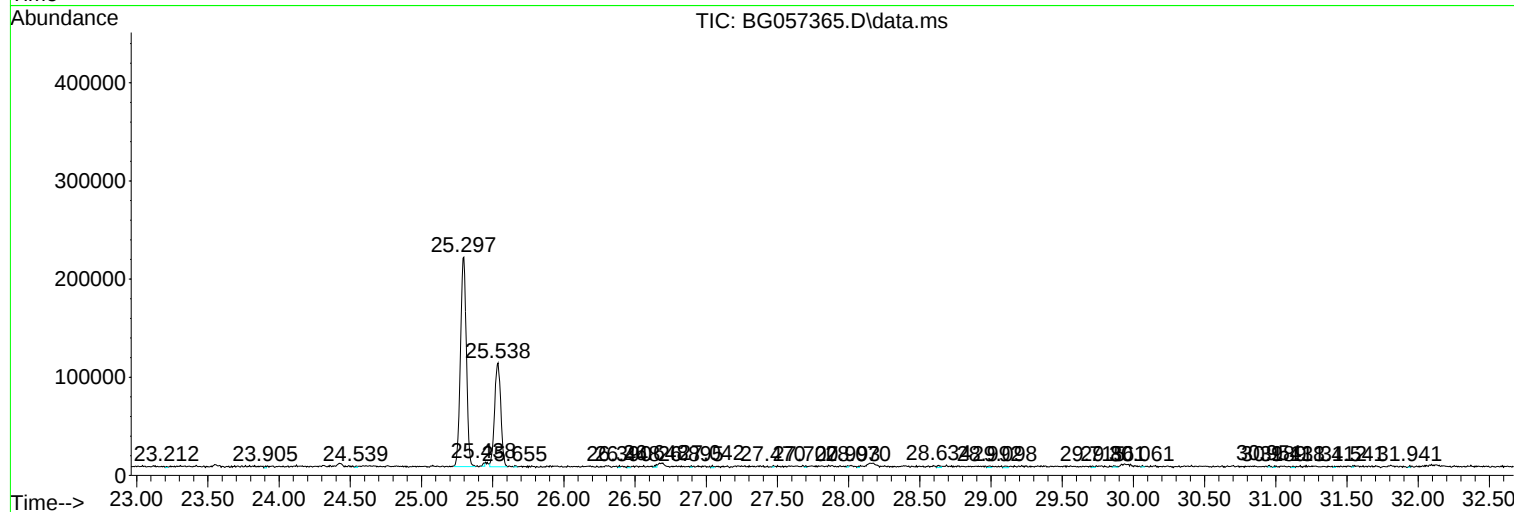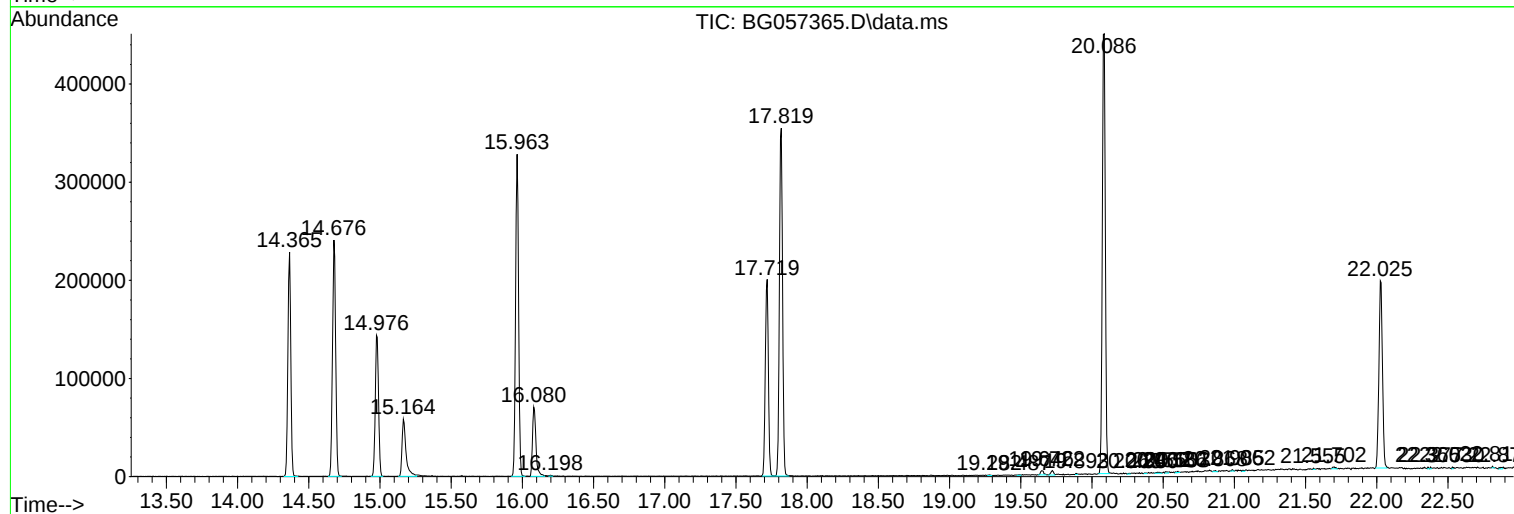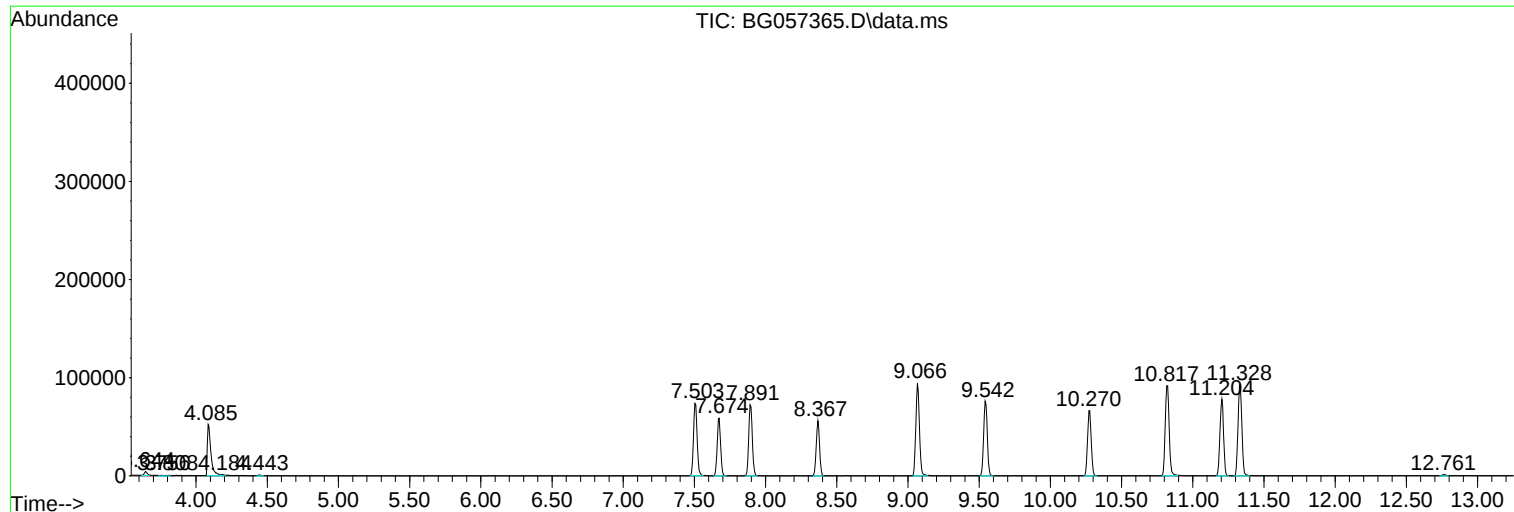

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057365.D
Acq On : 10 May 2023 11:12
Operator : CG/JU
Sample : PB152684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057365.D
Acq On : 10 May 2023 11:12
Operator : CG/JU
Sample : PB152684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------