

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
 Data File : BG057374.D
 Acq On : 10 May 2023 18:15
 Operator : CG/JU
 Sample : PB152674BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK674

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.644	14	18	23	rVB2	3066	5049	0.86%	0.091%
2	3.908	59	63	65	rBV	609	1173	0.20%	0.021%
3	4.084	90	93	108	rBV	47194	83431	14.26%	1.512%
4	4.184	108	110	115	rVB	1035	1478	0.25%	0.027%
5	4.390	143	145	150	rVB2	422	737	0.13%	0.013%
6	4.437	150	153	158	rBB	861	1379	0.24%	0.025%
7	7.503	669	675	684	rBV	69597	120754	20.64%	2.188%
8	7.668	696	703	711	rBB	53215	86780	14.83%	1.572%
9	7.891	735	741	749	rBB	66633	115009	19.66%	2.084%
10	8.367	816	822	828	rBB	59649	98661	16.87%	1.787%
11	9.066	933	941	956	rBV2	88590	154608	26.43%	2.801%
12	9.542	1015	1022	1030	rVB	70157	122011	20.86%	2.211%
13	10.270	1139	1146	1154	rBB	61464	109847	18.78%	1.990%
14	10.816	1232	1239	1250	rBV	88471	161396	27.59%	2.924%
15	11.204	1297	1305	1312	rVB	80989	146840	25.10%	2.660%
16	11.328	1320	1326	1336	rBV	80674	150657	25.75%	2.730%
17	11.956	1430	1433	1438	rBB	333	618	0.11%	0.011%
18	12.761	1566	1570	1575	rBV2	1126	1775	0.30%	0.032%
19	13.842	1750	1754	1759	rVB2	2342	3116	0.53%	0.056%
20	14.365	1836	1843	1850	rBV	203585	285322	48.78%	5.169%
21	14.676	1889	1896	1907	rBV	213452	331546	56.68%	6.007%
22	14.981	1939	1948	1955	rBV	153067	241441	41.27%	4.374%
23	15.169	1974	1980	1993	rBV2	49682	99198	16.96%	1.797%
24	15.962	2108	2115	2123	rBV	290539	432279	73.90%	7.832%
25	16.086	2131	2136	2154	rBV	51493	91728	15.68%	1.662%
26	16.203	2154	2156	2159	rBV2	985	805	0.14%	0.015%
27	17.507	2376	2378	2380	rBV	565	591	0.10%	0.011%
28	17.719	2407	2414	2421	rBV	223837	326057	55.74%	5.907%
29	17.819	2424	2431	2440	rBV	332946	487075	83.26%	8.825%
30	18.095	2477	2478	2481	rBV	637	686	0.12%	0.012%
31	19.170	2658	2661	2664	rBV2	594	994	0.17%	0.018%
32	19.217	2667	2669	2672	rVB2	679	727	0.12%	0.013%
33	19.258	2672	2676	2678	rBV3	904	1193	0.20%	0.022%
34	19.393	2697	2699	2703	rVB2	617	840	0.14%	0.015%
35	19.493	2714	2716	2719	rBV3	587	762	0.13%	0.014%
36	19.528	2719	2722	2723	rVV2	723	720	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
 Data File : BG057374.D
 Acq On : 10 May 2023 18:15
 Operator : CG/JU
 Sample : PB152674BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK674

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	19.575	2726	2730	2732	rVB3	941	922	0.16%	0.017%
38	19.646	2738	2742	2747	rBV3	4167	5408	0.92%	0.098%
39	19.722	2751	2755	2760	rVB	3723	5497	0.94%	0.100%
40	19.757	2760	2761	2764	rVB	1046	795	0.14%	0.014%
41	19.793	2764	2767	2769	rBV2	1394	1264	0.22%	0.023%
42	19.851	2776	2777	2780	rBV2	773	719	0.12%	0.013%
43	20.016	2803	2805	2807	rBV2	1270	1120	0.19%	0.020%
44	20.080	2810	2816	2825	rBV	405221	584974	100.00%	10.598%
45	20.198	2835	2836	2838	rBV	882	740	0.13%	0.013%
46	20.562	2895	2898	2899	rBV2	1253	1414	0.24%	0.026%
47	20.627	2907	2909	2911	rVB3	936	774	0.13%	0.014%
48	20.650	2911	2913	2914	rBV2	999	970	0.17%	0.018%
49	20.762	2929	2932	2934	rBV3	1526	1685	0.29%	0.031%
50	21.120	2992	2993	2996	rBV3	2039	2259	0.39%	0.041%
51	21.702	3089	3092	3097	rBV4	1996	2969	0.51%	0.054%
52	21.760	3100	3102	3103	rBV2	1354	1075	0.18%	0.019%
53	22.025	3141	3147	3156	rBV2	211172	349222	59.70%	6.327%
54	22.207	3176	3178	3181	rVB3	2270	1772	0.30%	0.032%
55	23.975	3476	3479	3482	rBV5	1730	3138	0.54%	0.057%
56	25.215	3688	3690	3691	rBV2	1958	1264	0.22%	0.023%
57	25.291	3692	3703	3715	rVV2	188039	536160	91.66%	9.714%
58	25.532	3734	3744	3758	rVB	115689	333625	57.03%	6.044%
59	26.466	3901	3903	3905	rBV2	1764	2055	0.35%	0.037%
60	26.936	3981	3983	3984	rVB2	1591	734	0.13%	0.013%
61	26.977	3988	3990	3991	rBV2	1962	1410	0.24%	0.026%
62	29.039	4339	4341	4342	rBV2	1623	783	0.13%	0.014%
63	29.456	4411	4412	4417	rBV4	2410	2925	0.50%	0.053%
64	29.644	4442	4444	4446	rBV2	2185	1332	0.23%	0.024%
65	29.720	4455	4457	4459	rVB2	1940	1358	0.23%	0.025%
66	31.647	4783	4785	4787	rBV3	1784	2359	0.40%	0.043%
67	32.311	4896	4898	4899	rBV2	1958	1559	0.27%	0.028%




Sum of corrected areas: 5519564

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057374.D
Acq On : 10 May 2023 18:15
Operator : CG/JU
Sample : PB152674BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK674

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

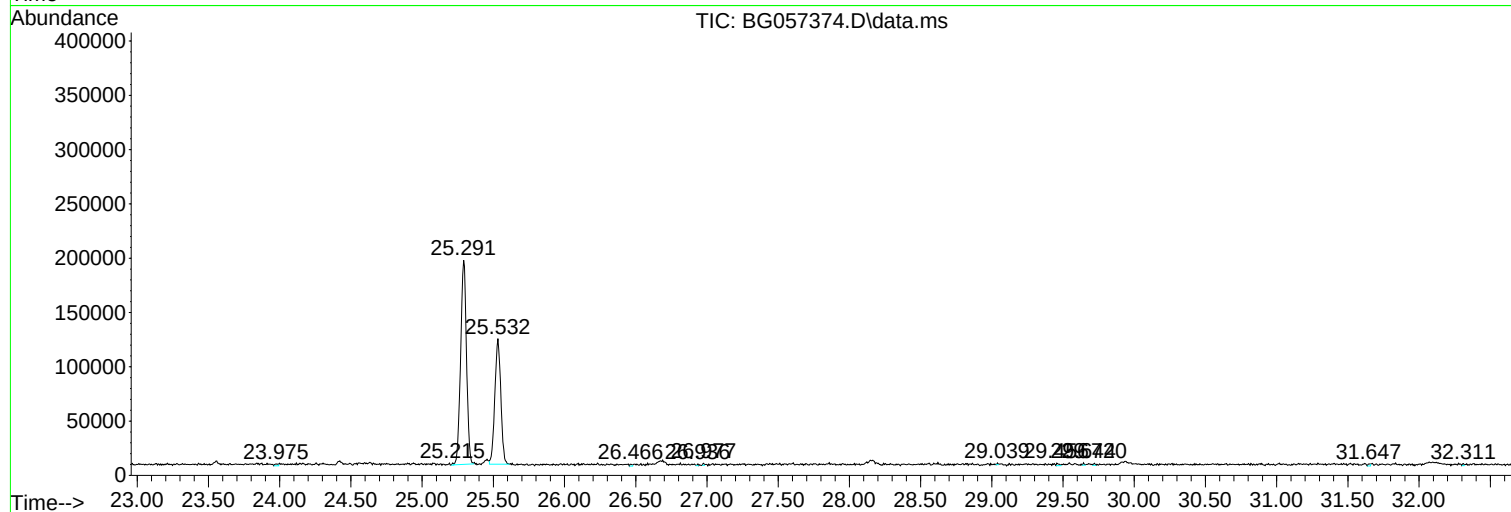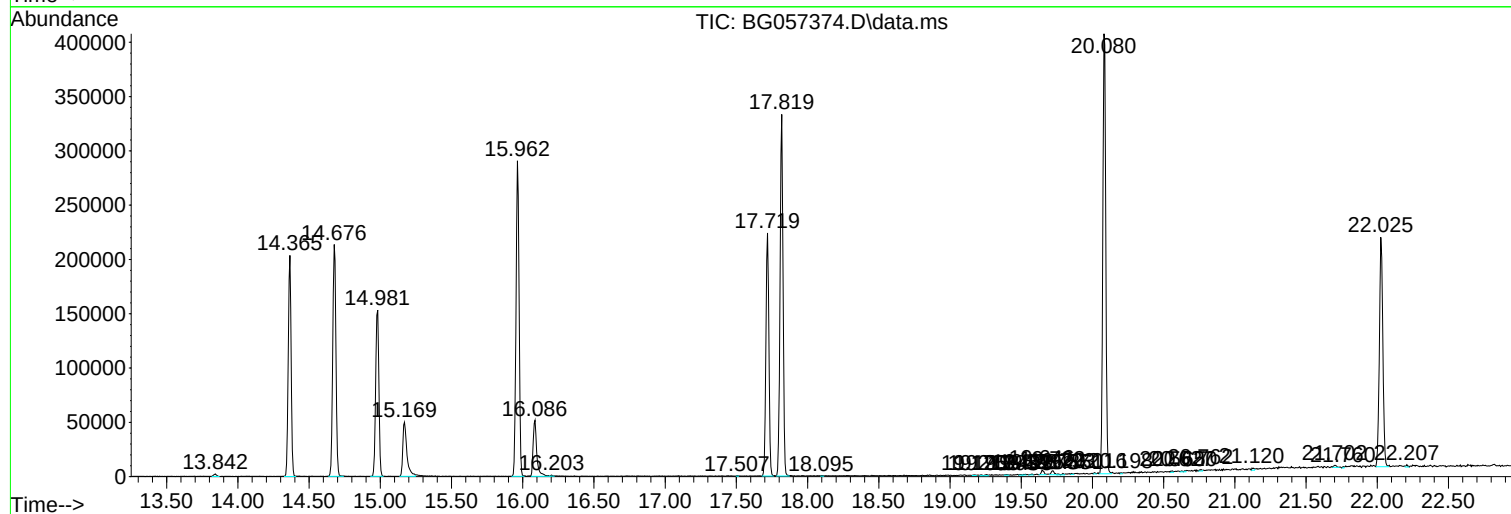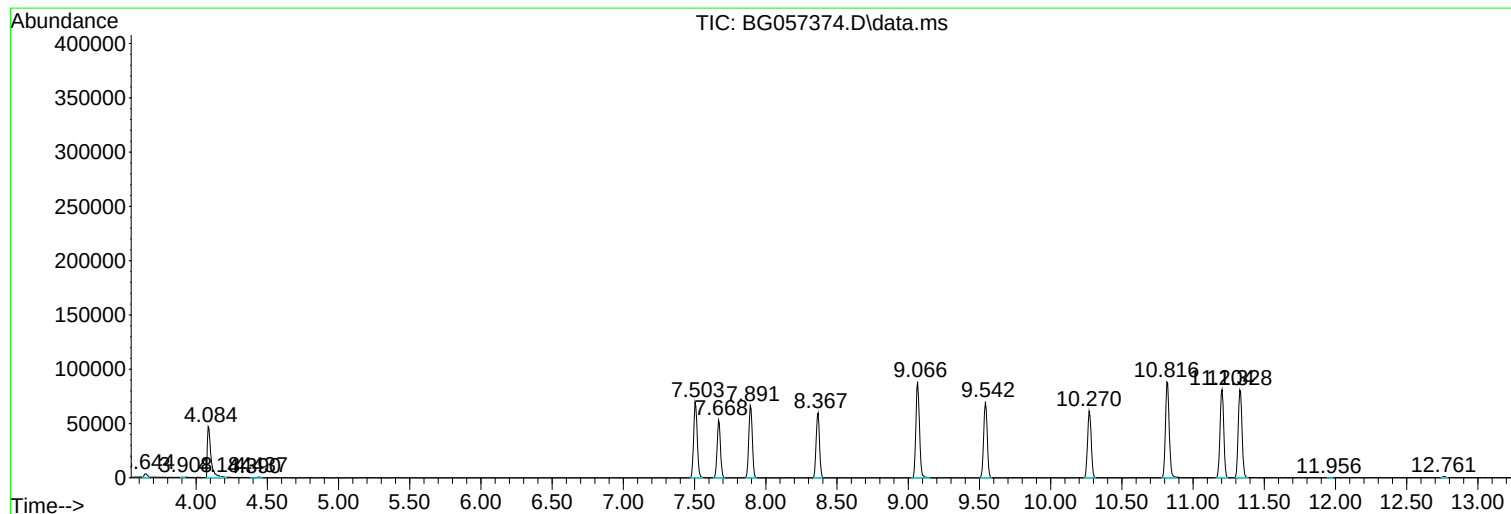

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057374.D
Acq On : 10 May 2023 18:15
Operator : CG/JU
Sample : PB152674BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK674

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051023\
Data File : BG057374.D
Acq On : 10 May 2023 18:15
Operator : CG/JU
Sample : PB152674BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK674

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc