
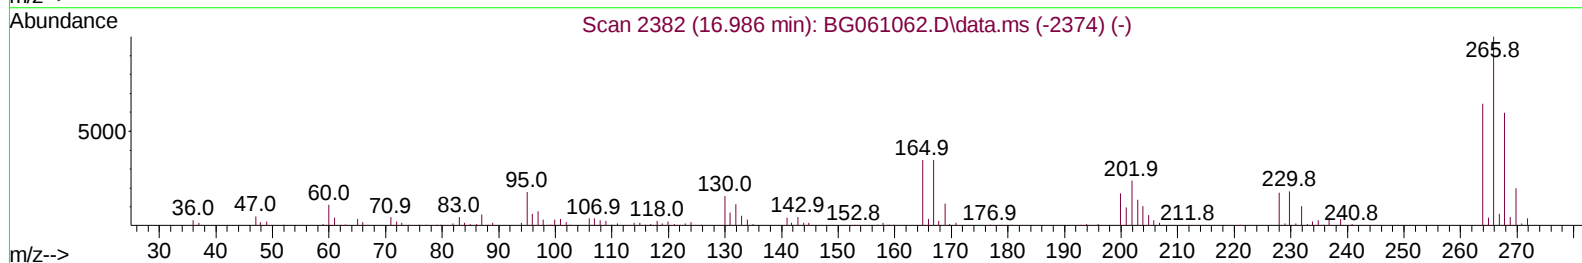
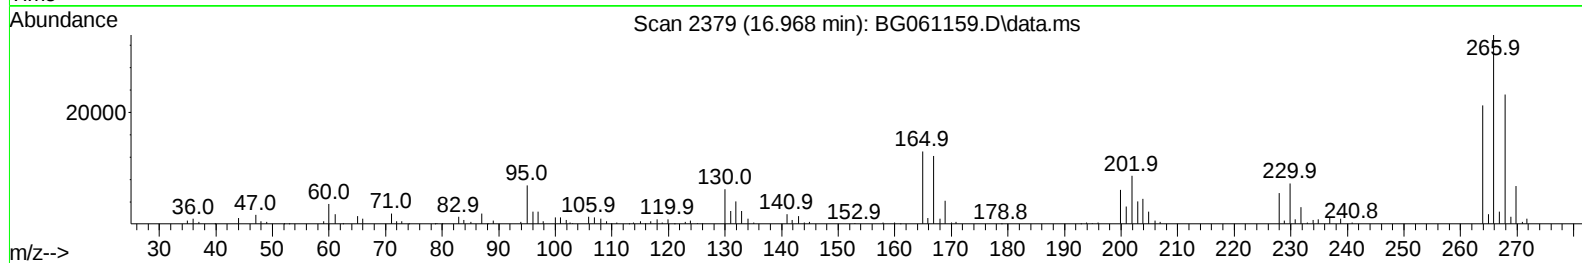


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051024\
Data File : BG061159.D
Acq On : 10 May 2024 11:06
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 13:01:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

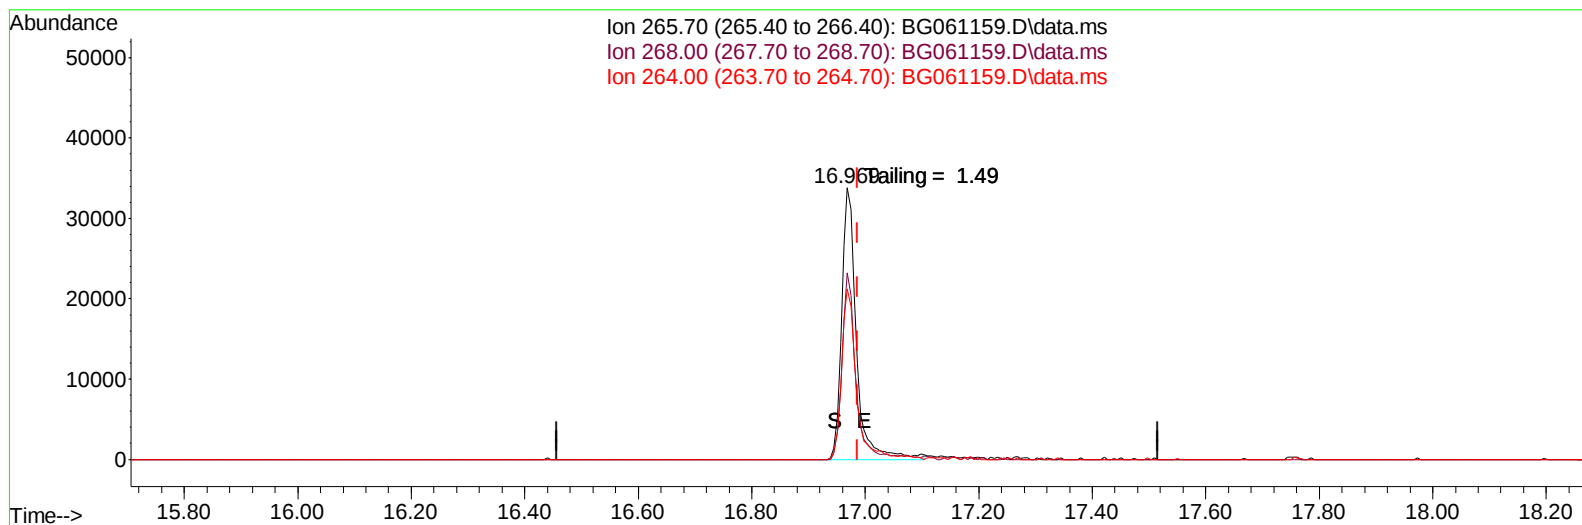




TIC: BG061159.D\data.ms

(70) Pentachlorophenol (C)**16.968min (-0.018) 14669.05 ng****response 59857**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	68.72
264.00	64.40	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051024\
Data File : BG061159.D
Acq On : 10 May 2024 11:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 13:01:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

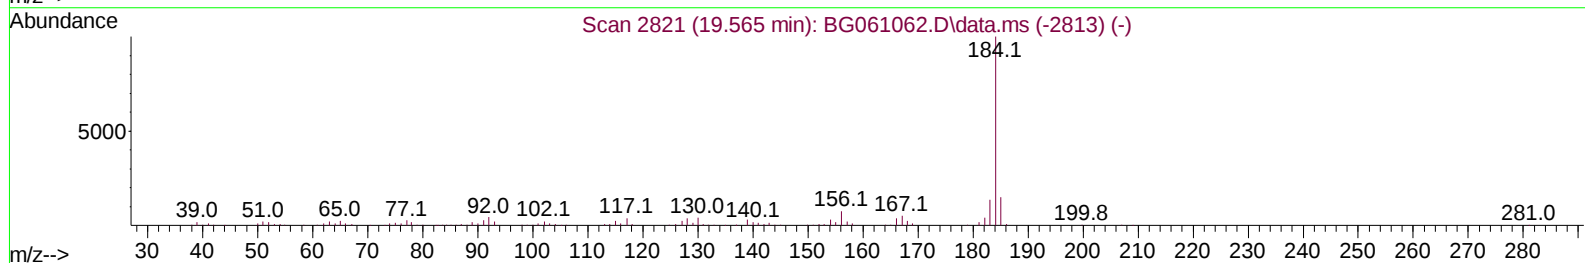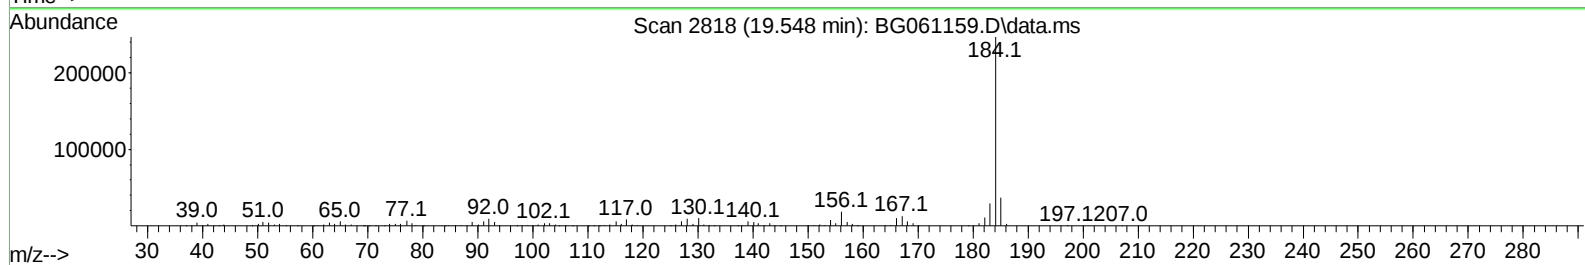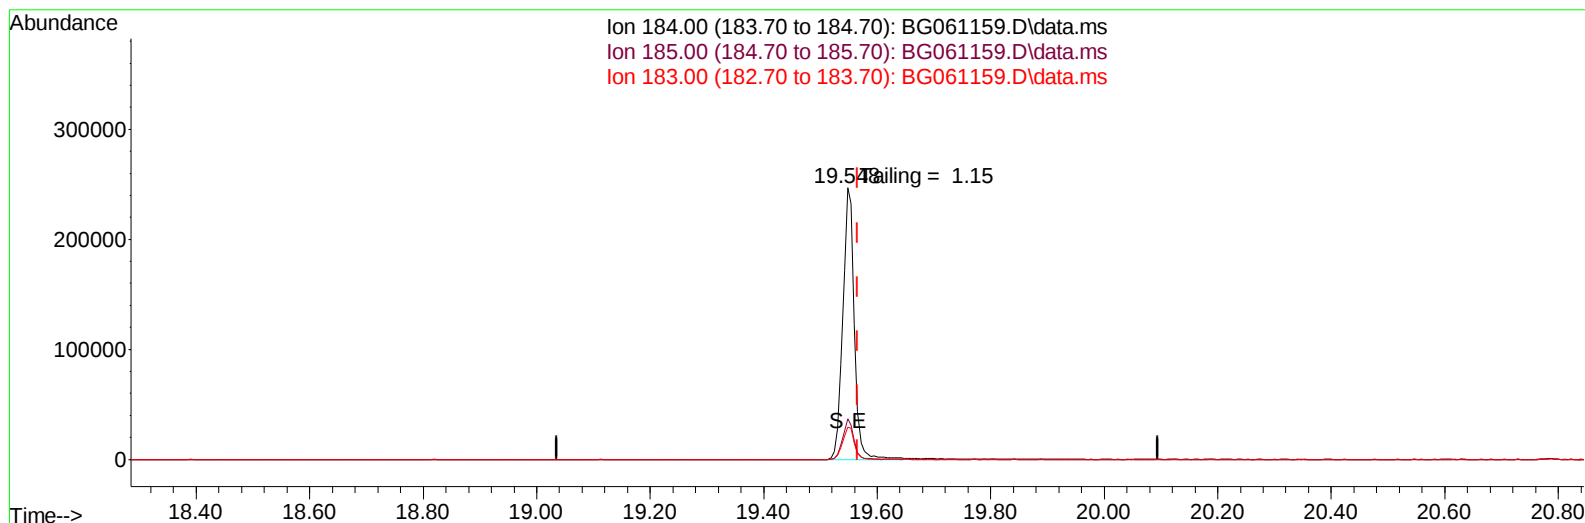

TIC: BG061159.D\data.ms

(77) Benzidine**19.548min (-0.017) 231168.22 ng****response 350318**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.98
183.00	13.60	11.85
0.00	0.00	0.00