


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051115\
 Data File : BG017065.D
 Acq On : 11 May 2015 23:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 12 04:00:00 2015

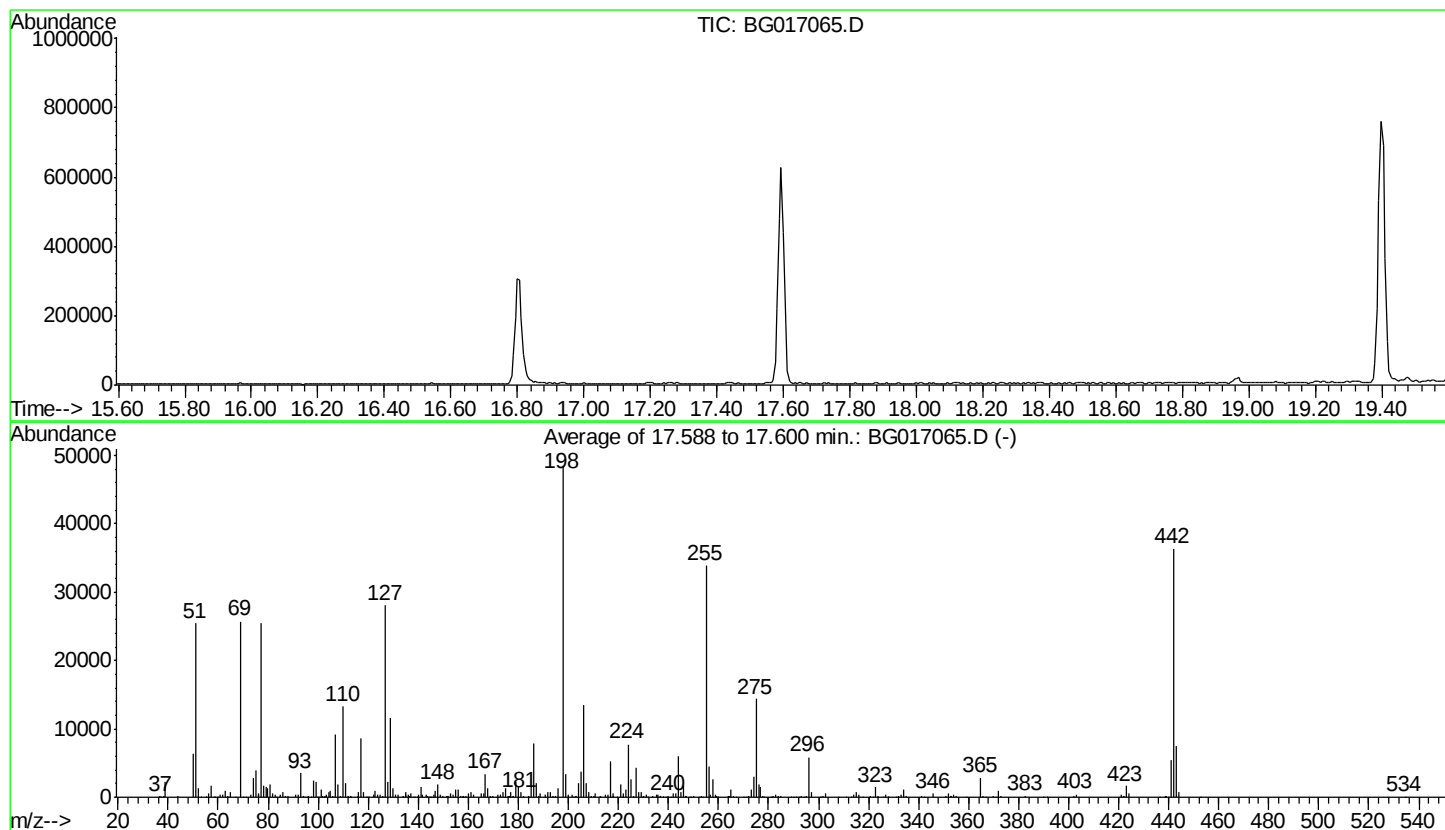

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	25430	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.0	25683	PASS
70	69	0.00	2	0.2	64	PASS
127	198	10	80	57.7	27997	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48496	PASS
199	198	5	9	6.8	3290	PASS
275	198	10	60	29.6	14377	PASS
365	198	1	100	5.8	2824	PASS
441	442	0.01	24	14.9	5401	PASS
442	198	50	100	75.0	36360	PASS
443	442	15	24	20.8	7581	PASS