
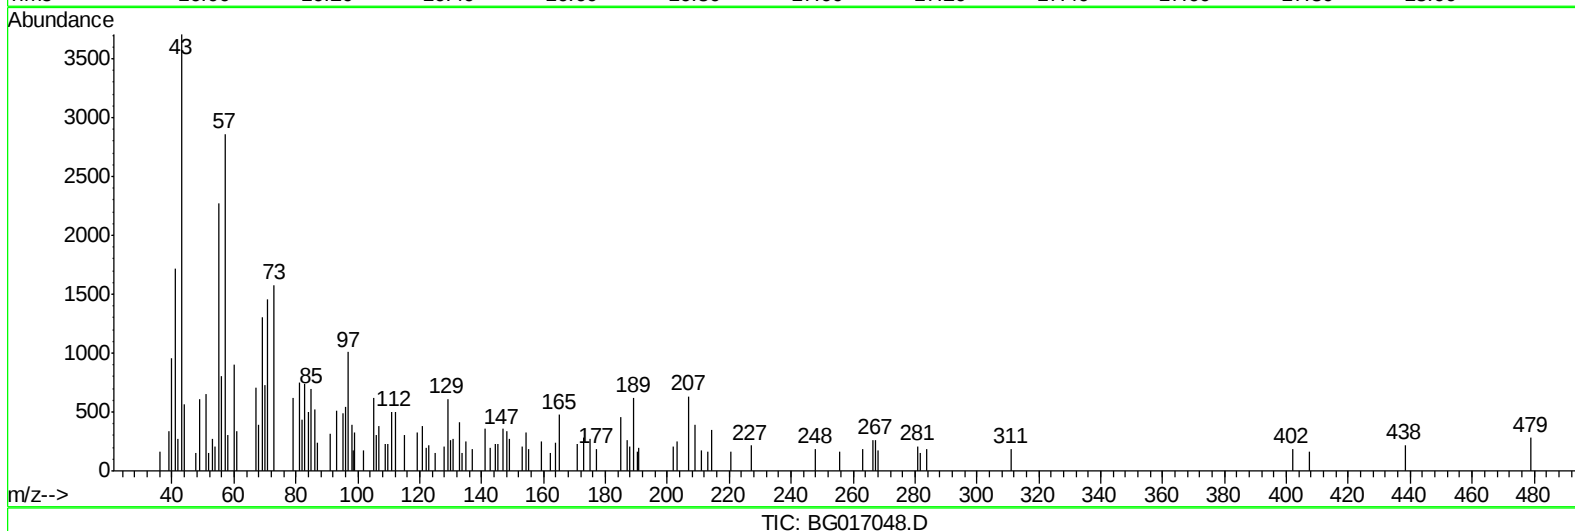


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051115\
Data File : BG017048.D
Acq On : 11 May 2015 11:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:38:53 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 04:56:17 2015
Response via : Initial Calibration

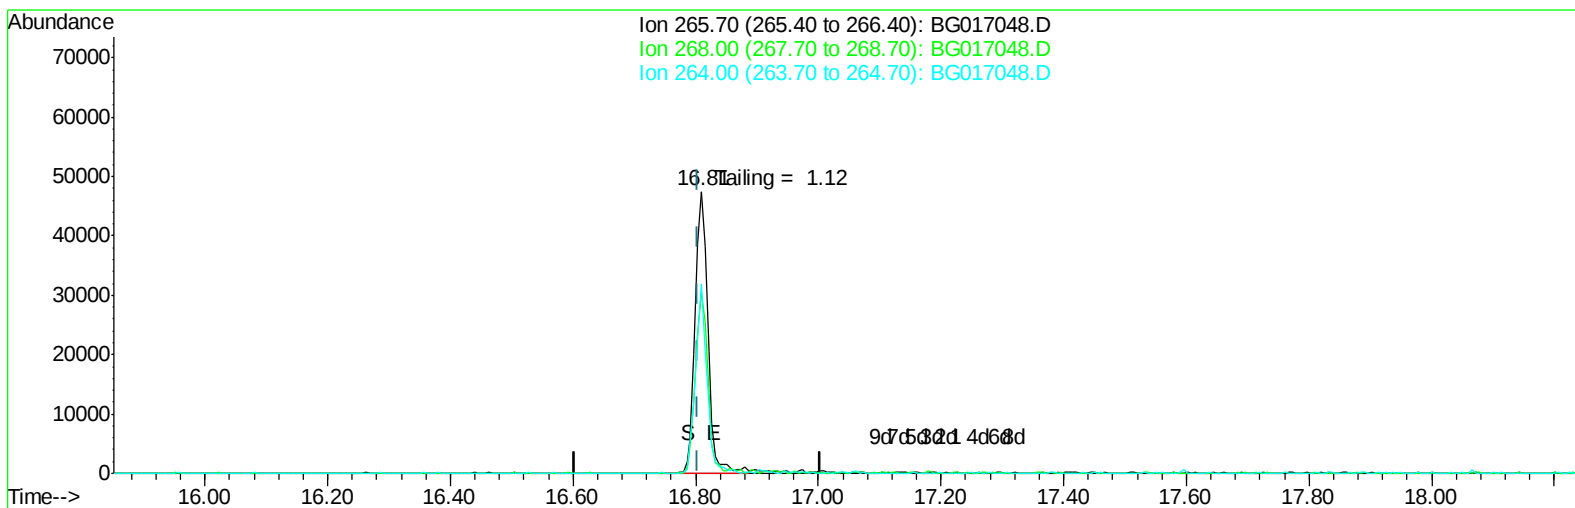

TIC: BG017048.D

(69) Pentachlorophenol (C)



17.226min (+0.422) 35.11ng

response 90

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	67.58
264.00	64.20	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051115\
Data File : BG017048.D
Acq On : 11 May 2015 11:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:38:53 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 04:56:17 2015
Response via : Initial Calibration

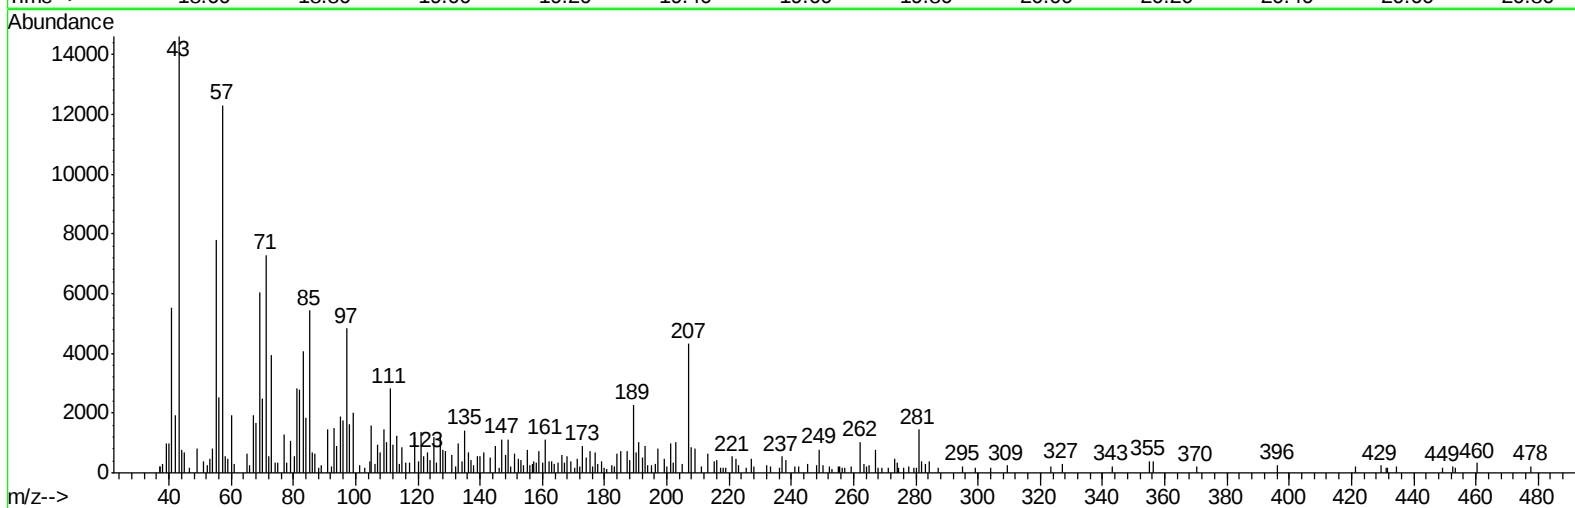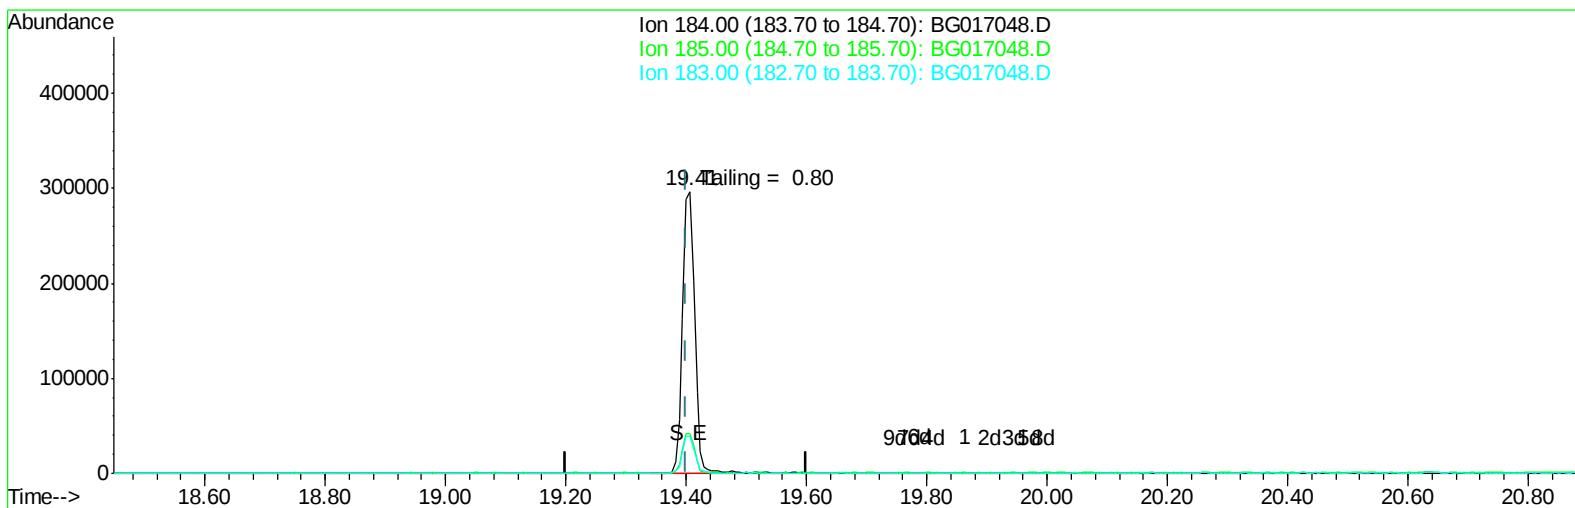

TIC: BG017048.D

(76) Benzidine

19.864min (+0.463) 195.49ng

response 1003

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	109.53#
183.00	13.20	34.04#
0.00	0.00	0.00