
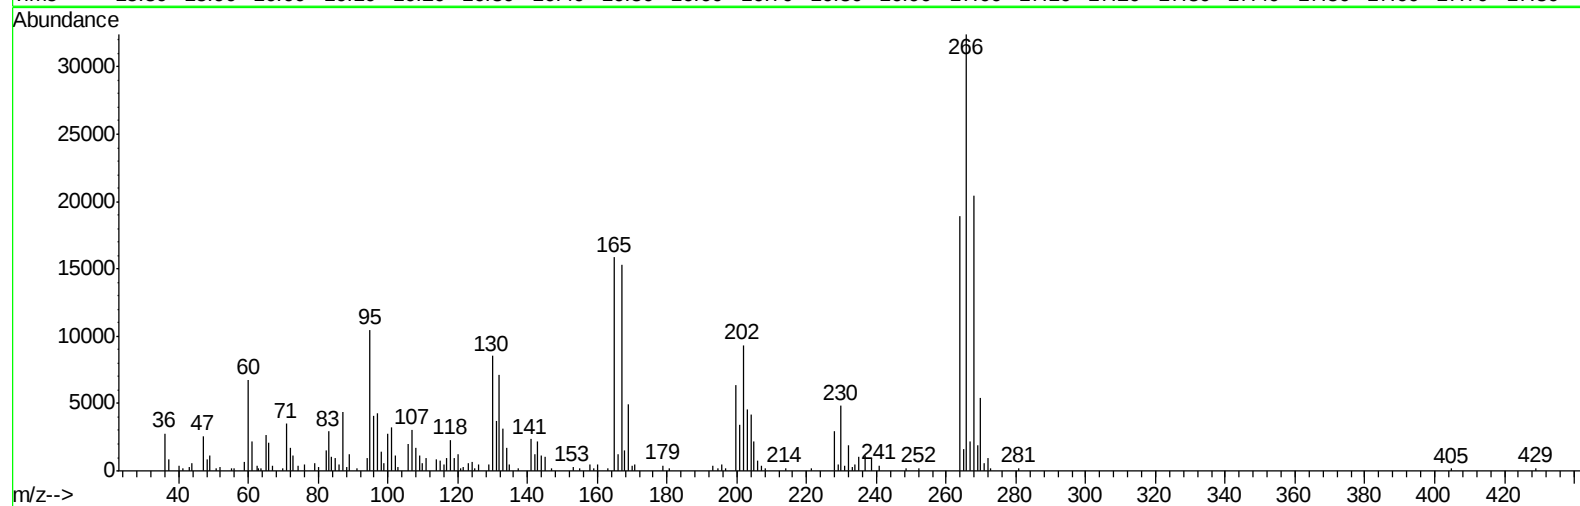


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051115\
Data File : BG017065.D
Acq On : 11 May 2015 23:50
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:40:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 04:56:17 2015
Response via : Initial Calibration

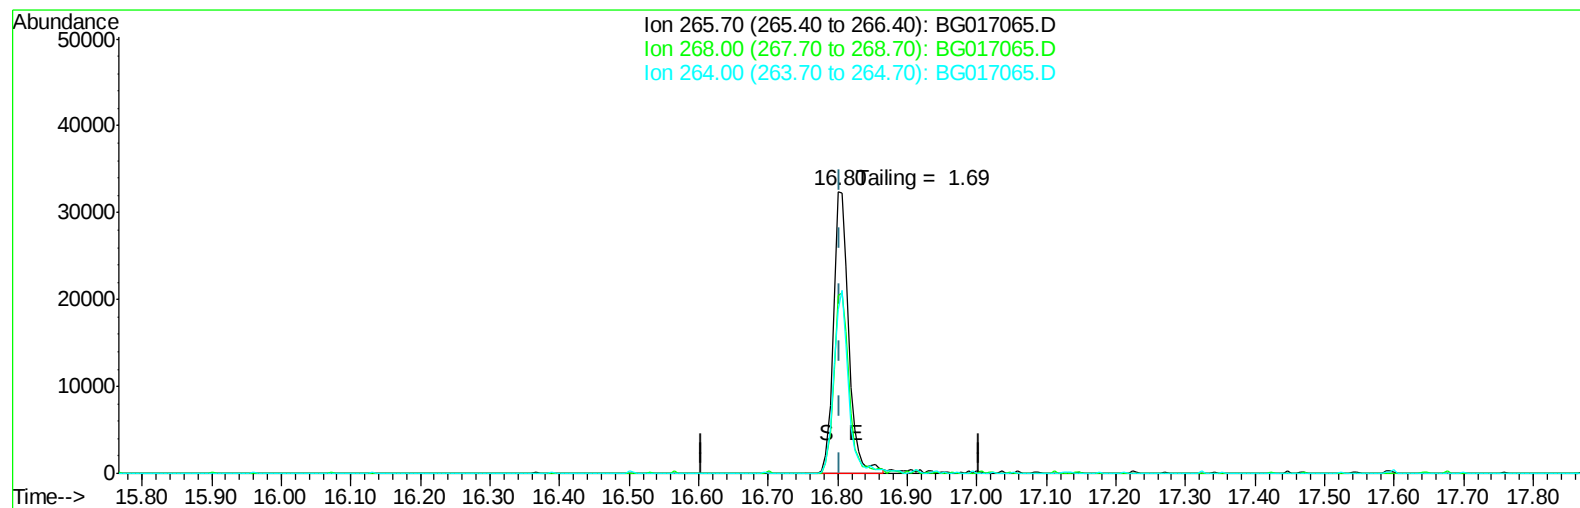

TIC: BG017065.D

(69) Pentachlorophenol (C)



16.801min (-0.003) 0.00ng

response 49899

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	63.19
264.00	64.20	58.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051115\
Data File : BG017065.D
Acq On : 11 May 2015 23:50
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:40:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 12 04:56:17 2015
Response via : Initial Calibration

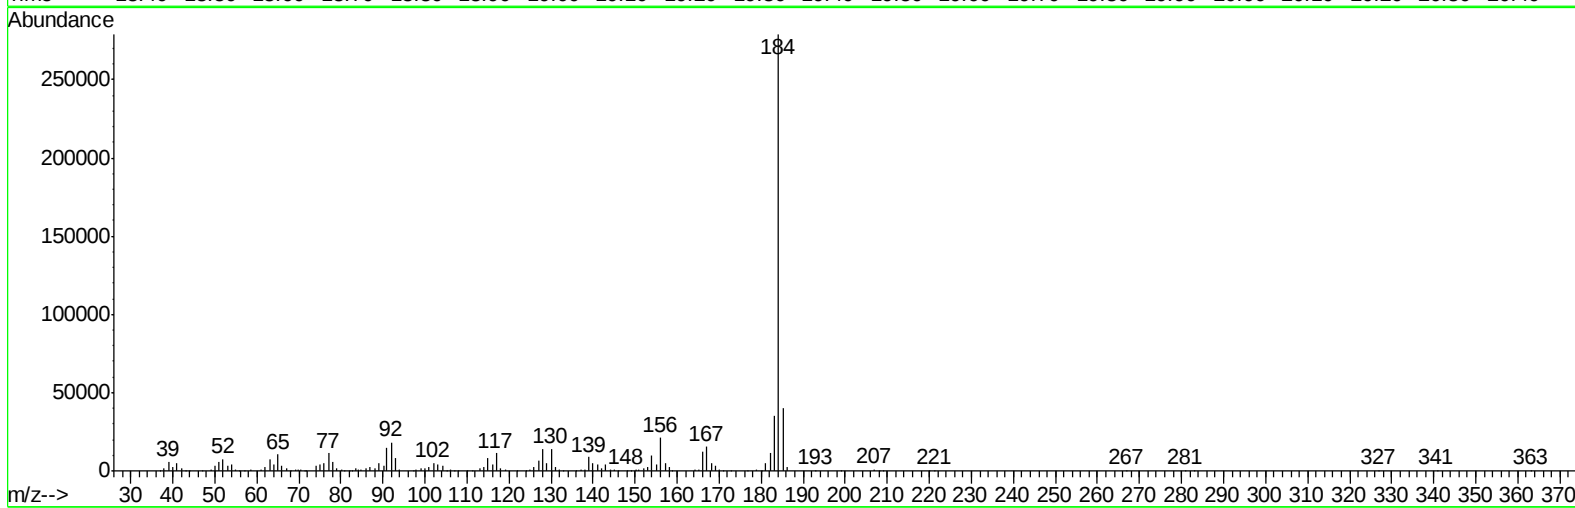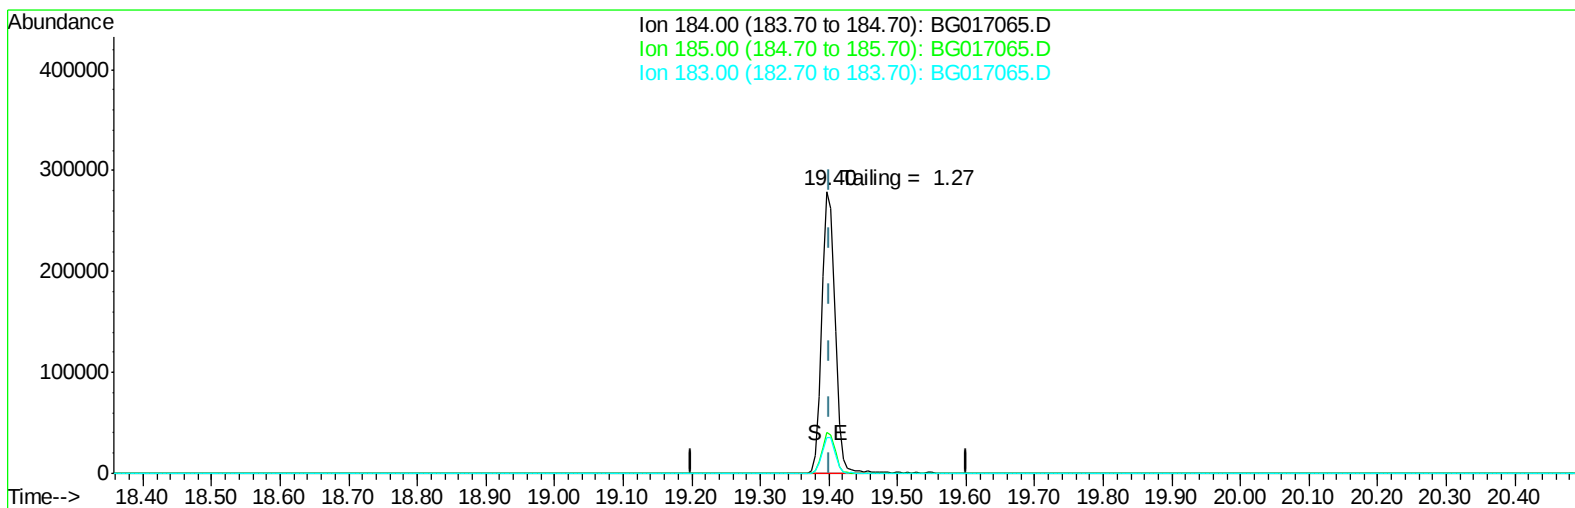

TIC: BG017065.D

(76) Benzidine

19.398min (-0.003) 24391.23ng

response 372951

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.37
183.00	13.20	12.70
0.00	0.00	0.00