

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051116\
 Data File : BG021858.D
 Acq On : 12 May 2016 00:21
 Operator : UM/SJ
 Sample : H2936-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9WF4

Quant Time: May 12 07:34:15 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 07:33:29 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	69941	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	340649	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	202699	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	429600	20.00	ng/ul	0.00
76) Chrysene-d12	21.84	240	415325	20.00	ng/ul	0.00
84) Perylene-d12	25.19	264	421284	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.57	96	4728	3.26	ng/uL	0.00
5) Phenol-d5	7.33	99	82453	15.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.50	67	46423	18.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	83818	20.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	53227	12.21	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	42502	18.98	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	46706	33.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	77916	19.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.33	131	434	0.10	ng/ul	0.20
44) Dimethylphthalate-d6	14.20	166	277947	19.52	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	375212	18.56	ng/ul	0.00
52) 4-Nitrophenol-d4	15.01	143	13927	5.71	ng/ul	0.00
58) Fluorene-d10	15.79	176	261506	17.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	28951	24.33	ng/ul	0.00
71) Anthracene-d10	17.65	188	364636	17.44	ng/ul	0.00
77) Pyrene-d10	19.92	212	376765	19.38	ng/ul	0.00
88) Benzo(a)pyrene-d12	24.95	264	358144	17.89	ng/ul	0.01

Target Compounds


					Ovalue	
4) Benzaldehyde	7.71	77	791	1.40	ng/ul	91
14) Acetophenone	9.02	105	8719	1.21	ng/ul#	70
28) Naphthalene	11.06	128	17698	1.04	ng/ul	95
34) 2-Methylnaphthalene	12.64	142	16279	1.29	ng/ul	94
35) 1-Methylnaphthalene	12.86	142	15623	1.25	ng/ul#	93
45) Dimethylphthalate	14.25	163	58358	4.02	ng/ul	97
70) Phenanthrene	17.59	178	188943	8.04	ng/ul	98
75) Fluoranthene	19.59	202	263826	9.89	ng/ul	96
79) Butylbenzylphthalate	20.82	149	7047	1.33	ng/ul	92
81) Benzo(a)anthracene	21.82	228	123322	5.34	ng/ul	97
82) Bis(2-ethylhexyl)phthalate	21.70	149	45537	5.25	ng/ul#	99
83) Chrysene	21.89	228	134902	5.90	ng/ul	96
86) Benzo(b)fluoranthene	24.12	252	195673	8.11	ng/ul#	95
87) Benzo(k)fluoranthene	24.12	252	195673	7.58	ng/ul#	95
89) Benzo(a)pyrene	25.03	252	120402	5.02	ng/ul#	94
90) Indeno(1,2,3-cd)pyrene	29.01	276	90761	3.19	ng/ul#	92
92) Benzo(g,h,i)perylene	30.21	276	42091	1.79	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051116\
Data File : BG021858.D
Acq On : 12 May 2016 00:21
Operator : UM/SJ
Sample : H2936-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9WF4

Quant Time: May 12 07:34:15 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 07:33:29 2016
Response via : Initial Calibration

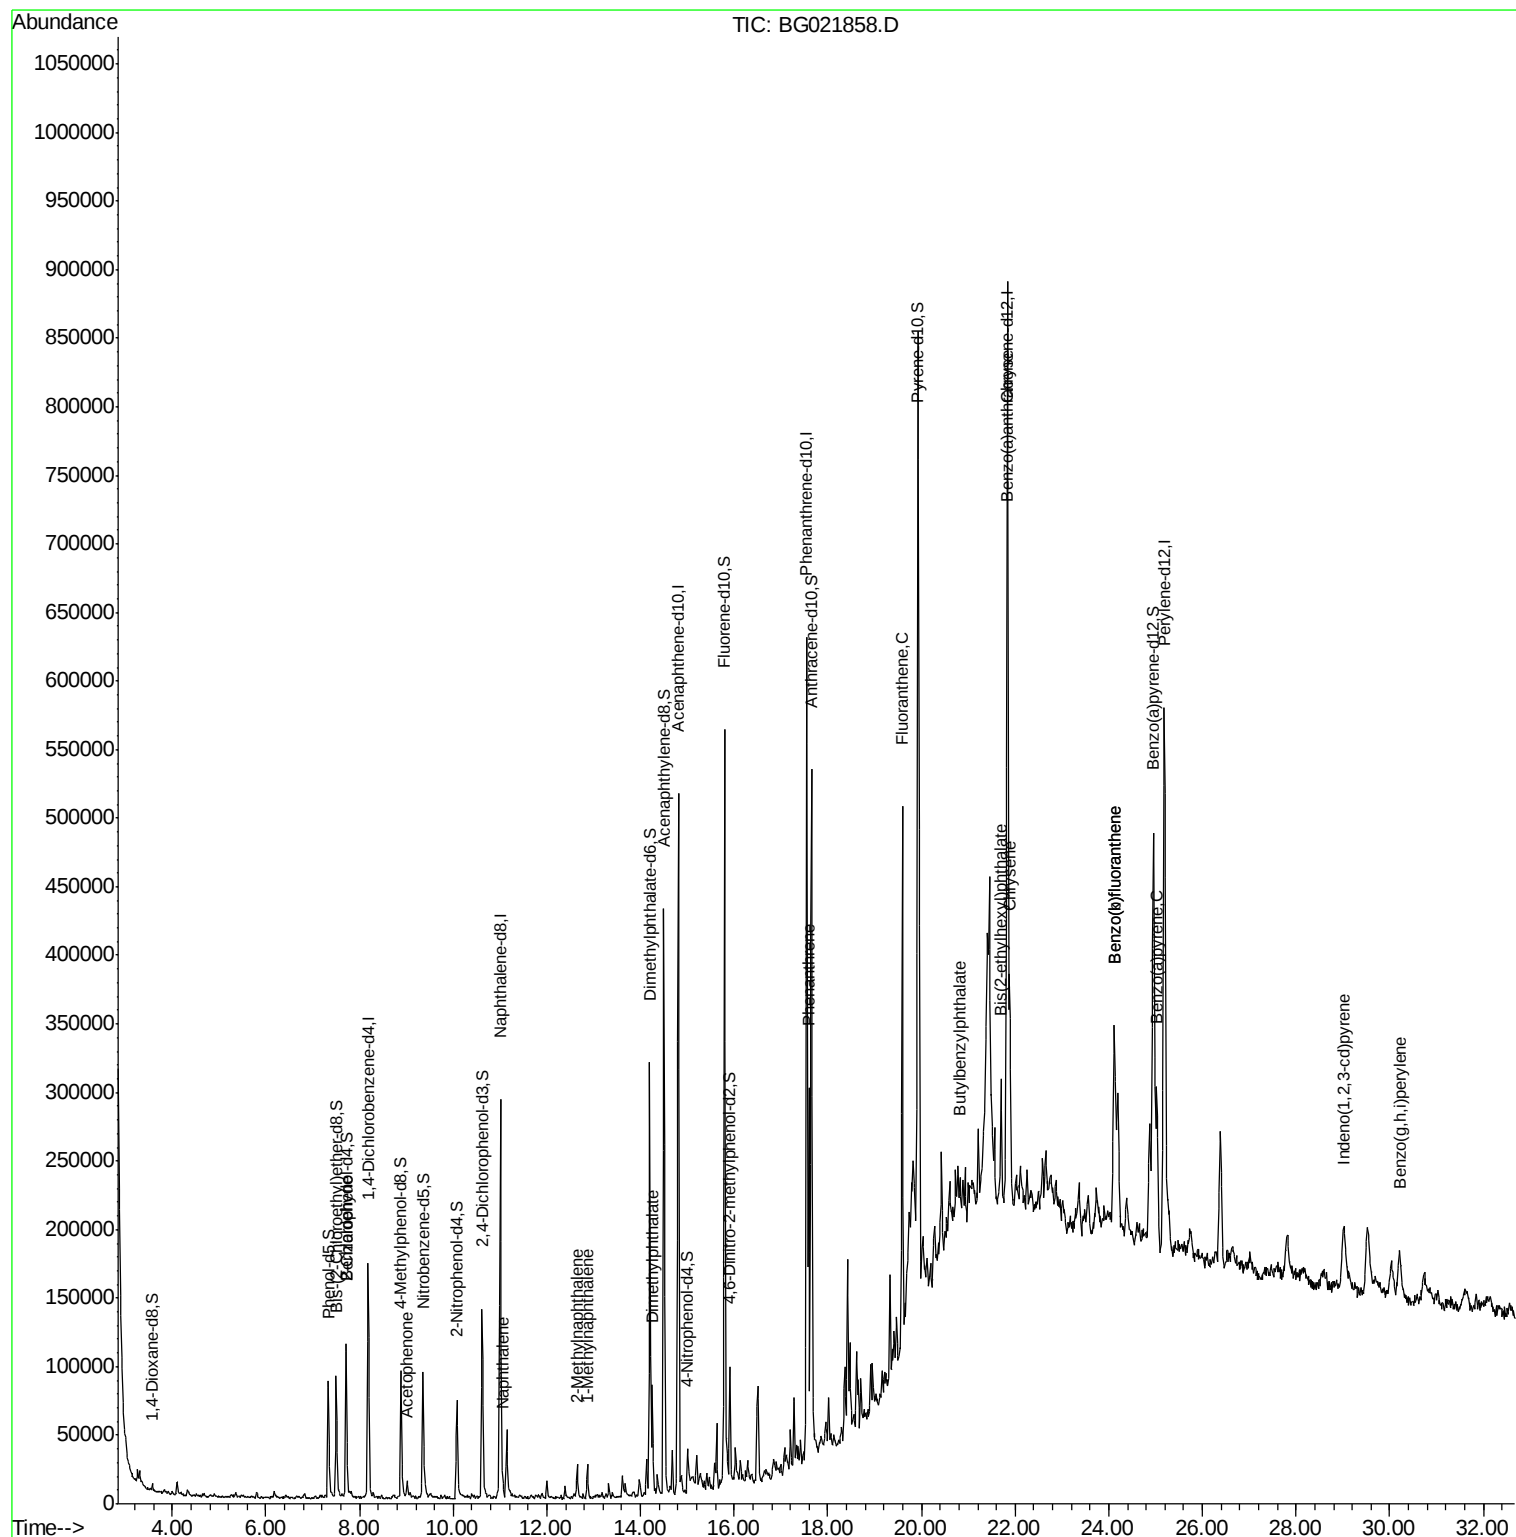

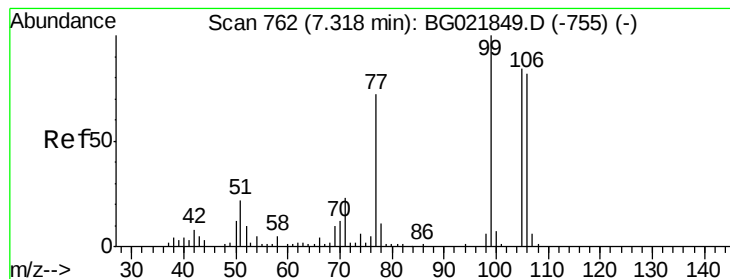

#4

Benzaldehyde

Concen: 1.40 ng/ul

RT: 7.71 min Scan# 829

Delta R.T. 0.39 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleID :

D9WF4


Tot Ion: 77 Resp: 791

Ion Ratio Lower Upper

77 100

105 75.3 68.5 102.7

106 86.5 65.0 97.4

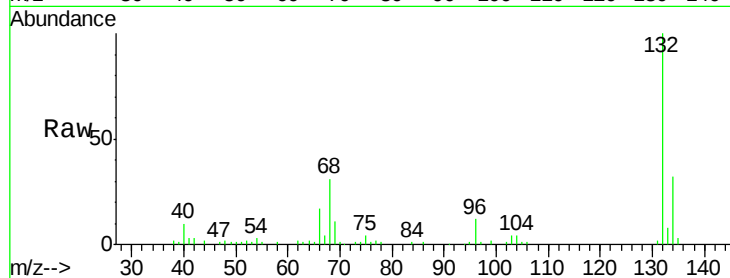

Abundance Ion 77.00 (76.70 to 77.70): BGC

Ion 105.00 (104.70 to 105.70): BGC

Ion 106.00 (105.70 to 106.70): BGC

7.71

600

400

200



0

7.68

7.70

7.72

Time-->

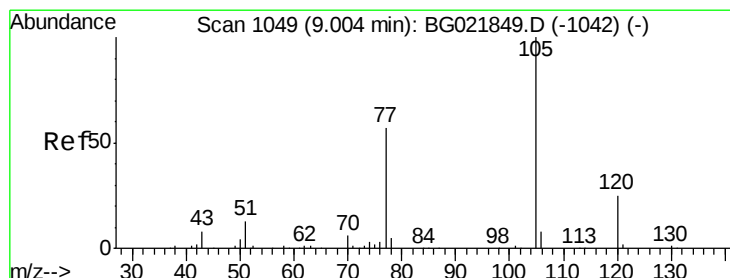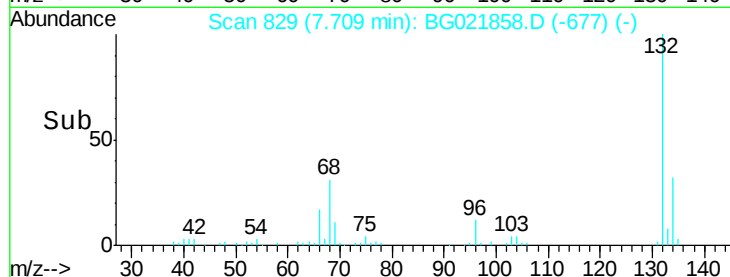

#14

Acetophenone

Concen: 1.21 ng/ul

RT: 9.02 min Scan# 1052

Delta R.T. 0.01 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21


Tgt Ion: 105 Resp: 8719

Ion Ratio Lower Upper

105 100

77 68.3 76.3 114.5#

51 14.5 27.6 41.4#

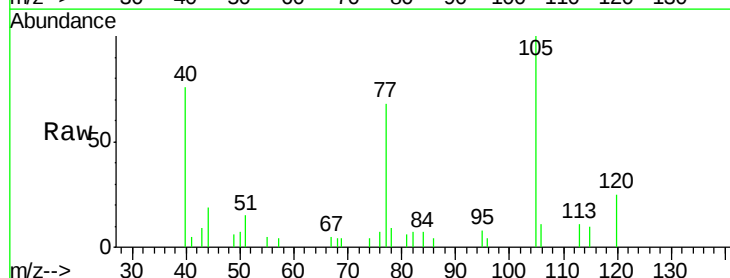

Abundance Ion 105.00 (104.70 to 105.70): BGC

Ion 77.00 (76.70 to 77.70): BGC

Ion 51.00 (50.70 to 51.70): BGC

9.02

5000

4000

3000

2000

1000


0


8.95

9.00

9.05

Time-->

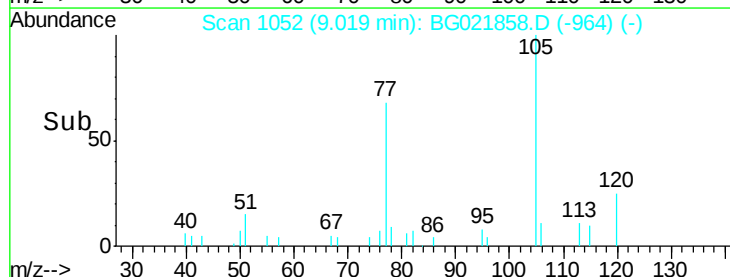

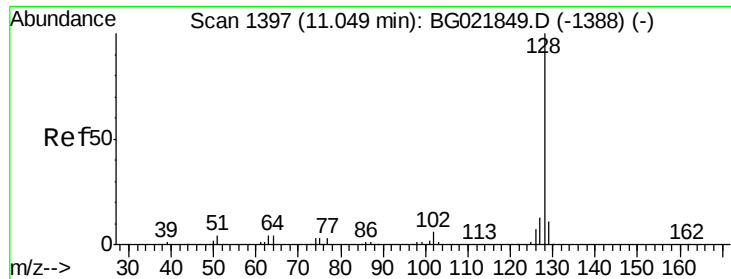

#28

Naphthalene

Concen: 1.04 ng/ul

RT: 11.06 min Scan# 1399

Delta R.T. 0.01 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleId :

D9WF4


Tot Ion:128 Resp: 17698

Ion Ratio Lower Upper

128 100

129 12.2 8.3 12.5




127 15.4 10.8 16.2

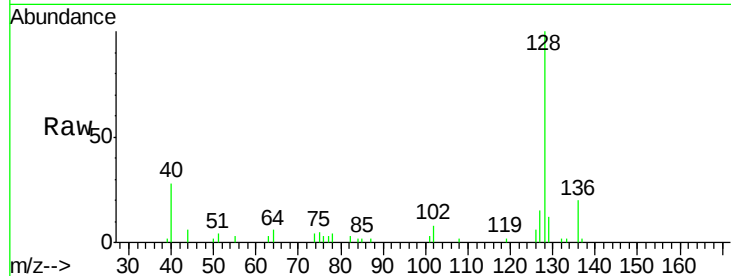

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

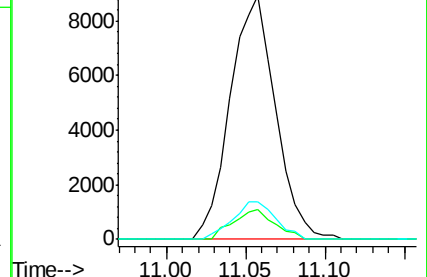

#34

2-Methylnaphthalene

Concen: 1.29 ng/ul

RT: 12.64 min Scan# 1669

Delta R.T. 0.00 min

Lab File: BG021858.D


Acq: 12 May 2016 00:21

Tgt Ion:142 Resp: 16279

Ion Ratio Lower Upper



142 100


141 94.7 71.3 106.9



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

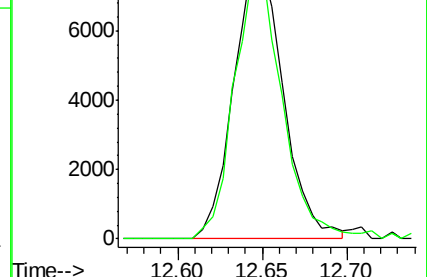







#35
 1-Methyl-naphthalene
 Concen: 1.25 ng/ul
 RT: 12.86 min Scan# 1706
 Delta R.T. 0.00 min
 Lab File: BG021858.D
 Acq: 12 May 2016 00:21

Instrument :
 BNA_G
 ClientSampleID :
 D9WF4

Tot Ion:142 Resp: 15623
 Ion Ratio Lower Upper
 142 100
 141 89.6 77.0 115.4
 116 2.7 4.2 6.4#




Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 116.00 (115.70 to 116.70): E


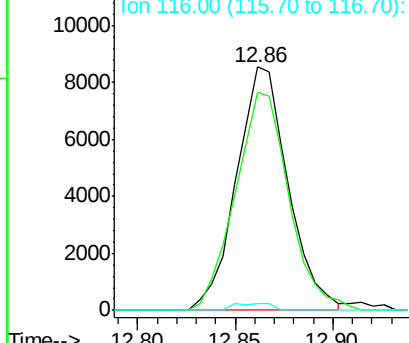



#45
 Dimethylphthalate
 Concen: 4.02 ng/ul
 RT: 14.25 min Scan# 1942
 Delta R.T. 0.00 min
 Lab File: BG021858.D
 Acq: 12 May 2016 00:21

Tgt Ion:163 Resp: 58358
 Ion Ratio Lower Upper
 163 100
 194 4.7 3.9 5.9
 164 9.6 8.7 13.1



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

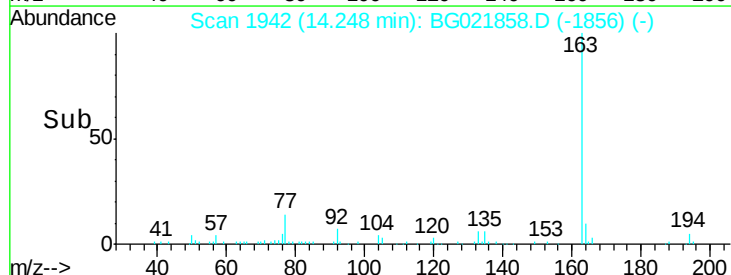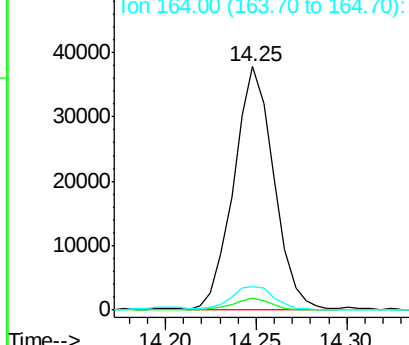

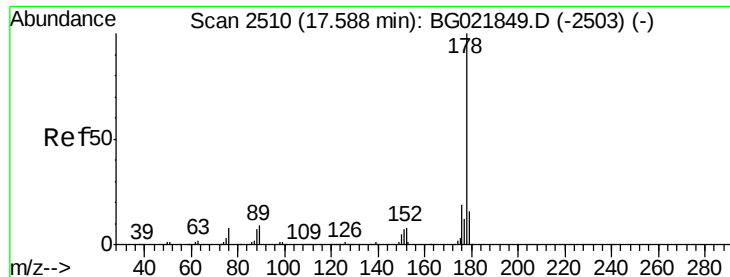

#70

Phenanthrene

Concen: 8.04 ng/ul

RT: 17.59 min Scan# 2511

Delta R.T. 0.00 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleId :

D9WF4


Tot Ion:178 Resp: 188943

Ion Ratio Lower Upper

178 100

179 15.8 11.8 17.8




176 19.4 14.8 22.2

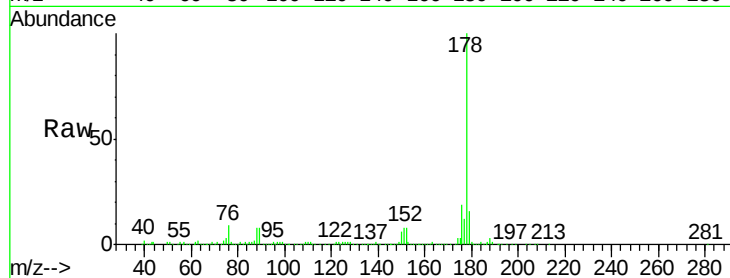

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

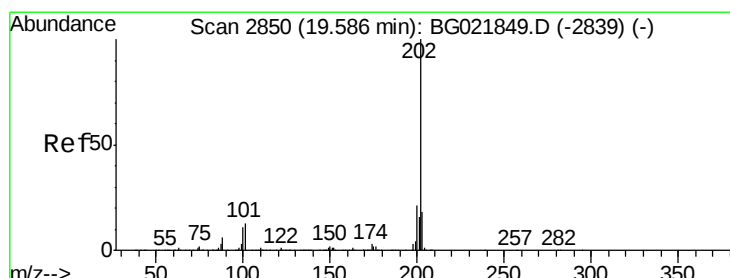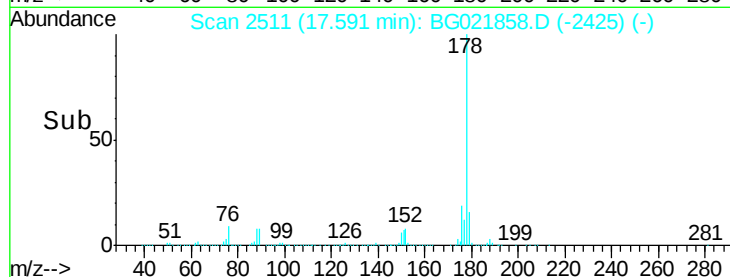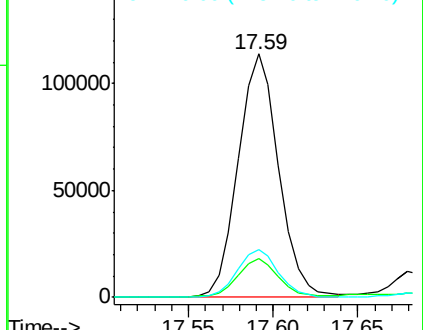

#75

Fluoranthene

Concen: 9.89 ng/ul

RT: 19.59 min Scan# 2851

Delta R.T. 0.00 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21


Tgt Ion:202 Resp: 263826

Ion Ratio Lower Upper

202 100

101 12.6 8.9 13.3



100 10.0 7.0 10.4

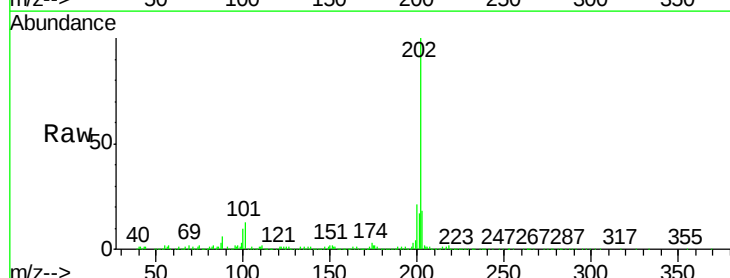


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



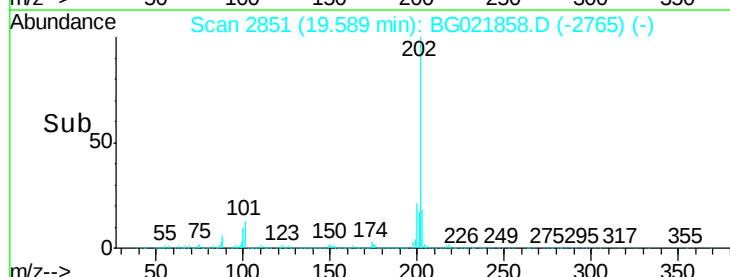
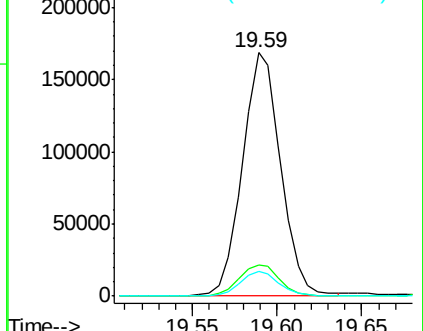


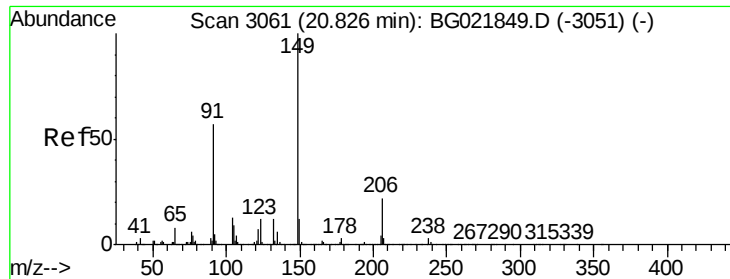

#79
Butylbenzylphthalate
Concen: 1.33 ng/ul
RT: 20.82 min Scan# 3061
Delta R.T. -0.00 min
Lab File: BG021858.D
Acq: 12 May 2016 00:21




Instrument :
BNA_G
ClientSampleId :
D9WF4


Tot Ion:149 Resp: 7047
Ion Ratio Lower Upper
149 100
91 74.7 65.8 98.8
206 21.1 15.5 23.3

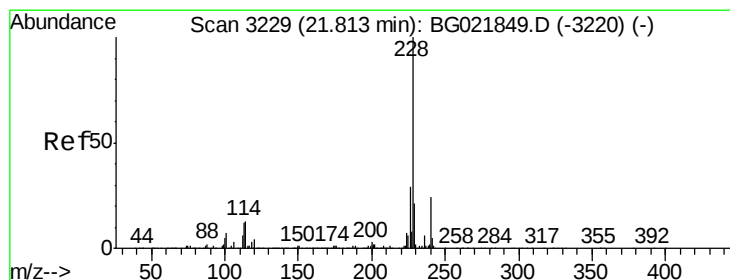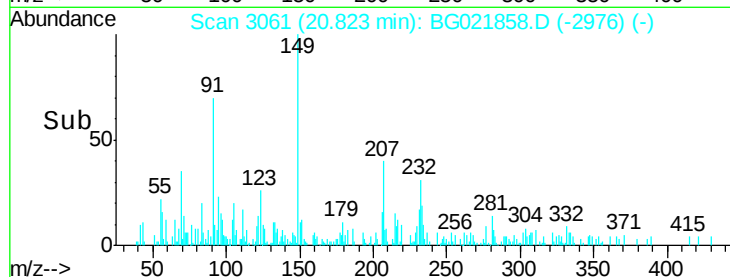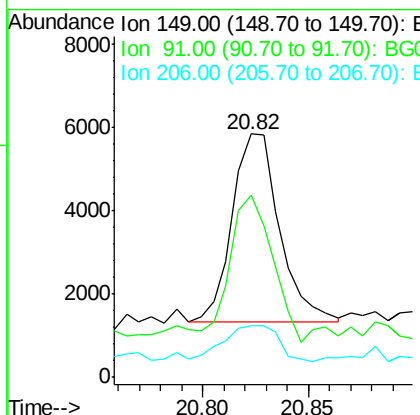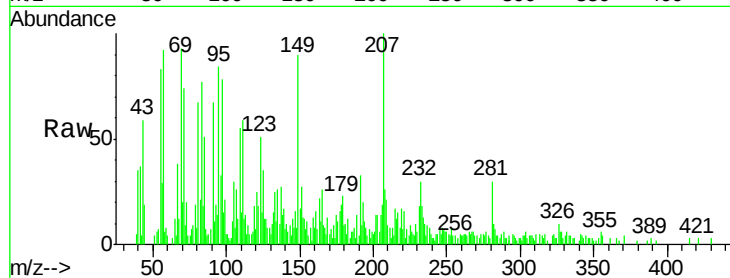

#81
Benzo(a)anthracene
Concen: 5.34 ng/ul
RT: 21.82 min Scan# 3230
Delta R.T. 0.00 min
Lab File: BG021858.D
Acq: 12 May 2016 00:21

Tgt Ion:228 Resp: 123322
Ion Ratio Lower Upper
228 100
229 21.1 16.6 25.0
226 29.1 21.0 31.4

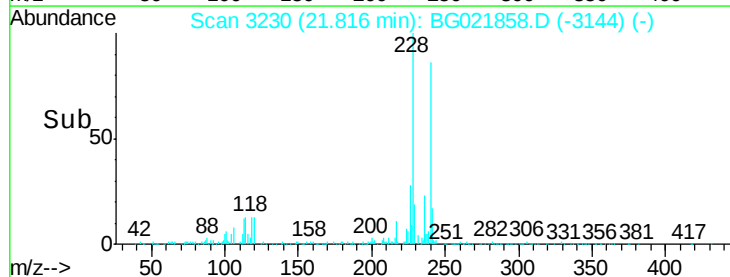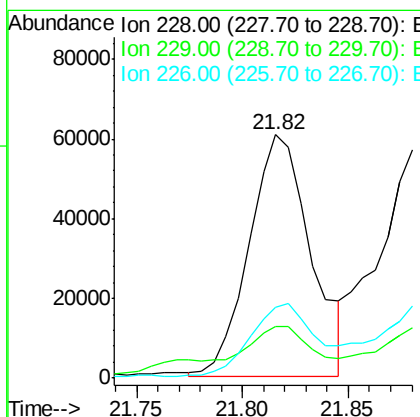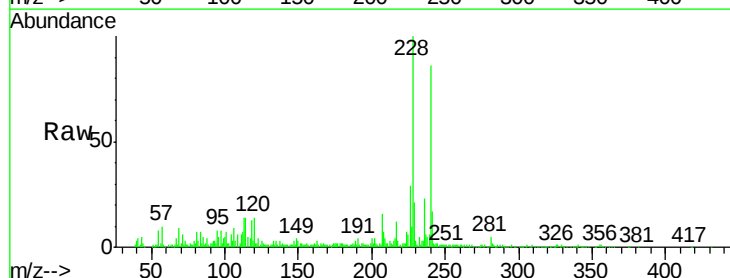

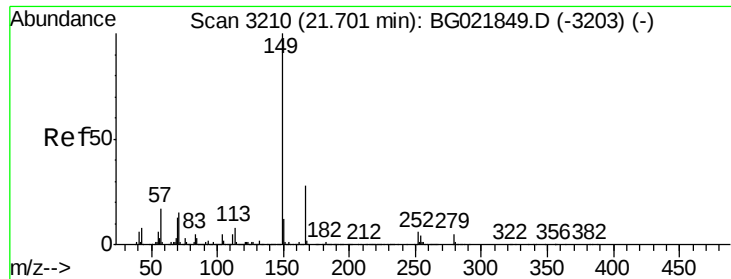

#82

Bis(2-ethylhexyl)phthalate

Concen: 5.25 ng/ul

RT: 21.70 min Scan# 3211

Delta R.T. 0.00 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleId :

D9WF4


Tot Ion:149 Resp: 45537

Ion Ratio Lower Upper

149 100

167 25.2 20.5 30.7




279 6.0 3.7 5.5#

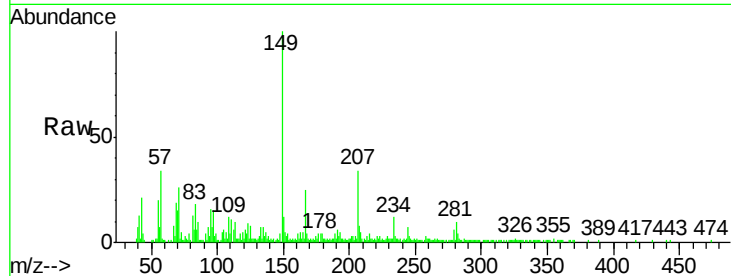

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

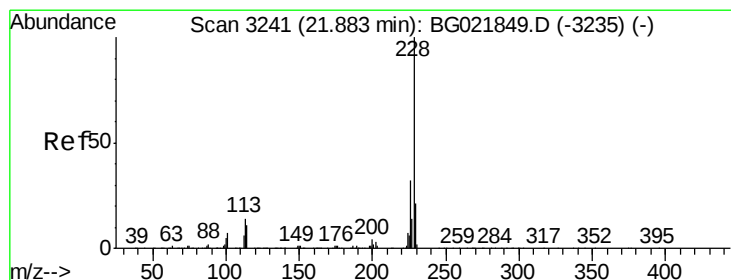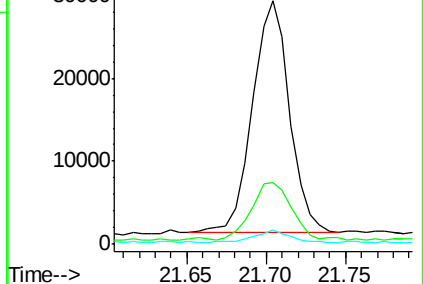

#83

Chrysene

Concen: 5.90 ng/ul

RT: 21.89 min Scan# 3242

Delta R.T. 0.00 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21


Tgt Ion:228 Resp: 134902

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.2



229 22.9 16.2 24.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




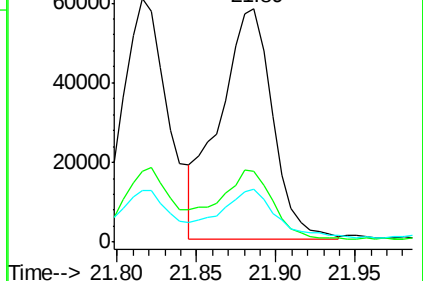


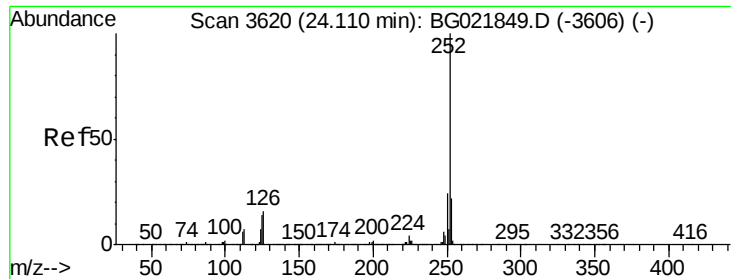

#86
Benzo(b)fluoranthene
Concen: 8.11 ng/ul
RT: 24.12 min Scan# 3623
Delta R.T. 0.01 min
Lab File: BG021858.D
Acq: 12 May 2016 00:21




Instrument :
BNA_G
ClientSampleId :
D9WF4


Tot Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.1	27.1
125	15.5	7.6	11.4

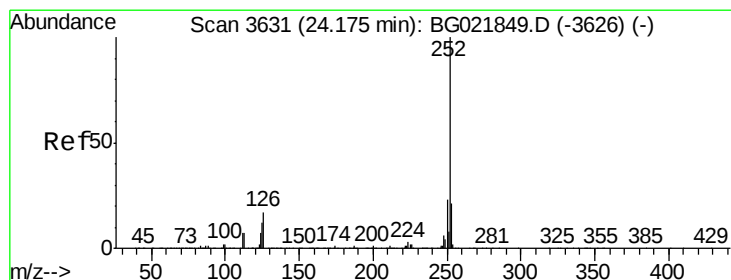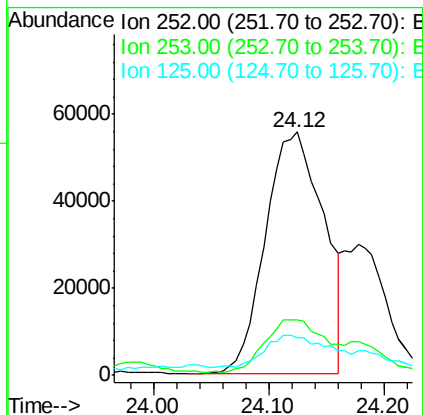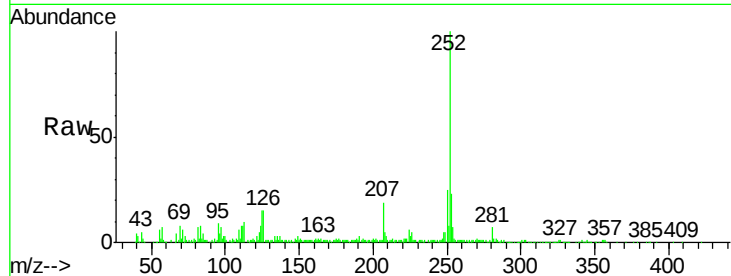

#87
Benzo(k)fluoranthene
Concen: 7.58 ng/ul
RT: 24.12 min Scan# 3623
Delta R.T. -0.05 min
Lab File: BG021858.D
Acq: 12 May 2016 00:21

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.8	26.8
125	15.5	7.7	11.5

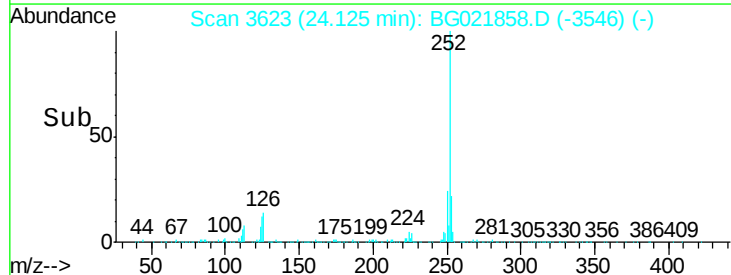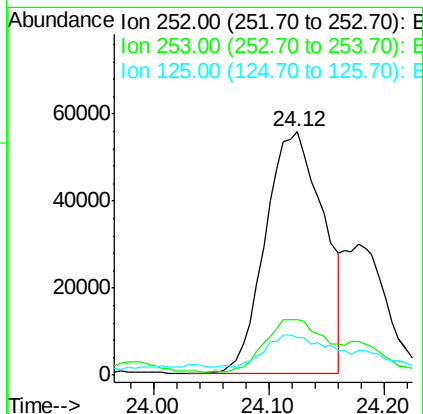



#89

Benzo(a)pyrene

Concen: 5.02 ng/ul

RT: 25.03 min Scan# 3777

Delta R.T. 0.01 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleId :

D9WF4





Tot Ion:252 Resp: 120402

Ion Ratio Lower Upper

252 100

253 22.7 17.4 26.0

125 16.1 8.2 12.2#

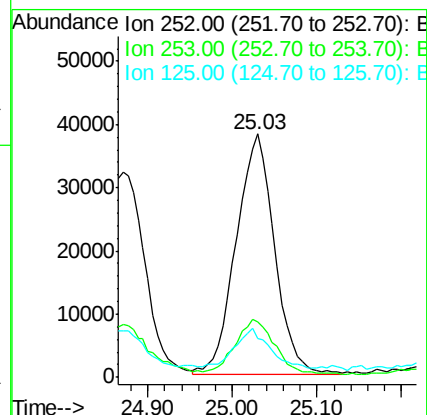

#90

Indeno(1,2,3-cd)pyrene

Concen: 3.19 ng/ul

RT: 29.01 min Scan# 4455

Delta R.T. 0.00 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21




Tgt Ion:276 Resp: 90761


Ion Ratio Lower Upper

276 100

138 25.7 15.8 23.6#

277 25.9 19.0 28.6

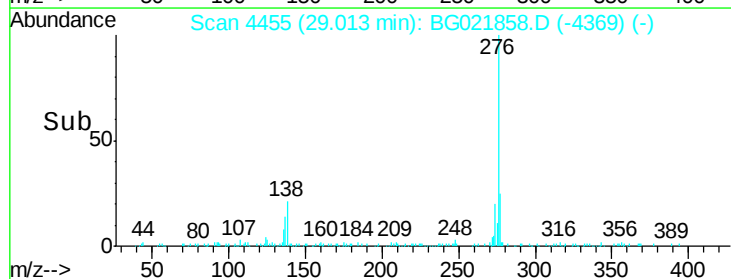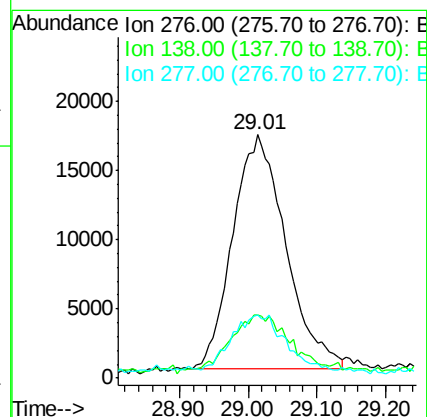



#92

Benzo(a,h,i)perylene

Concen: 1.79 ng/ul

RT: 30.21 min Scan# 4659

Delta R.T. 0.01 min

Lab File: BG021858.D

Acq: 12 May 2016 00:21

Instrument :

BNA_G

ClientSampleId :

D9WF4


Tot Ion: 276 Resp: 42091

Ion Ratio Lower Upper

276 100

138 26.2 13.9 20.9#

277 24.6 19.8 29.6



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

