

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051116\
 Data File : BG021847.D
 Acq On : 11 May 2016 16:59
 Operator : UM/SJ
 Sample : H2937-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9X93

Manual Integrations
 APPROVED

sohil
 5/12/2016 7:30:54 PM

Quant Time: May 12 07:05:06 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 04:46:15 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	65075	20.00	ng/ul	0.00
18) Naphthalene-d8	11.00	136	359237	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.80	164	222140	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	457964	20.00	ng/ul	0.00
76) Chrysene-d12	21.83	240	446376	20.00	ng/ul	0.00
84) Perylene-d12	25.18	264	443898	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.57	96	3443	2.55	ng/uL	0.00
5) Phenol-d5	7.33	99	69348	14.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.50	67	33570	14.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	64175	17.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.89	113	48469	11.95	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	32920	13.94	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	34136	22.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	66519m	15.77	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	71092m	15.64	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	231135	14.81	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	315733	14.25	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	27502m	10.28	ng/ul	0.01
58) Fluorene-d10	15.79	176	211129	12.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	23587	18.59	ng/ul	0.00
71) Anthracene-d10	17.65	188	288634	12.95	ng/ul	0.00
77) Pyrene-d10	19.92	212	306825	14.68	ng/ul	0.00
88) Benzo(a)pyrene-d12	24.95	264	286755	13.60	ng/ul	0.00

Target Compounds

						Ovalue
45) Dimethylphthalate	14.24	163	31971	2.01	ng/ul#	99
82) Bis(2-ethylhexyl)phthalate	21.70	149	11054	1.19	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG051116\
Data File : BG021847.D
Acq On : 11 May 2016 16:59
Operator : UM/SJ
Sample : H2937-15
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
D9X93

Manual Integrations
APPROVED

sohil
5/12/2016 7:30:54 PM

Quant Time: May 12 07:05:06 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 04:46:15 2016
Response via : Initial Calibration

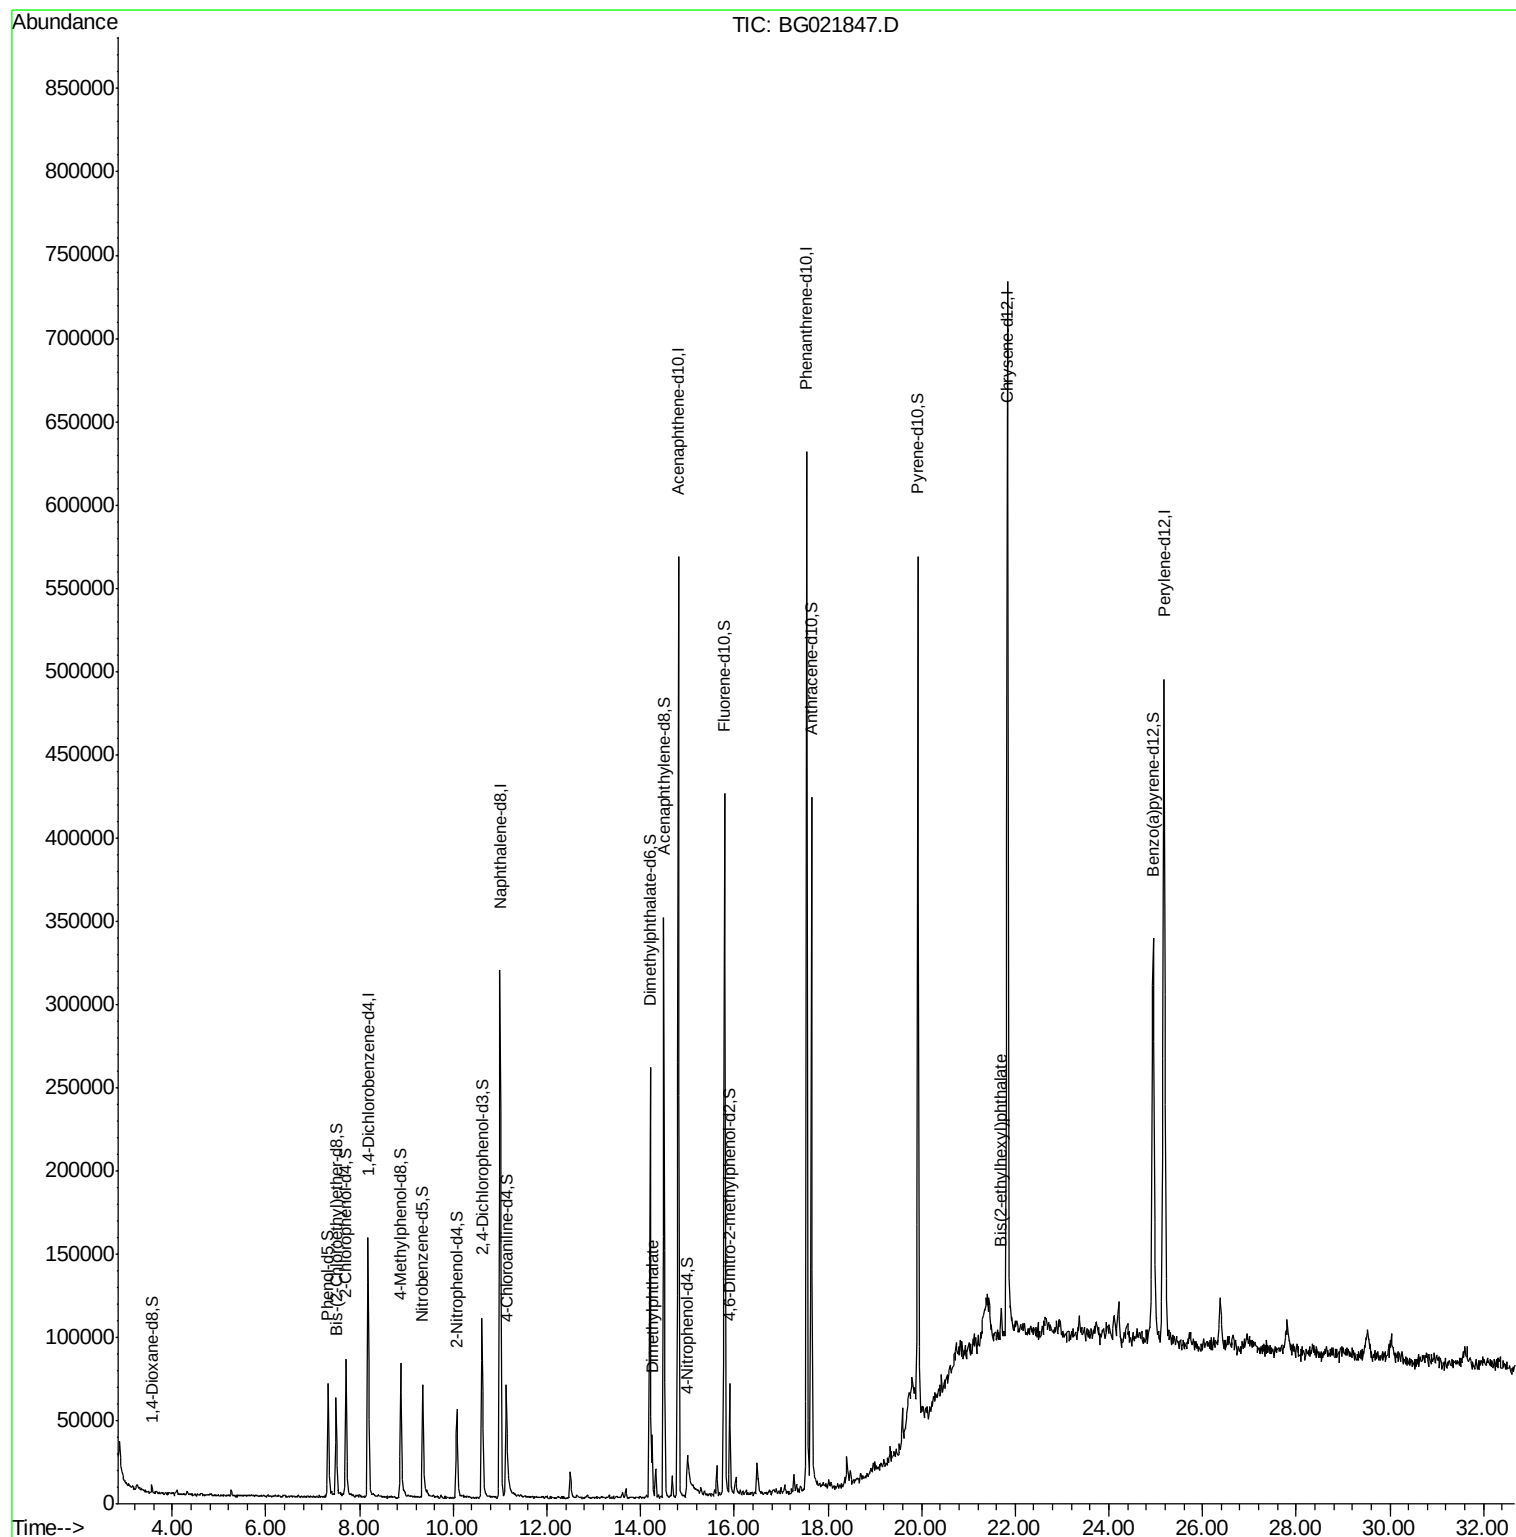

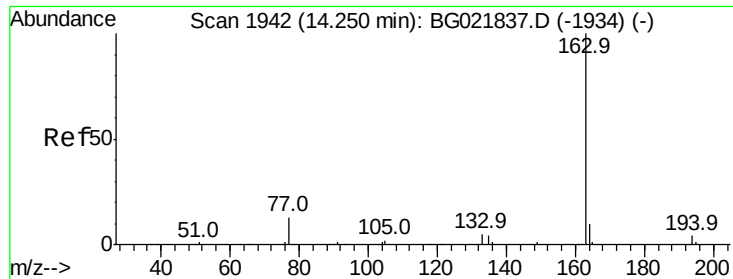





#45
Dimethylphthalate
Concen: 2.01 ng/ul
RT: 14.24 min Scan# 1941
Delta R.T. -0.01 min
Lab File: BG021847.D
Acq: 11 May 2016 16:59

Instrument :
BNA_G
ClientSampleId :
D9X93

Tot Ion	Ratio	Resp	Lower	Upper
163	100	31971		
194	3.6		3.9	5.9#
164	10.7		8.7	13.1

Manual Integrations
APPROVED

sohil
5/12/2016 7:30:54 PM

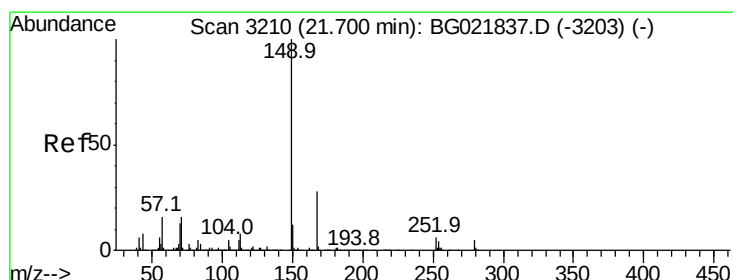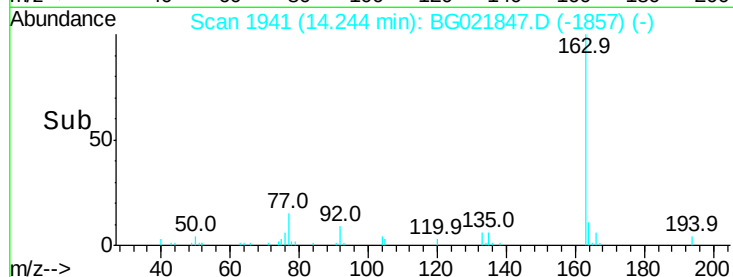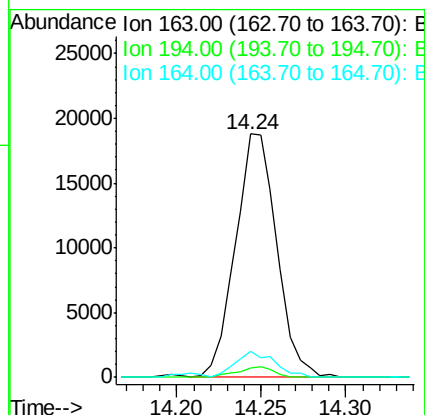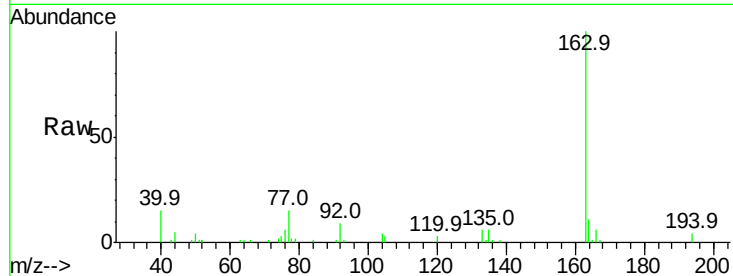

#82
Bis(2-ethylhexyl)phthalate
Concen: 1.19 ng/ul
RT: 21.70 min Scan# 3210
Delta R.T. -0.00 min
Lab File: BG021847.D
Acq: 11 May 2016 16:59

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	11054		
167	27.1		20.5	30.7
279	6.3		3.7	5.5#

