


Data Path : Z:\HPCHEM1\BNA G\DATA\BG051117\
 Data File : BG026946.D
 Acq On : 11 May 2017 16:25
 Operator : SJ/MA
 Sample : DFTPP61
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION
 Last Update : Fri May 12 04:35:42 2017

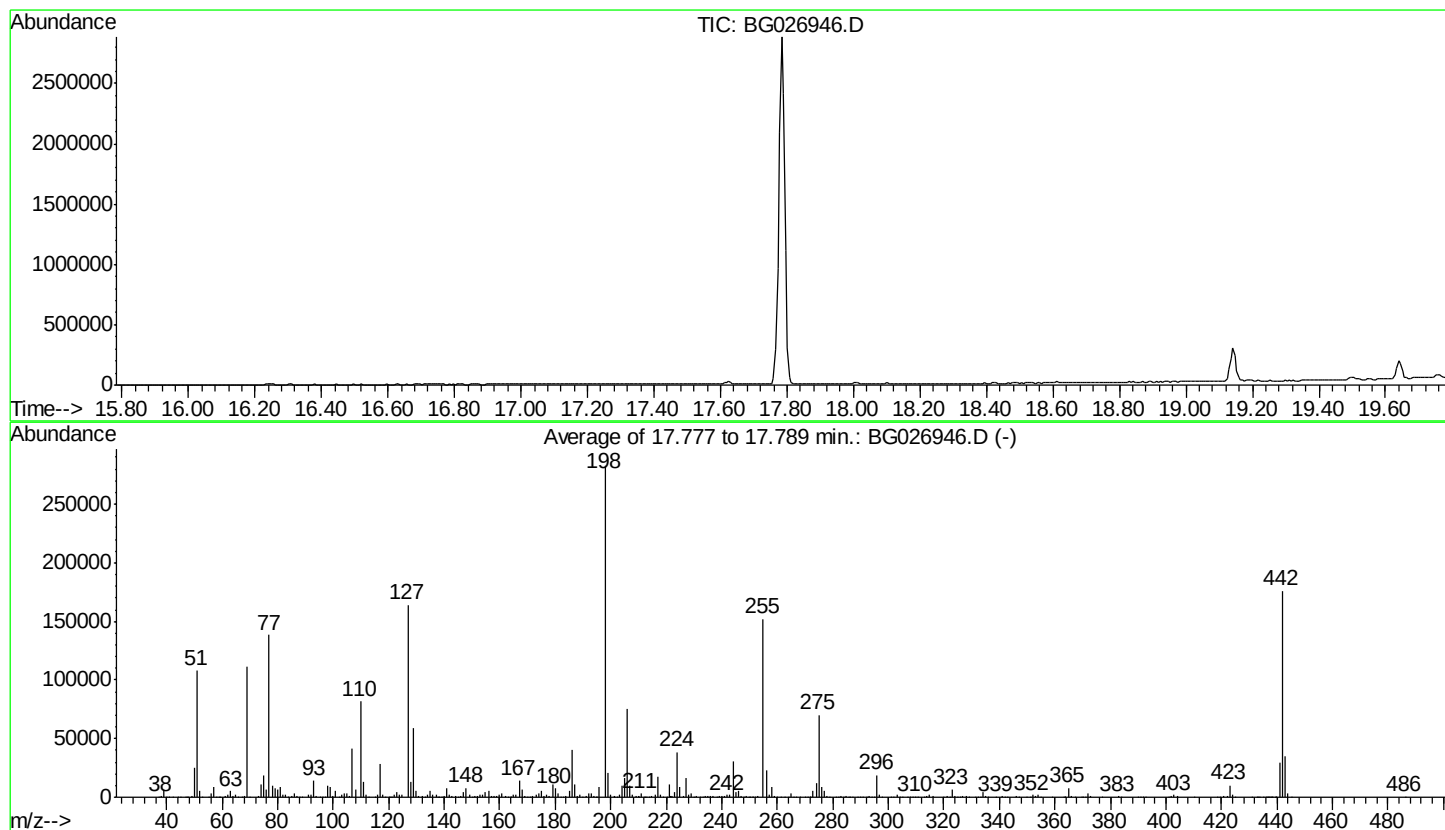

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	107628	PASS
68	69	0.00	2	0.6	620	PASS
69	198	0.00	100	39.4	111470	PASS
70	69	0.00	2	0.5	515	PASS
127	198	10	80	58.1	164352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	282922	PASS
199	198	5	9	7.3	20658	PASS
275	198	10	60	24.7	70021	PASS
365	198	1	100	2.8	8036	PASS
441	442	0.01	100	16.6	29266	PASS
442	198	50	100	62.3	176325	PASS
443	442	15	24	19.8	34949	PASS