


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051120\
 Data File : BG045309.D
 Acq On : 12 May 2020 00:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 12 15:48:20 2020

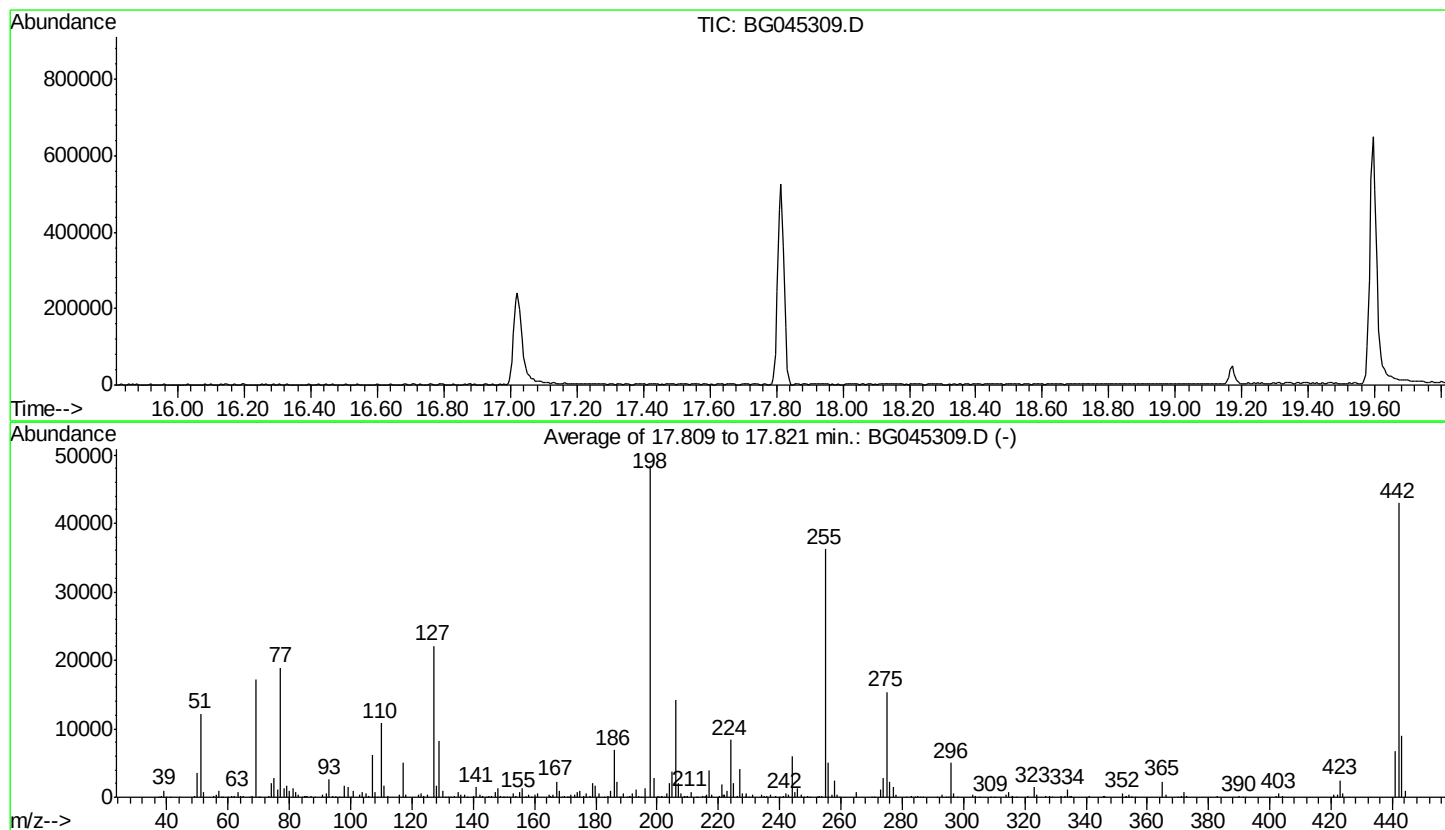

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	12187	PASS
68	69	0.00	2	1.6	273	PASS
69	198	0.00	100	35.6	17220	PASS
70	69	0.00	2	0.6	96	PASS
127	198	10	80	45.7	22128	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48432	PASS
199	198	5	9	5.9	2843	PASS
275	198	10	60	31.7	15340	PASS
365	198	1	100	4.7	2275	PASS
441	198	0.01	100	13.9	6746	PASS
442	198	50	100	88.7	42936	PASS
443	442	15	24	21.1	9051	PASS