

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057397.D
 Acq On : 11 May 2023 13:19
 Operator : CG/JU
 Sample : 02591-10DL 30X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JREB7DL

Quant Time: May 11 23:34:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 10 11:18:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.366	152	15276	20.000	ng/ul	0.00
20) Naphthalene-d8	11.203	136	63588	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.981	164	53190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.718	188	128338	20.000	ng/ul	0.00
79) Chrysene-d12	22.030	240	117775	20.000	ng/ul	0.00
88) Perylene-d12	25.537	264	125071	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	4.107	84	57	0.052	ng/ul	0.02
7) Phenol-d5	7.520	99	457	0.316	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.667	67	156	0.184	ng/ul	0.00
11) 2-Chlorophenol-d4	7.890	132	226	0.237	ng/ul	0.00
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.845	165	202	0.177	ng/ul	0.03
31) 4-Chloroaniline-d4	11.350	131	151	0.100	ng/ul	0.02
46) Dimethylphthalate-d6	14.364	166	2081	0.494	ng/ul	0.00
49) Acenaphthylene-d8	14.681	160	2146	0.453	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.968	176	1827	0.465	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.818	188	3484	0.595	ng/ul	0.00
81) Pyrene-d10	20.086	212	3641	0.521	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.302	264	3393	0.532	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.854	149	165041	42.150	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057397.D
Acq On : 11 May 2023 13:19
Operator : CG/JU
Sample : 02591-10DL 30X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JREB7DL

Quant Time: May 11 23:34:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 10 11:18:43 2023
Response via : Initial Calibration

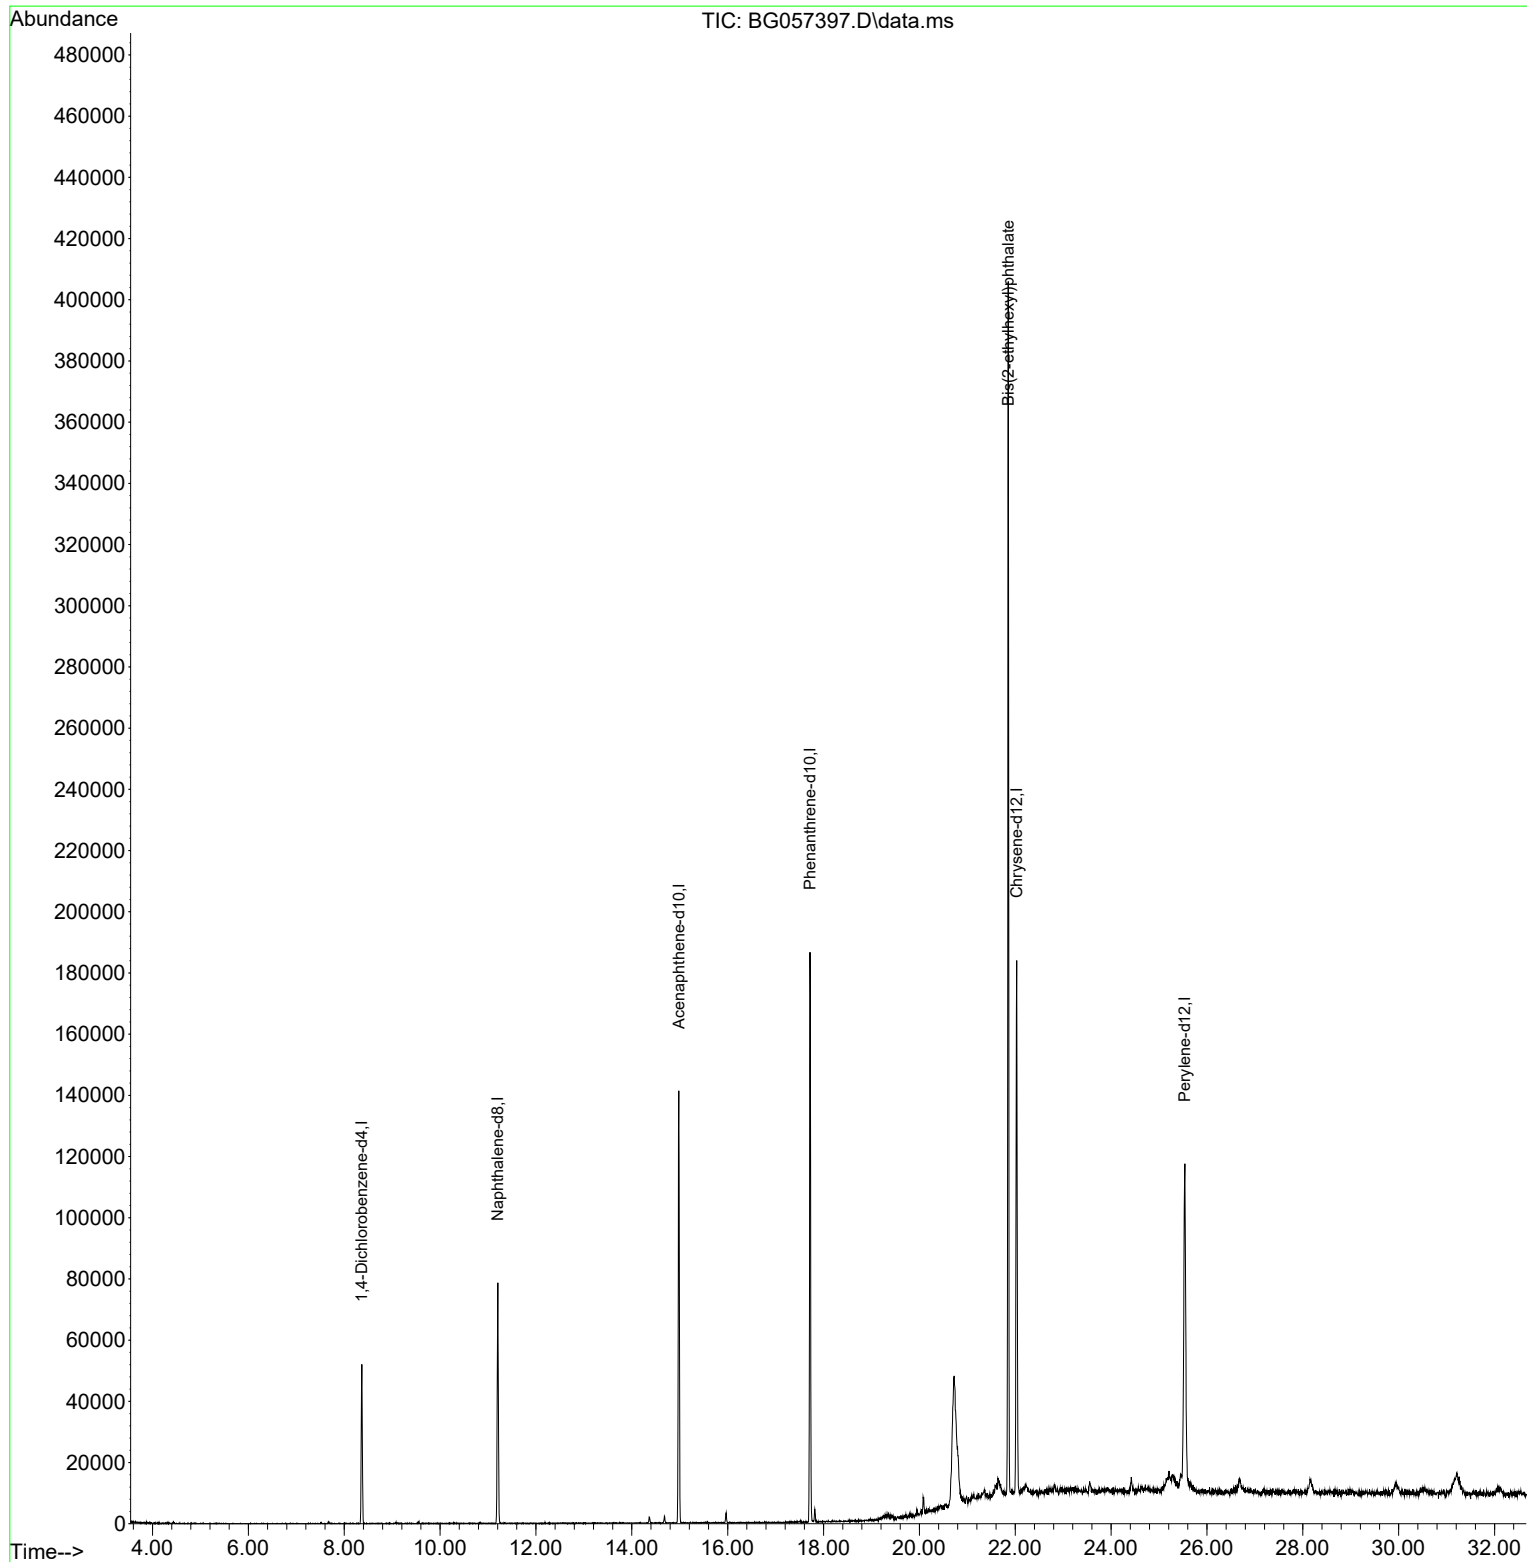

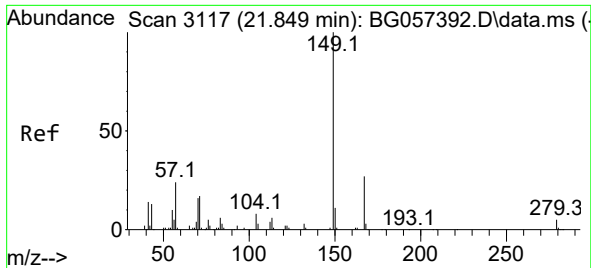

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 42.150 ng/ul
 RT: 21.854 min Scan# 3118
 Delta R.T. 0.005 min
 Lab File: BG057397.D
 Acq: 11 May 2023 13:19

Instrument :
 BNA_G
 ClientSampleId :
 JREB7DL

Tgt Ion:149 Resp: 165041
 Ion Ratio Lower Upper
 149 100
 167 27.7 23.0 34.6
 279 4.5 3.6 5.4

