

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057397.D
 Acq On : 11 May 2023 13:19
 Operator : CG/JU
 Sample : 02591-10DL 30X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JREB7DL

Quant Time: May 11 23:52:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 10 11:18:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.366	152	15276	20.000	ng/u1	0.00
20) Naphthalene-d8	11.203	136	63588	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.981	164	53190	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.718	188	128338	20.000	ng/u1	0.00
79) Chrysene-d12	22.030	240	117775	20.000	ng/u1	0.00
88) Perylene-d12	25.537	264	125071	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	0.000	99	0d	0.000	ng/u1	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/u1	
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/u1	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/u1	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/u1	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/u1	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/u1	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/u1	
46) Dimethylphthalate-d6	14.364	166	2081	0.494	ng/u1	0.00
49) Acenaphthylene-d8	14.681	160	2146	0.453	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/u1	
60) Fluorene-d10	15.968	176	1827	0.465	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/u1	
73) Anthracene-d10	17.818	188	3484	0.595	ng/u1	0.00
81) Pyrene-d10	20.086	212	3641	0.521	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.302	264	3393	0.532	ng/u1	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.854	149	165041	42.150	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057397.D
Acq On : 11 May 2023 13:19
Operator : CG/JU
Sample : 02591-10DL 30X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JREB7DL


Quant Time: May 11 23:52:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 10 11:18:43 2023
Response via : Initial Calibration

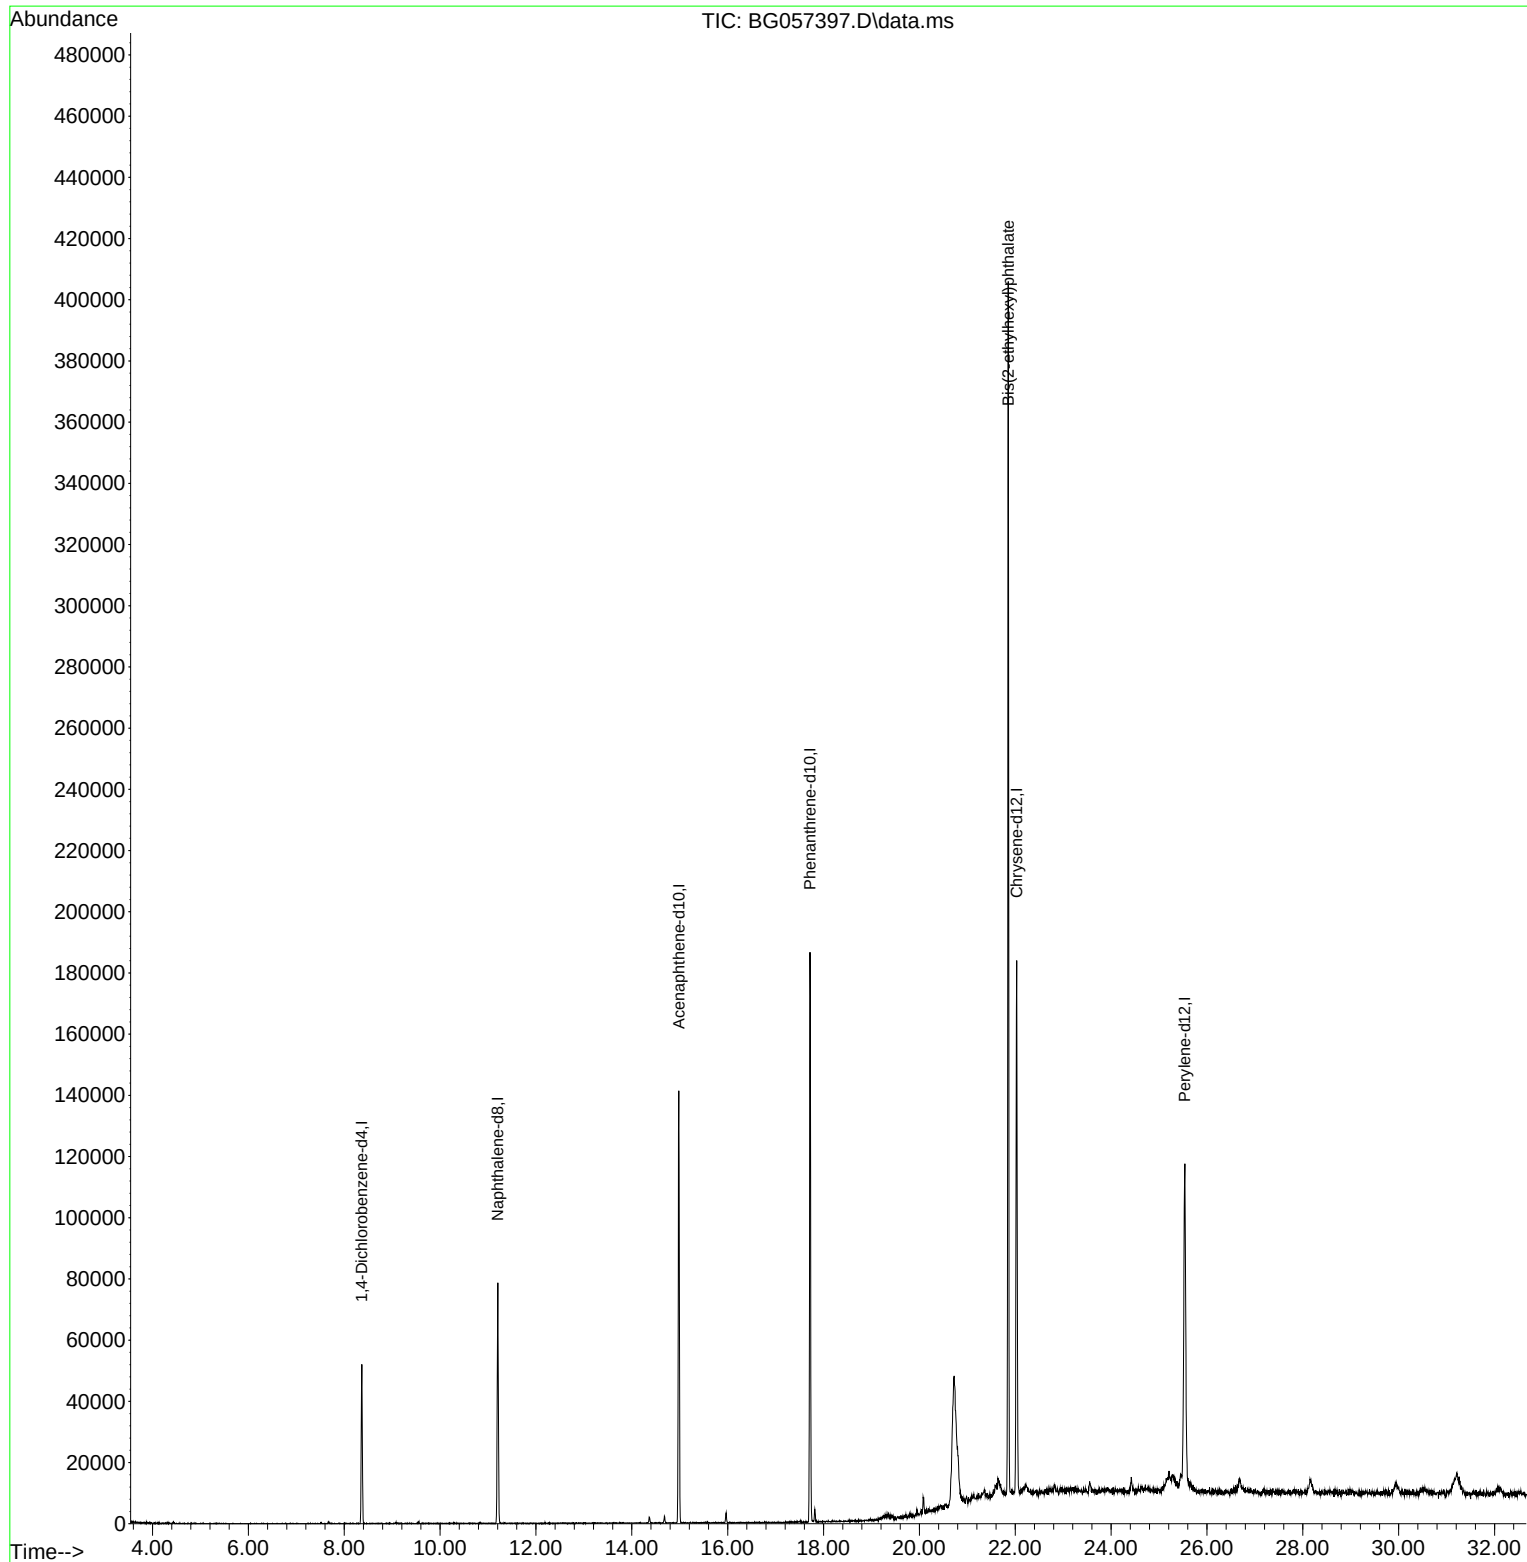

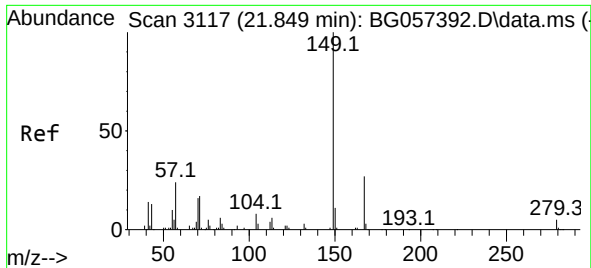

#86
Bis(2-ethylhexyl)phthalate
Concen: 42.150 ng/ul
RT: 21.854 min Scan# 3118
Delta R.T. 0.005 min
Lab File: BG057397.D
Acq: 11 May 2023 13:19

Instrument :
BNA_G
ClientSampleId :
JREB7DL

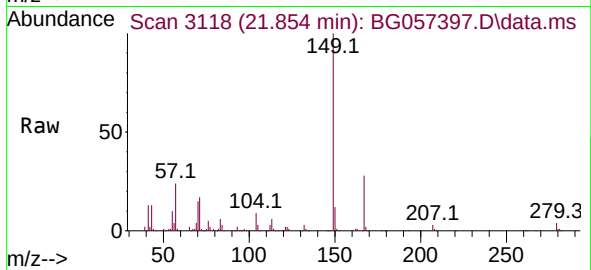

Tgt Ion:	149	Resp:	165041
Ion	Ratio	Lower	Upper
149	100		
167	27.7	23.0	34.6
279	4.5	3.6	5.4

