

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057393.D
 Acq On : 11 May 2023 10:38
 Operator : CG/JU
 Sample : PB152703BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK703

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.644	16	18	21	rVB2	1583	1590	0.21%	0.031%
2	4.090	91	94	104	rBV	15210	25682	3.43%	0.494%
3	7.509	670	676	684	rBV	21322	38146	5.10%	0.733%
4	7.668	697	703	710	rBB	15824	25786	3.45%	0.496%
5	7.897	736	742	748	rBB2	20595	34119	4.56%	0.656%
6	8.367	815	822	829	rBV	44908	73005	9.76%	1.403%
7	9.066	935	941	954	rBV	37683	67045	8.96%	1.289%
8	9.542	1015	1022	1031	rBB2	26654	46007	6.15%	0.884%
9	10.276	1141	1147	1155	rBB2	26045	44844	5.99%	0.862%
10	10.822	1234	1240	1249	rBV	43603	78782	10.53%	1.514%
11	11.204	1297	1305	1316	rBV	64132	115453	15.43%	2.219%
12	11.333	1320	1327	1335	rBV	63887	114896	15.36%	2.208%
13	12.761	1569	1570	1576	rVB	840	1175	0.16%	0.023%
14	14.365	1837	1843	1852	rVB	238142	332233	44.41%	6.386%
15	14.682	1890	1897	1906	rVB	198720	315701	42.20%	6.068%
16	14.981	1941	1948	1956	rVB	122779	188475	25.20%	3.622%
17	15.169	1974	1980	2001	rBV	63891	130537	17.45%	2.509%
18	15.962	2108	2115	2124	rBV	307535	475220	63.53%	9.134%
19	16.086	2130	2136	2153	rBV	69732	124215	16.61%	2.387%
20	16.197	2153	2155	2162	rVB4	1094	1664	0.22%	0.032%
21	17.719	2407	2414	2420	rBV	178418	257709	34.45%	4.953%
22	17.819	2424	2431	2444	rVV	400456	607003	81.14%	11.667%
23	19.569	2727	2729	2732	rVB2	1049	888	0.12%	0.017%
24	19.652	2739	2743	2746	rVV4	4982	6664	0.89%	0.128%
25	19.722	2750	2755	2759	rBV	4376	6547	0.88%	0.126%
26	19.857	2777	2778	2784	rBV3	603	1071	0.14%	0.021%
27	19.963	2793	2796	2798	rBV3	524	772	0.10%	0.015%
28	20.086	2810	2817	2825	rVV	519363	748054	100.00%	14.378%
29	20.697	2919	2921	2923	rBV2	1091	958	0.13%	0.018%
30	20.744	2927	2929	2930	rVB2	1267	874	0.12%	0.017%
31	21.020	2974	2976	2978	rBV2	1103	1054	0.14%	0.020%
32	21.179	3002	3003	3005	rBV2	1263	832	0.11%	0.016%
33	21.261	3015	3017	3018	rBV2	1257	1216	0.16%	0.023%
34	21.337	3028	3030	3034	rVB4	2732	1942	0.26%	0.037%
35	21.478	3052	3054	3055	rBV2	1094	791	0.11%	0.015%
36	21.760	3100	3102	3104	rVB2	1627	897	0.12%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057393.D
 Acq On : 11 May 2023 10:38
 Operator : CG/JU
 Sample : PB152703BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK703

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	22.031	3139	3148	3155	rBV	166327	288622	38.58%	5.547%
38	22.424	3214	3215	3217	rVB	1697	1014	0.14%	0.019%
39	24.169	3511	3512	3514	rBV2	1630	1348	0.18%	0.026%
40	24.216	3519	3520	3522	rBV2	1705	837	0.11%	0.016%
41	24.422	3551	3555	3559	rBV5	2584	5600	0.75%	0.108%
42	24.557	3576	3578	3581	rBV2	1936	1513	0.20%	0.029%
43	24.627	3588	3590	3591	rBV	2156	1314	0.18%	0.025%
44	25.297	3690	3704	3717	rBV2	248000	725526	96.99%	13.945%
45	25.450	3726	3730	3734	rVV5	2854	5485	0.73%	0.105%
46	25.532	3734	3744	3756	rVB2	88879	271837	36.34%	5.225%
47	26.078	3835	3837	3840	rBV4	1685	1735	0.23%	0.033%
48	26.378	3886	3888	3890	rBV3	1440	885	0.12%	0.017%
49	26.577	3920	3922	3924	rBV3	1623	907	0.12%	0.017%
50	26.660	3934	3936	3937	rBV2	1744	1043	0.14%	0.020%
51	27.141	4016	4018	4020	rBV3	1533	1498	0.20%	0.029%
52	27.735	4117	4119	4120	rBV2	1784	891	0.12%	0.017%
53	27.940	4150	4154	4157	rBV3	1488	2468	0.33%	0.047%
54	27.970	4157	4159	4160	rBV	1269	774	0.10%	0.015%
55	28.857	4308	4310	4311	rBV2	1798	1441	0.19%	0.028%
56	29.421	4405	4406	4408	rBV2	1301	839	0.11%	0.016%
57	30.173	4532	4534	4535	rVB2	1897	857	0.11%	0.016%
58	30.220	4540	4542	4543	rVB2	2128	1296	0.17%	0.025%
59	30.237	4543	4545	4547	rBV3	1677	1888	0.25%	0.036%
60	30.813	4641	4643	4644	rBV	1563	1347	0.18%	0.026%
61	31.148	4698	4700	4701	rBV	1434	870	0.12%	0.017%
62	31.189	4705	4707	4709	rBV2	1170	1142	0.15%	0.022%
63	31.277	4720	4722	4725	rBV3	1161	1093	0.15%	0.021%
64	31.741	4799	4801	4802	rBV2	1282	912	0.12%	0.018%
65	31.929	4831	4833	4834	rBV2	1374	1106	0.15%	0.021%
66	32.005	4844	4846	4847	rBV	1471	916	0.12%	0.018%
67	32.070	4855	4857	4859	rBV3	1422	1543	0.21%	0.030%
68	32.358	4904	4906	4908	rVB3	1693	1086	0.15%	0.021%
69	32.546	4936	4938	4939	rBV	1453	1432	0.19%	0.028%




Sum of corrected areas: 5202912

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057393.D
Acq On : 11 May 2023 10:38
Operator : CG/JU
Sample : PB152703BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK703

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

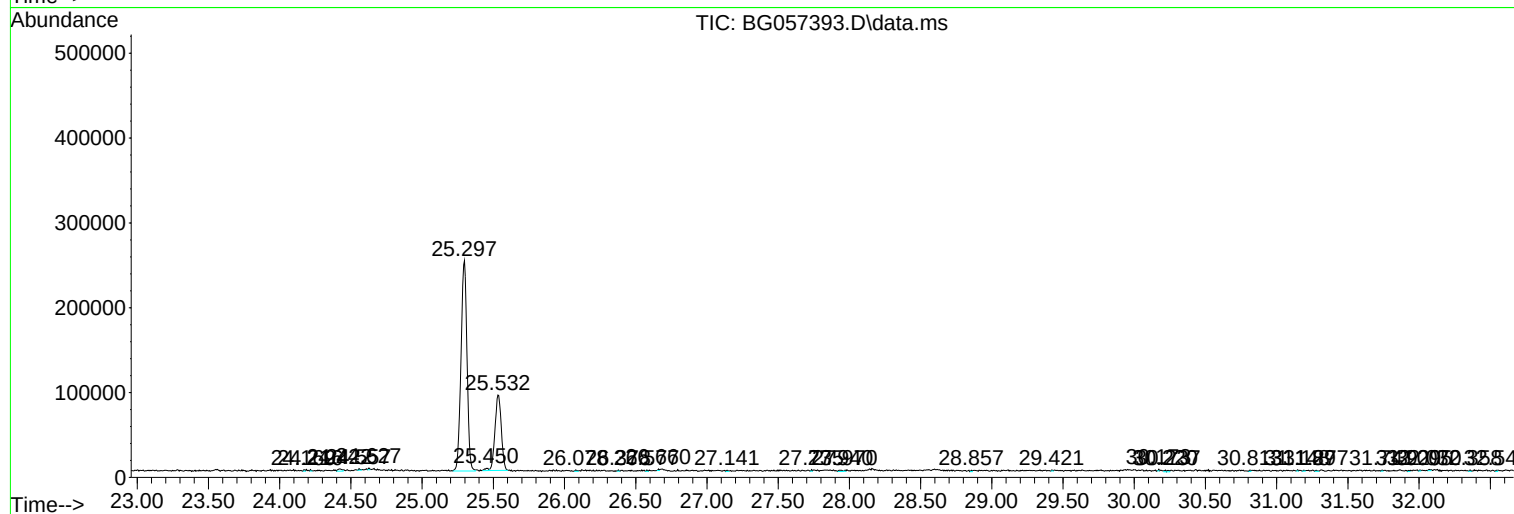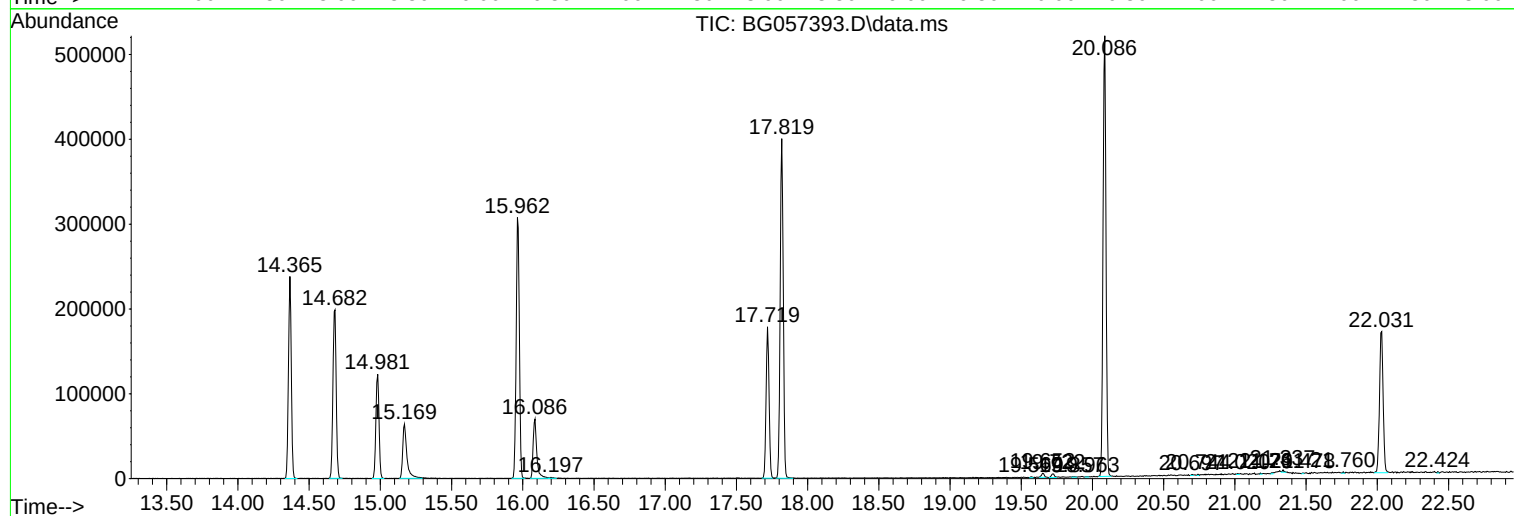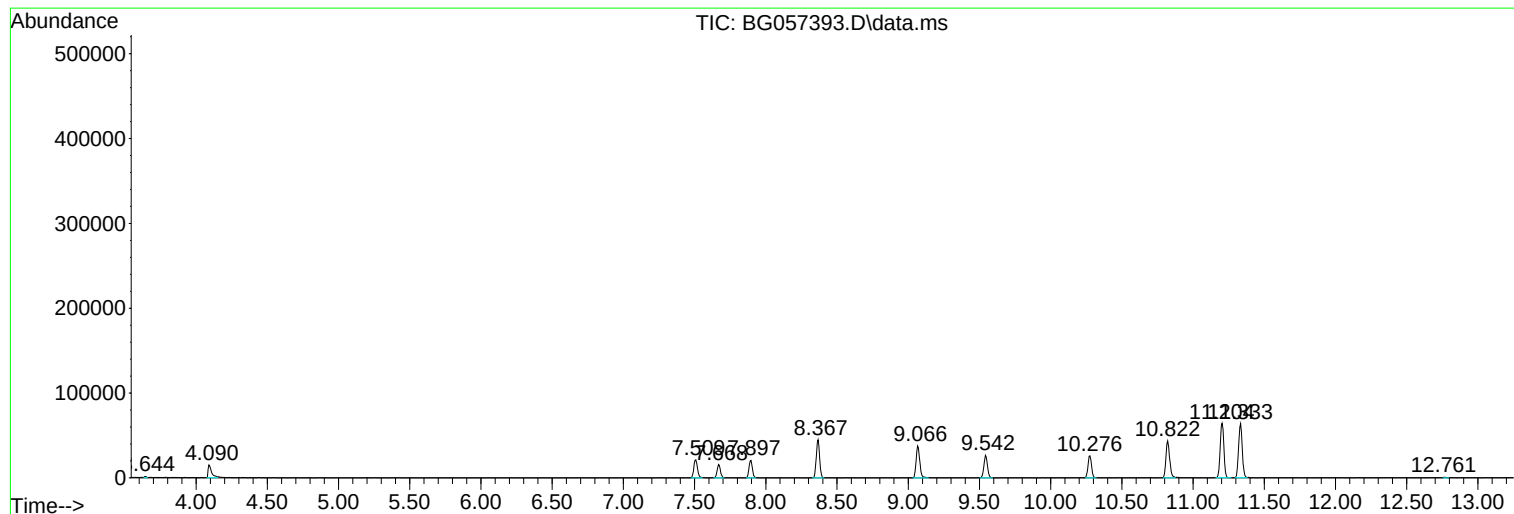

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057393.D
Acq On : 11 May 2023 10:38
Operator : CG/JU
Sample : PB152703BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK703

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057393.D
Acq On : 11 May 2023 10:38
Operator : CG/JU
Sample : PB152703BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK703

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc