

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057400.D
 Acq On : 11 May 2023 16:03
 Operator : CG/JU
 Sample : PB152685BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG057400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.650	15	19	22	rVB	1201	1460	0.20%	0.027%
2	4.090	92	94	105	rVV	16597	27491	3.68%	0.512%
3	4.437	150	153	155	rBV	917	760	0.10%	0.014%
4	7.509	670	676	684	rBV	23886	41457	5.54%	0.772%
5	7.668	697	703	710	rBV	17236	27558	3.69%	0.513%
6	7.891	734	741	748	rBB	21385	36740	4.91%	0.684%
7	8.367	816	822	830	rBB	48496	78118	10.45%	1.455%
8	9.066	935	941	952	rBB2	39638	71234	9.53%	1.326%
9	9.542	1012	1022	1030	rBB	28872	49714	6.65%	0.926%
10	10.270	1140	1146	1153	rVB	27232	46702	6.25%	0.870%
11	10.822	1234	1240	1248	rBV	46235	85221	11.40%	1.587%
12	11.204	1298	1305	1312	rVB	65567	119148	15.94%	2.219%
13	11.327	1320	1326	1337	rVB	67474	124339	16.63%	2.315%
14	14.365	1836	1843	1849	rBV	238483	344015	46.01%	6.406%
15	14.676	1889	1896	1903	rBV	207325	332006	44.41%	6.182%
16	14.975	1941	1947	1954	rVB	124289	195513	26.15%	3.641%
17	15.169	1974	1980	1994	rBV	67816	133428	17.85%	2.485%
18	15.287	1999	2000	2004	rVB3	993	1148	0.15%	0.021%
19	15.962	2108	2115	2130	rVB	339643	495099	66.22%	9.219%
20	16.080	2130	2135	2149	rBV	83212	135522	18.13%	2.524%
21	16.168	2149	2150	2153	rVV2	1198	1032	0.14%	0.019%
22	16.197	2153	2155	2160	rVB3	870	1026	0.14%	0.019%
23	17.719	2407	2414	2421	rBV	177745	260384	34.83%	4.849%
24	17.819	2424	2431	2438	rVV2	396992	610034	81.59%	11.360%
25	17.872	2438	2440	2444	rVB2	790	790	0.11%	0.015%
26	19.651	2738	2743	2747	rVB4	5006	7335	0.98%	0.137%
27	19.716	2749	2754	2764	rBV3	4872	7949	1.06%	0.148%
28	19.804	2767	2769	2771	rBV	964	938	0.13%	0.017%
29	20.016	2800	2805	2806	rVB4	748	813	0.11%	0.015%
30	20.080	2810	2816	2824	rBV	524373	747677	100.00%	13.923%
31	20.415	2871	2873	2876	rBV2	829	983	0.13%	0.018%
32	20.474	2882	2883	2887	rBV2	712	812	0.11%	0.015%
33	20.544	2892	2895	2896	rBV2	1361	952	0.13%	0.018%
34	20.562	2896	2898	2902	rBV2	1220	1442	0.19%	0.027%
35	20.738	2926	2928	2930	rBV2	722	798	0.11%	0.015%
36	20.956	2963	2965	2966	rVB2	1262	779	0.10%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
 Data File : BG057400.D
 Acq On : 11 May 2023 16:03
 Operator : CG/JU
 Sample : PB152685BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Title : SVOA CALIBRATION

37	20.973	2966	2968	2969	rBV2	1246	778	0.10%	0.014%
38	21.179	3000	3003	3004	rBV2	1301	1705	0.23%	0.032%
39	21.702	3091	3092	3094	rBV2	1517	1059	0.14%	0.020%
40	21.819	3110	3112	3114	rBV3	1439	1110	0.15%	0.021%
41	22.025	3141	3147	3155	rBV	172034	284169	38.01%	5.292%
42	22.330	3197	3199	3203	rBV4	1614	1425	0.19%	0.027%
43	22.401	3209	3211	3213	rBV2	1670	1052	0.14%	0.020%
44	22.430	3215	3216	3221	rBV4	1882	2217	0.30%	0.041%
45	22.642	3250	3252	3253	rBV2	1404	1253	0.17%	0.023%
46	22.894	3293	3295	3297	rBV3	1352	1192	0.16%	0.022%
47	23.094	3327	3329	3332	rBV4	1409	1030	0.14%	0.019%
48	23.258	3356	3357	3360	rVB3	1592	1034	0.14%	0.019%
49	23.552	3402	3407	3413	rBV8	5858	9872	1.32%	0.184%
50	24.098	3498	3500	3501	rBV2	1297	779	0.10%	0.015%
51	24.263	3526	3528	3529	rVB2	1702	921	0.12%	0.017%
52	24.333	3538	3540	3541	rVB	1400	840	0.11%	0.016%
53	24.416	3549	3554	3560	rBV7	5930	12530	1.68%	0.233%
54	24.686	3598	3600	3601	rBV2	1641	1253	0.17%	0.023%
55	24.909	3636	3638	3641	rBV3	1571	1785	0.24%	0.033%
56	25.291	3692	3703	3719	rVB2	243170	715768	95.73%	13.329%
57	25.449	3723	3730	3733	rVV8	7358	15741	2.11%	0.293%
58	25.526	3734	3743	3755	rVB2	93133	269162	36.00%	5.012%
59	25.978	3818	3820	3822	rBV2	1379	1349	0.18%	0.025%
60	26.577	3920	3922	3924	rVB3	1611	1079	0.14%	0.020%
61	26.677	3931	3939	3946	rVB9	6398	17148	2.29%	0.319%
62	26.818	3961	3963	3964	rVB	1767	1057	0.14%	0.020%
63	26.836	3964	3966	3973	rBV6	1360	2230	0.30%	0.042%
64	26.965	3986	3988	3989	rBV	1841	1674	0.22%	0.031%
65	27.088	4007	4009	4011	rBV3	1428	1470	0.20%	0.027%
66	27.347	4049	4053	4056	rBV5	1492	3034	0.41%	0.056%
67	28.093	4179	4180	4182	rBV2	1789	1512	0.20%	0.028%
68	28.146	4184	4189	4192	rVV5	3629	7992	1.07%	0.149%
69	28.675	4277	4279	4280	rBV2	1530	918	0.12%	0.017%
70	28.839	4305	4307	4309	rBV2	1392	1109	0.15%	0.021%
71	29.180	4364	4365	4368	rBV3	1318	1164	0.16%	0.022%
72	29.268	4379	4380	4382	rBV2	1461	1256	0.17%	0.023%
73	30.825	4643	4645	4648	rBV4	1481	1758	0.24%	0.033%
74	31.623	4779	4781	4784	rVB4	1919	1565	0.21%	0.029%
75	31.647	4784	4785	4787	rBV2	1709	1137	0.15%	0.021%
76	31.694	4791	4793	4794	rBV2	1780	1019	0.14%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057400.D
Acq On : 11 May 2023 16:03
Operator : CG/JU
Sample : PB152685BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Title : SVOA CALIBRATION

77	31.929	4831	4833	4835	rBV2	1266	833	0.11%	0.016%
78	32.035	4849	4851	4853	rBV3	1749	1511	0.20%	0.028%
79	32.387	4909	4911	4913	rBV2	1273	1324	0.18%	0.025%
80	32.587	4943	4945	4947	rVB2	1664	934	0.12%	0.017%



Sum of corrected areas: 5370165

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057400.D
Acq On : 11 May 2023 16:03
Operator : CG/JU
Sample : PB152685BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

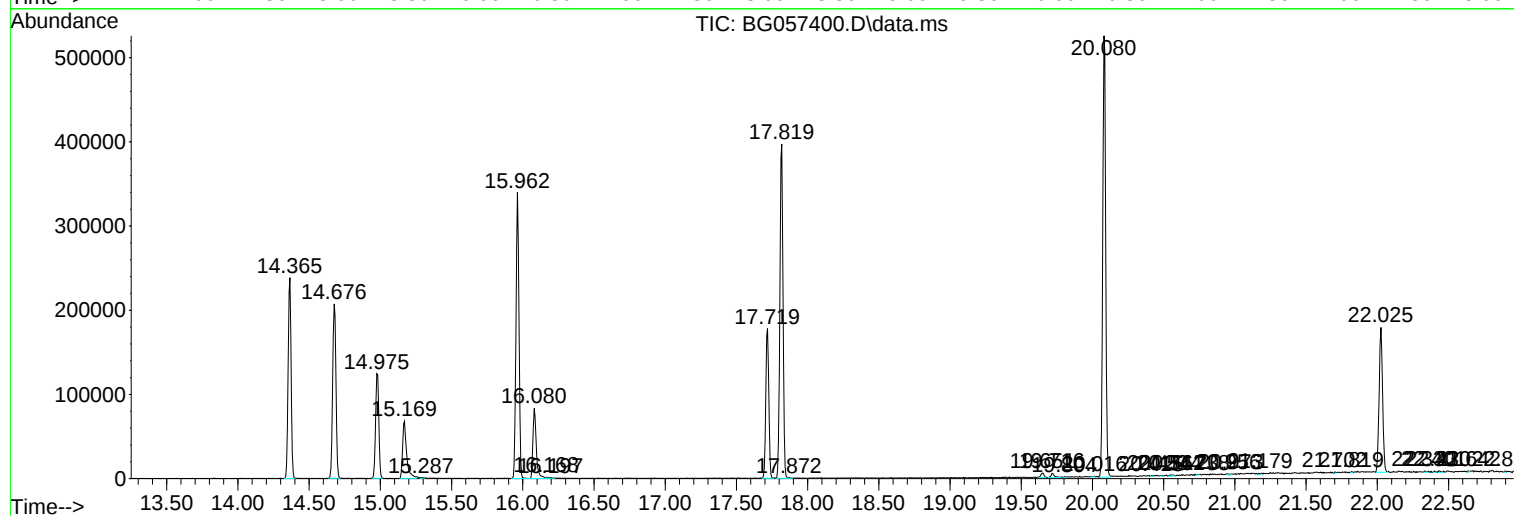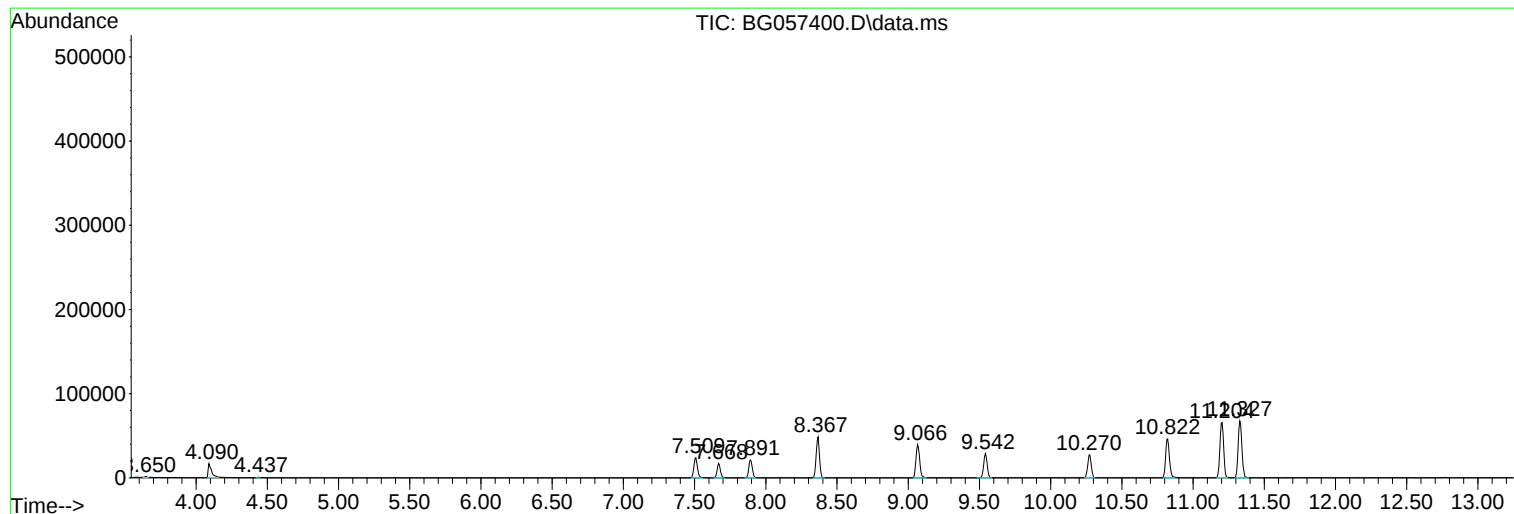

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057400.D
Acq On : 11 May 2023 16:03
Operator : CG/JU
Sample : PB152685BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051123\
Data File : BG057400.D
Acq On : 11 May 2023 16:03
Operator : CG/JU
Sample : PB152685BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------