


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051215\
 Data File : BG017084.D
 Acq On : 12 May 2015 12:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 05 16:13:58 2015

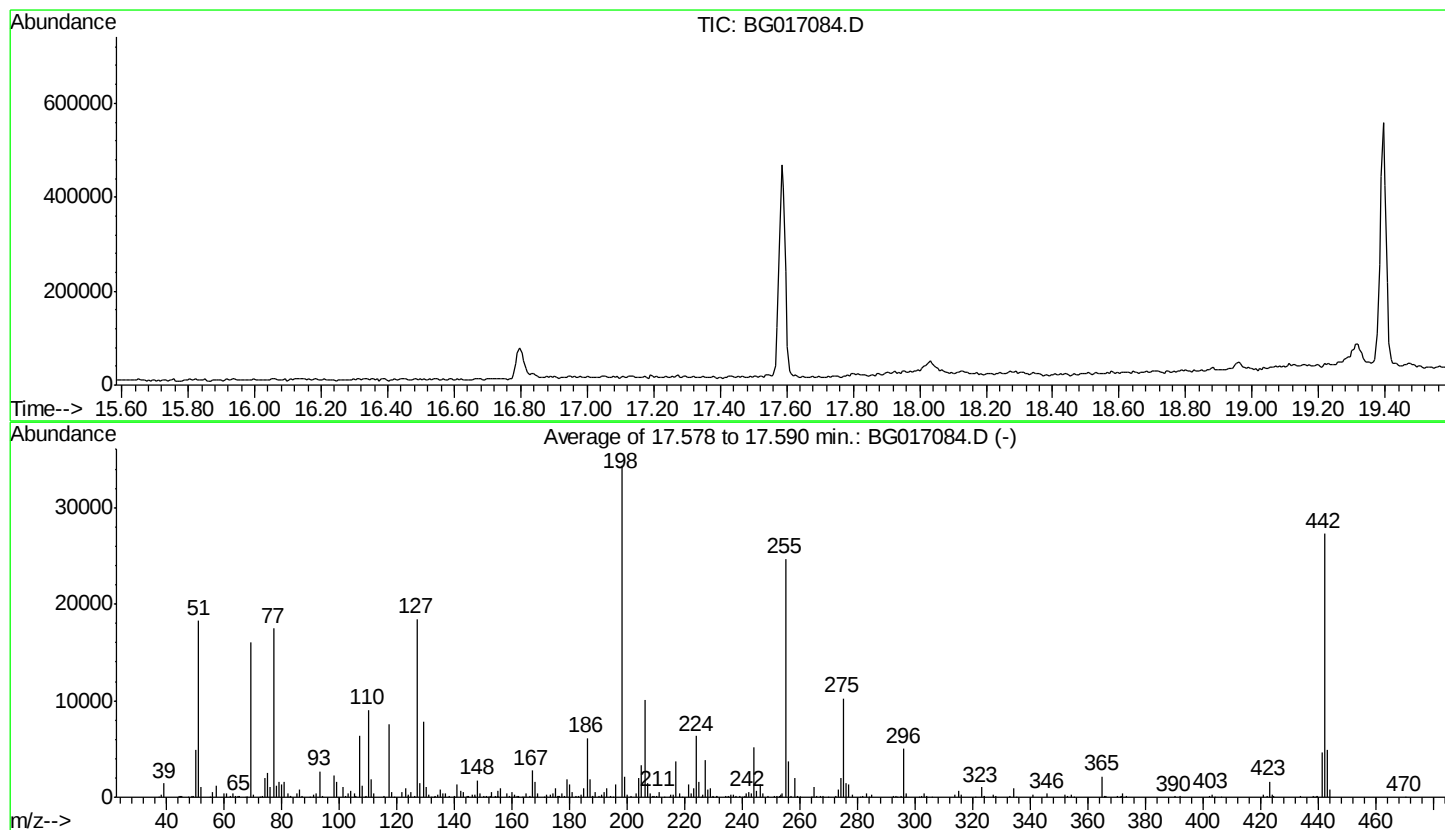

AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	18252	PASS
68	69	0.00	2	0.3	51	PASS
69	198	0.00	100	46.7	16051	PASS
70	69	0.00	2	1.9	304	PASS
127	198	10	80	53.8	18463	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34338	PASS
199	198	5	9	6.2	2139	PASS
275	198	10	60	29.9	10262	PASS
365	198	1	100	6.3	2160	PASS
441	442	0.01	24	17.1	4649	PASS
442	198	50	100	79.4	27258	PASS
443	442	15	24	17.9	4892	PASS