
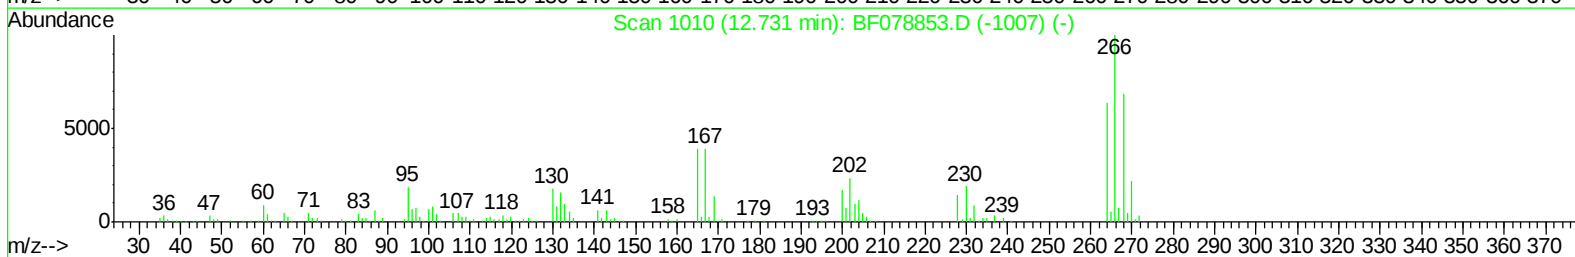
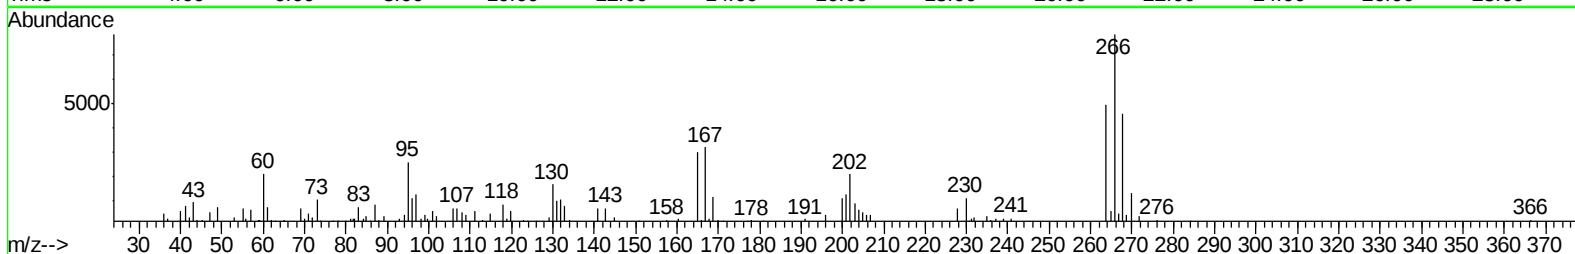


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051215\
Data File : BG017084.D
Acq On : 12 May 2015 12:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:31:44 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

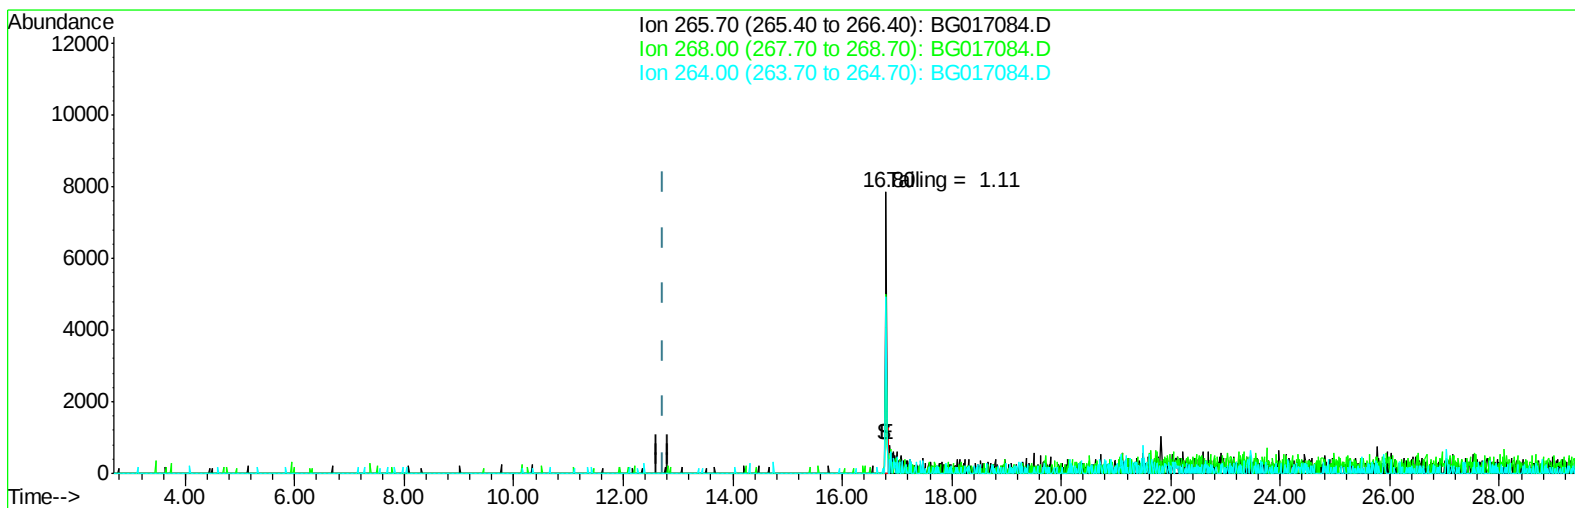

TIC: BG017084.D

(69) Pentachlorophenol (C)




12.760min (+0.030) 0.00ng

response 67

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	0.00#
264.00	60.20	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG051215\
Data File : BG017084.D
Acq On : 12 May 2015 12:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:31:44 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 19:07:47 2015
Response via : Initial Calibration

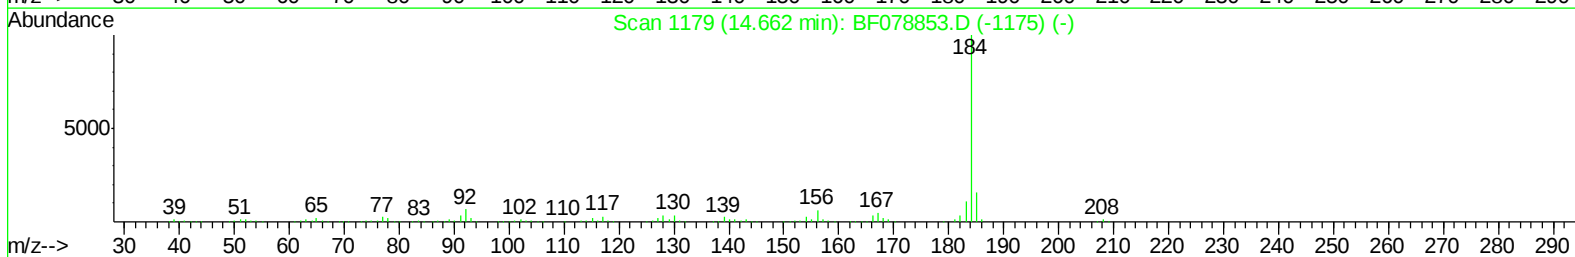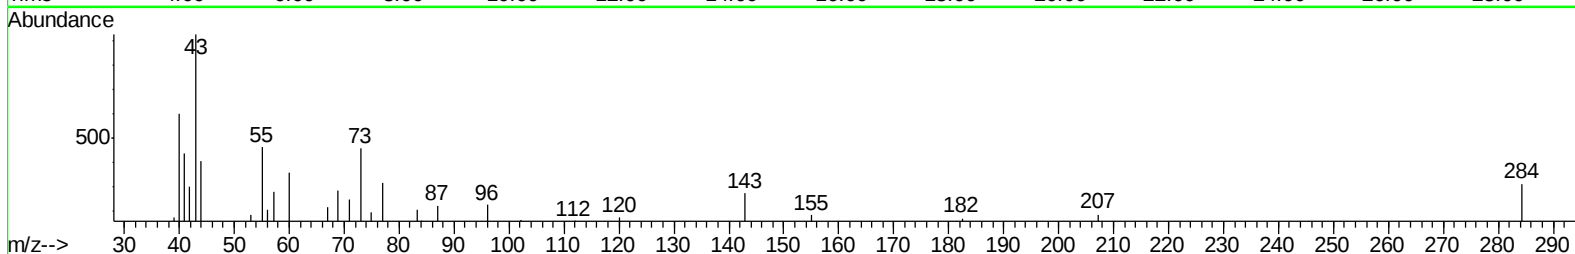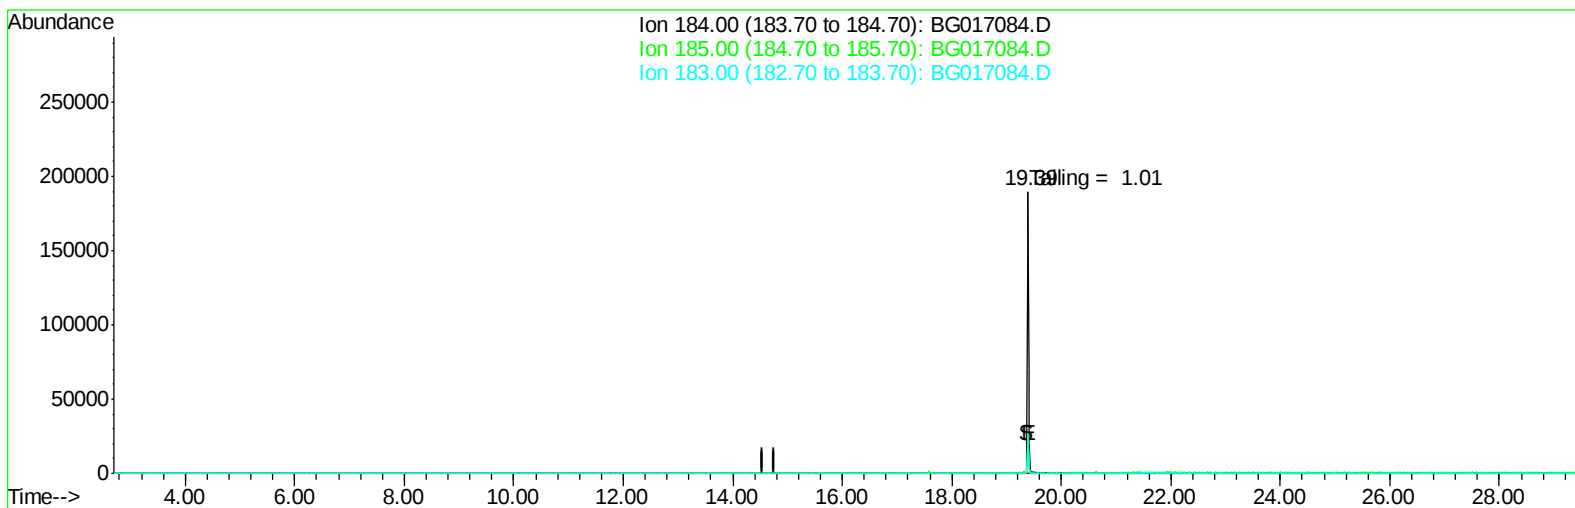

TIC: BG017084.D

(76) Benzidine

14.663min (-14.663) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.40	0.00#
183.00	10.50	0.00#
0.00	0.00	0.00